




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041522\
 Data File : VW022555.D
 Acq On : 15 Apr 2022 13:41
 Operator : SY/VA
 Sample : N2373-11
 Misc : 5.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFF0

Manual IntegrationsAPPROVED

Quant Time: Apr 15 23:18:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 15 23:17:23 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/17/2022
 Supervised By :Mahesh Dadoda 04/20/2022

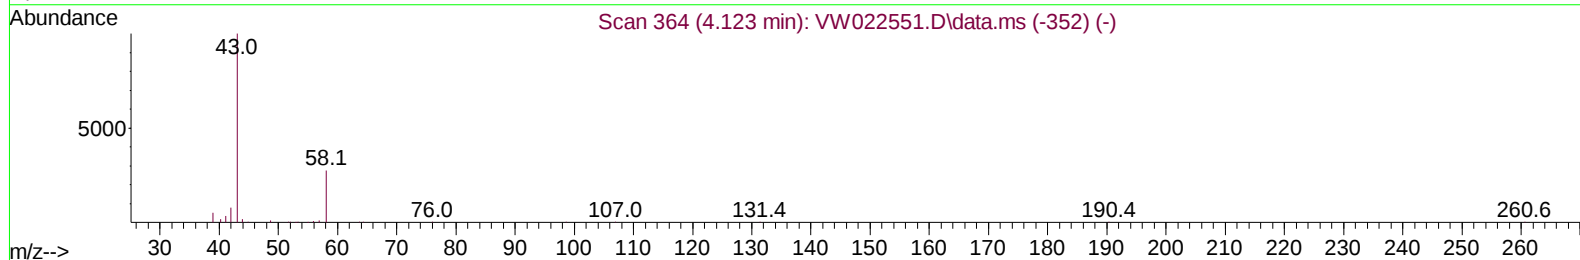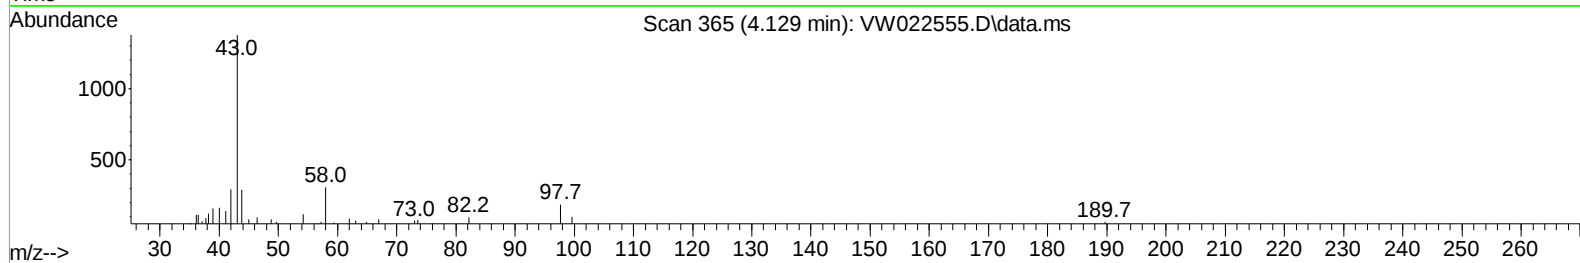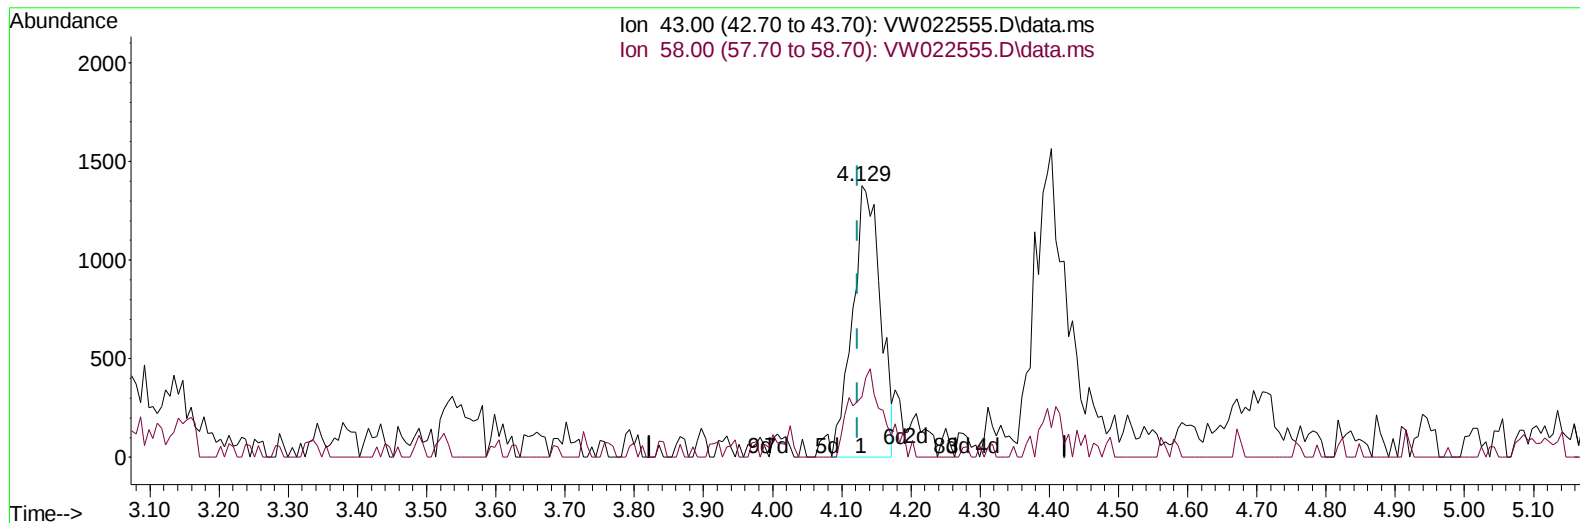

TIC: VW022555.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 4.98 ug/L

response 3836

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	21.38
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041522\
 Data File : VW022555.D
 Acq On : 15 Apr 2022 13:41
 Operator : SY/VA
 Sample : N2373-11
 Misc : 5.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFF0

Manual IntegrationsAPPROVED

Quant Time: Apr 15 23:18:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 15 23:17:23 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/17/2022
 Supervised By :Mahesh Dadoda 04/20/2022

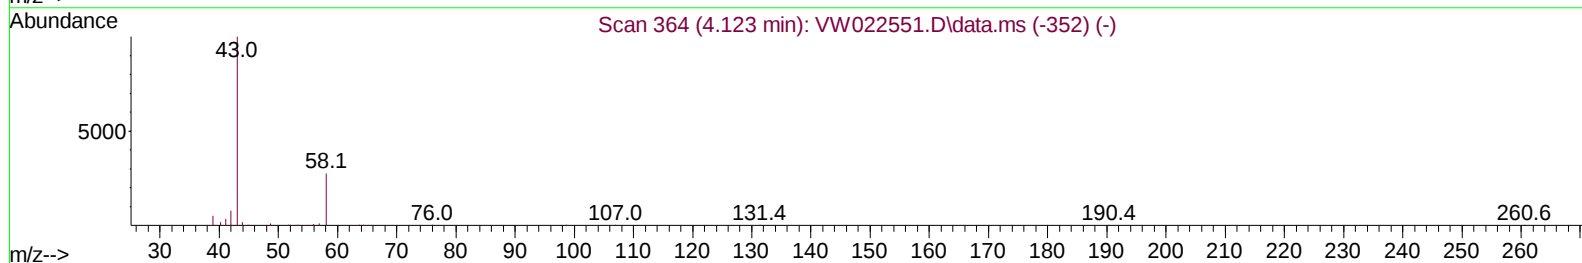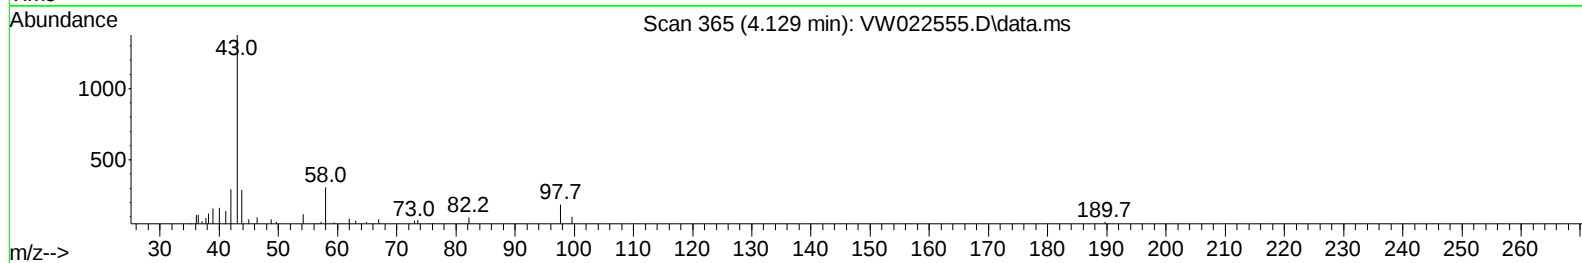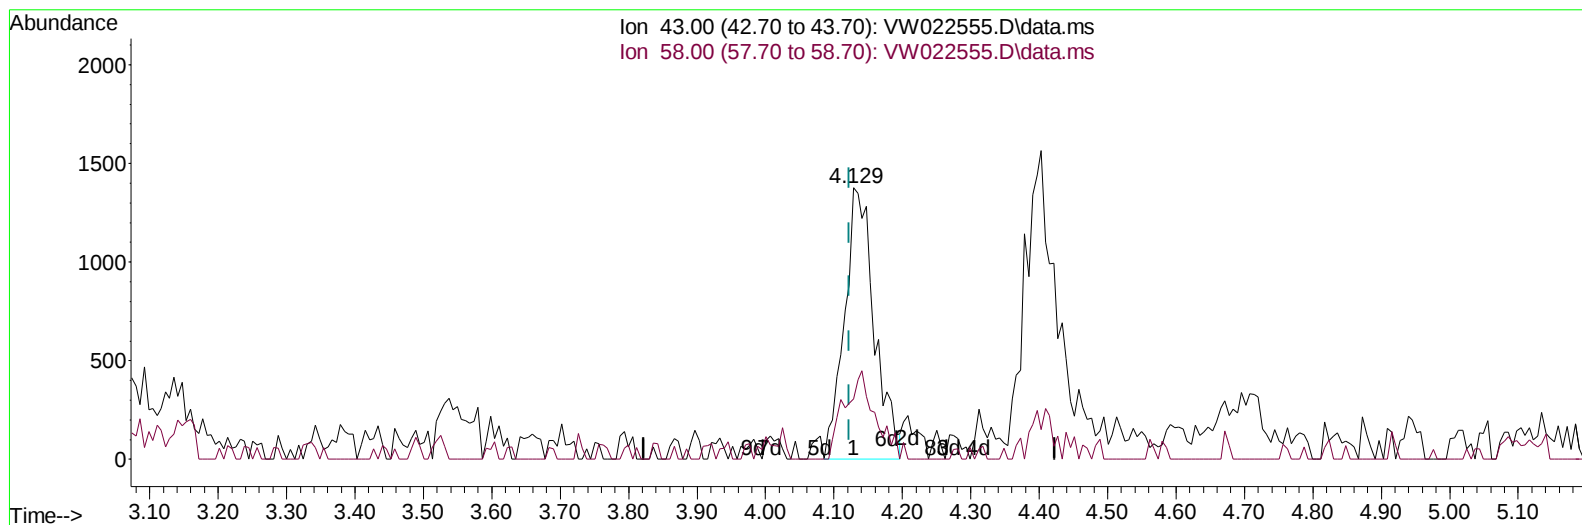

TIC: VW022555.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 5.40 ug/L m

response 4159

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	19.72
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041522\
Data File : VW022555.D
Acq On : 15 Apr 2022 13:41
Operator : SY/VA
Sample : N2373-11
Misc : 5.55g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFFF0

Manual IntegrationsAPPROVED

Quant Time: Apr 15 23:18:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 15 23:17:23 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/17/2022
Supervised By :Mahesh Dadoda 04/20/2022

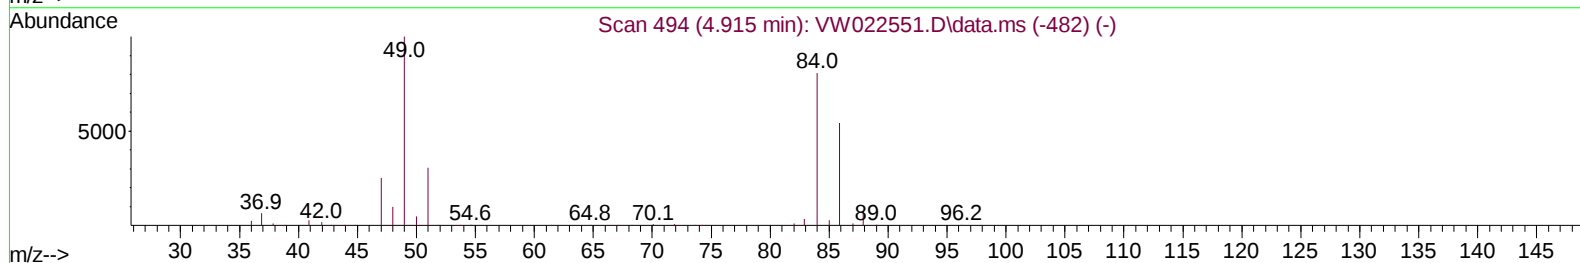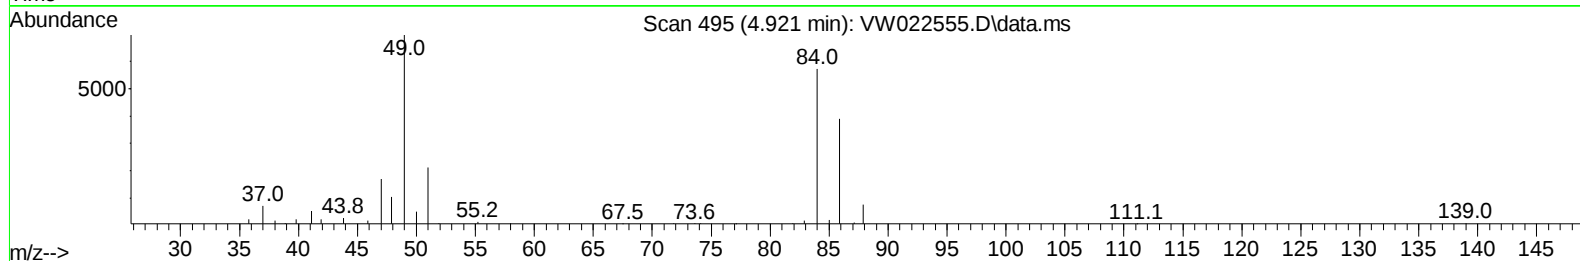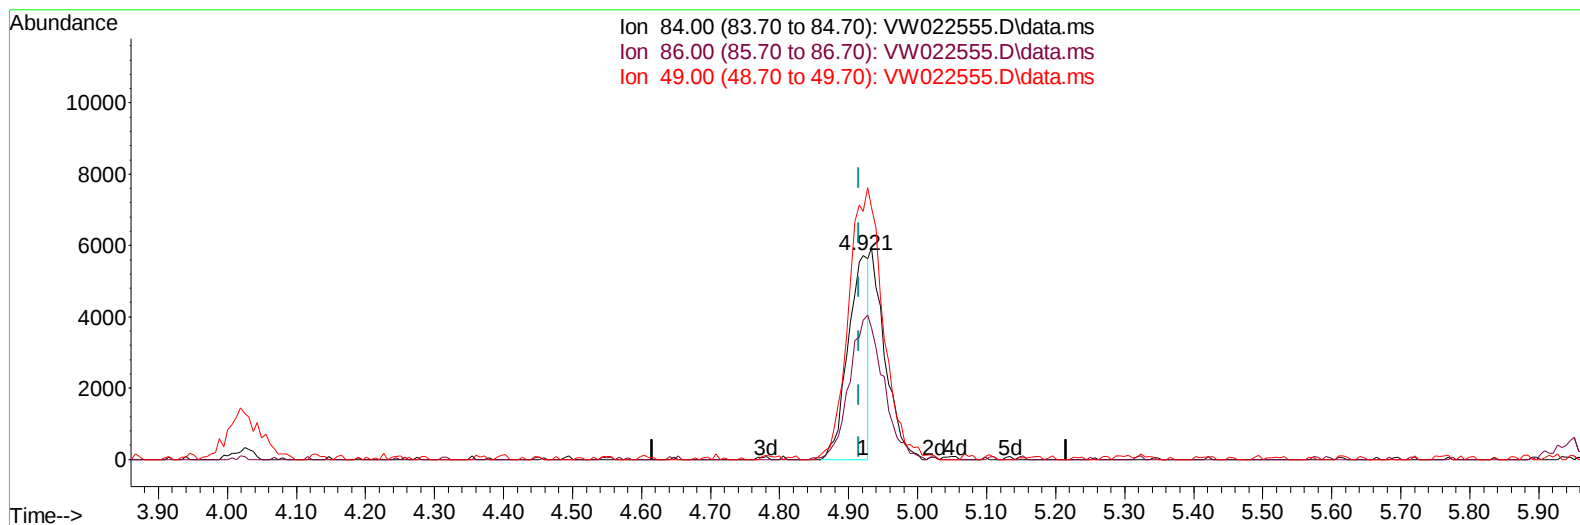

TIC: VW022555.D\data.ms

(16) Methylene chloride (T)

4.921min (+ 0.006) 2.66 ug/L

response 11748

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.10	68.05
49.00	134.60	121.60
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041522\
 Data File : VW022555.D
 Acq On : 15 Apr 2022 13:41
 Operator : SY/VA
 Sample : N2373-11
 Misc : 5.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFF0

Manual IntegrationsAPPROVED

Quant Time: Apr 15 23:18:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 15 23:17:23 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/17/2022
 Supervised By :Mahesh Dadoda 04/20/2022

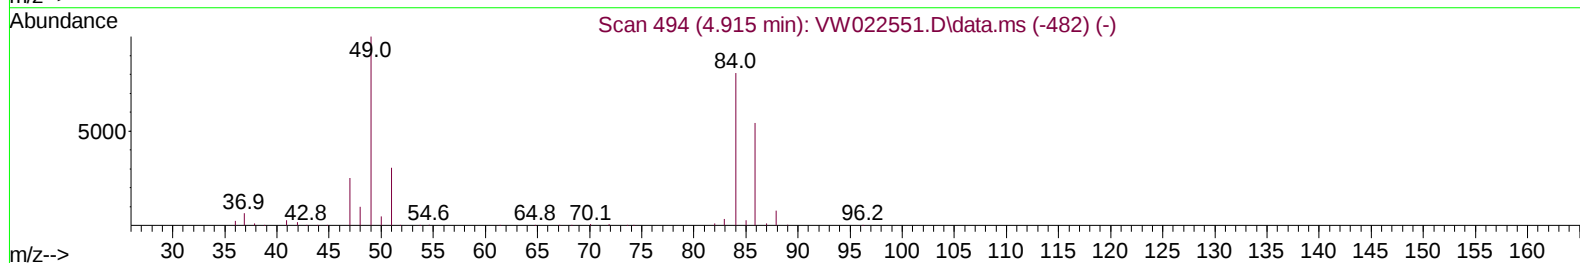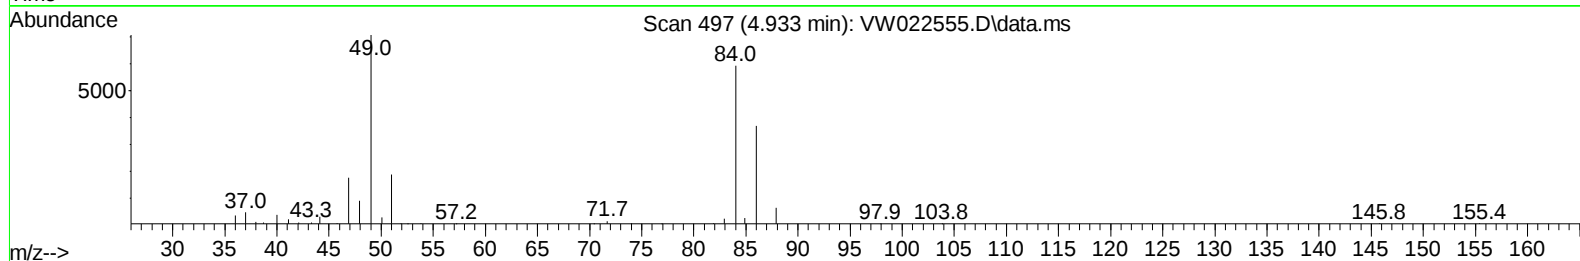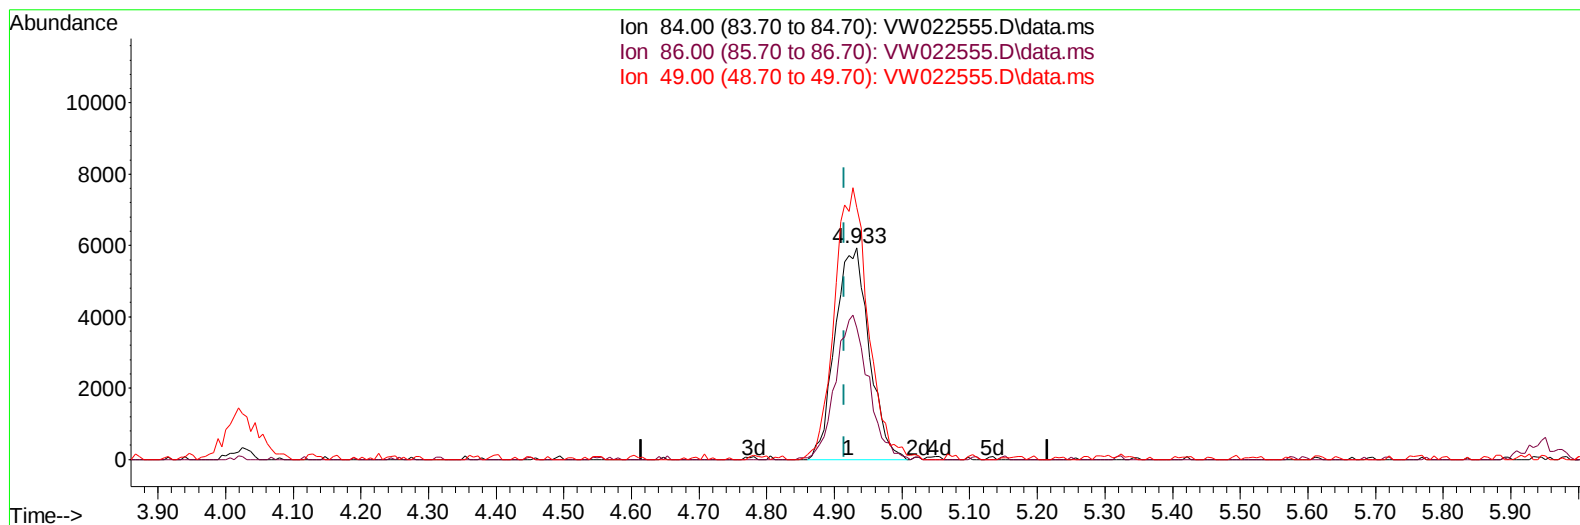

TIC: VW022555.D\data.ms

(16) Methylene chloride (T)

4.933min (+ 0.018) 4.71 ug/L m

response 20776

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.10	62.17
49.00	134.60	119.04
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041522\
 Data File : VW022555.D
 Acq On : 15 Apr 2022 13:41
 Operator : SY/VA
 Sample : N2373-11
 Misc : 5.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFF0

Manual IntegrationsAPPROVED

Quant Time: Apr 15 23:18:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 15 23:17:23 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/17/2022
 Supervised By :Mahesh Dadoda 04/20/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		293089	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.633	117		223032	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152		68935	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.361	65		100737	15.547	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	62.200%	
7) Chloroethane-d5	2.891	69		73370	18.068	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	72.280%	
11) 1,1-Dichloroethene-d2	4.019	63		103614	12.329	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	49.320%	
21) 2-Butanone-d5	7.079	46		70098	61.968	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	123.940%	
24) Chloroform-d	7.652	84		206065	22.494	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	89.960%	
26) 1,2-Dichloroethane-d4	8.305	65		122675	23.437	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	93.760%	
32) Benzene-d6	8.280	84		340176	24.965	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	99.840%	
36) 1,2-Dichloropropane-d6	9.274	67		113690	28.831	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	115.320%	
41) Toluene-d8	10.323	98		275496	20.643	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	82.560%	
43) trans-1,3-Dichloroprop...	10.579	79		35323	18.980	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	75.920%	
47) 2-Hexanone-d5	10.920	63		45003	61.340	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	122.680%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		100458	29.961	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	119.840%	
66) 1,2-Dichlorobenzene-d4	13.852	152		57243	23.444	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	93.760%	
Target Compounds							
13) Acetone	4.129	43		4159m	5.400	ug/L	Qvalue
16) Methylene chloride	4.933	84		20776m	4.711	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041522\
Data File : VW022555.D
Acq On : 15 Apr 2022 13:41
Operator : SY/VA
Sample : N2373-11
Misc : 5.55g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFFF0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/17/2022
Supervised By :Mahesh Dadoda 04/20/2022

Quant Time: Apr 15 23:18:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 15 23:17:23 2022
Response via : Initial Calibration

