




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041624\
 Data File : VW028444.D
 Acq On : 16 Apr 2024 11:10
 Operator : SY/MD
 Sample : VW0416SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK465

Manual IntegrationsAPPROVED

Quant Time: Apr 17 05:35:20 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 17 05:34:21 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/17/2024
 Supervised By :Mahesh Dadoda 04/17/2024

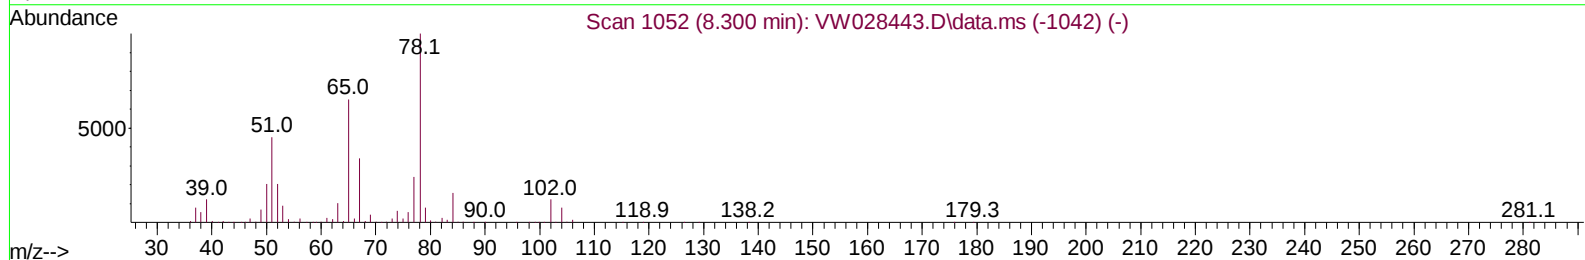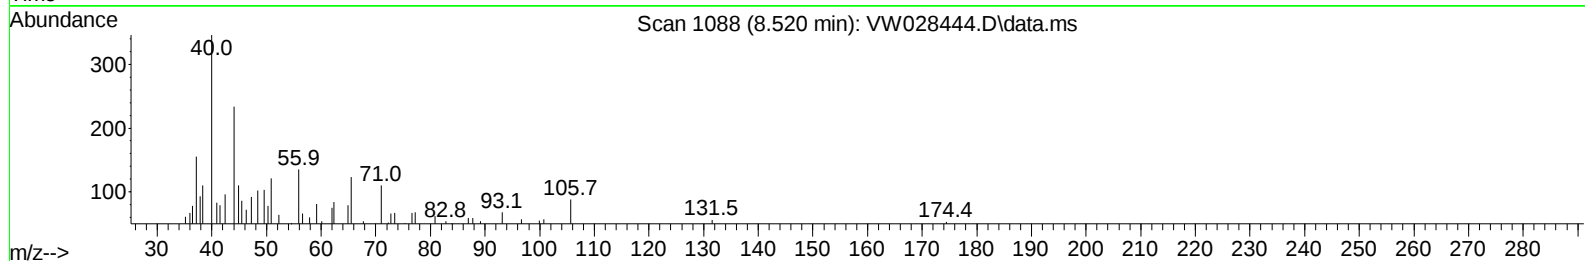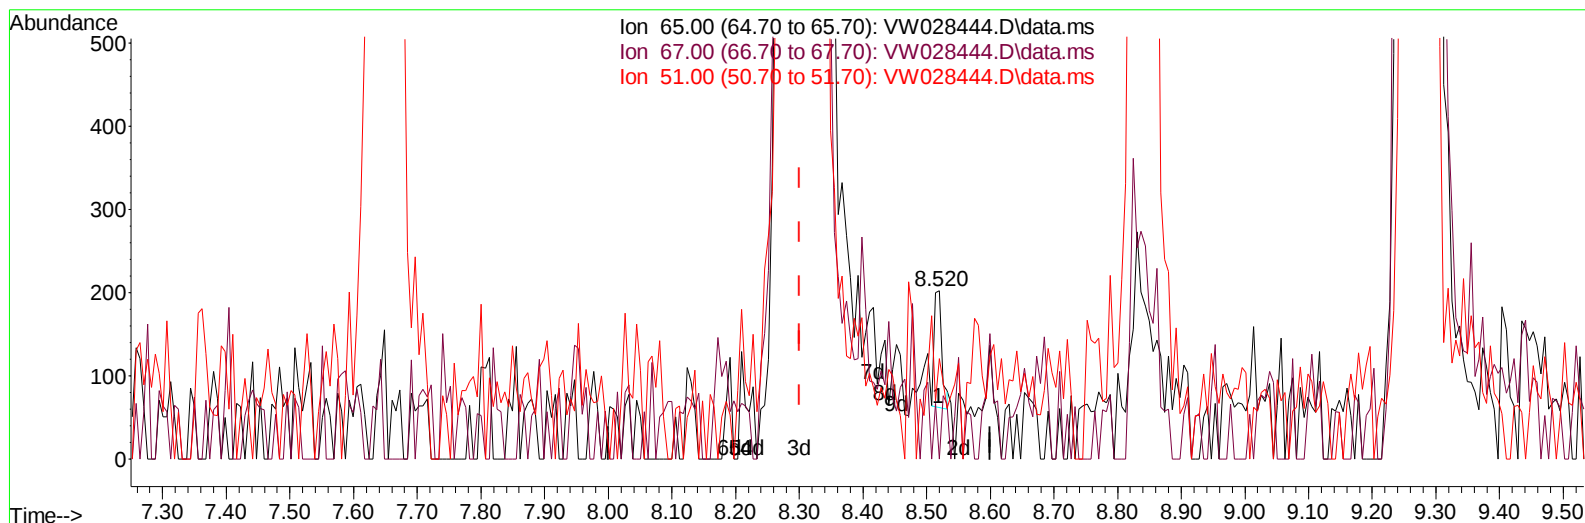

TIC: VW028444.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.520min (+ 0.220) 0.03 ug/L

response 119

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.10	43.70
51.00	108.40	84.03
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041624\
Data File : VW028444.D
Acq On : 16 Apr 2024 11:10
Operator : SY/MD
Sample : VW0416SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK465

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/17/2024
Supervised By :Mahesh Dadoda 04/17/2024

Quant Time: Apr 17 05:35:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 17 05:34:21 2024
Response via : Initial Calibration

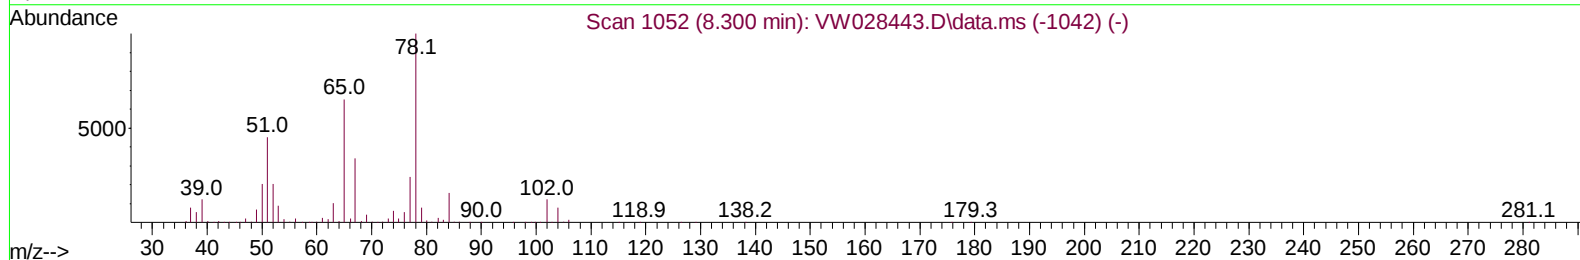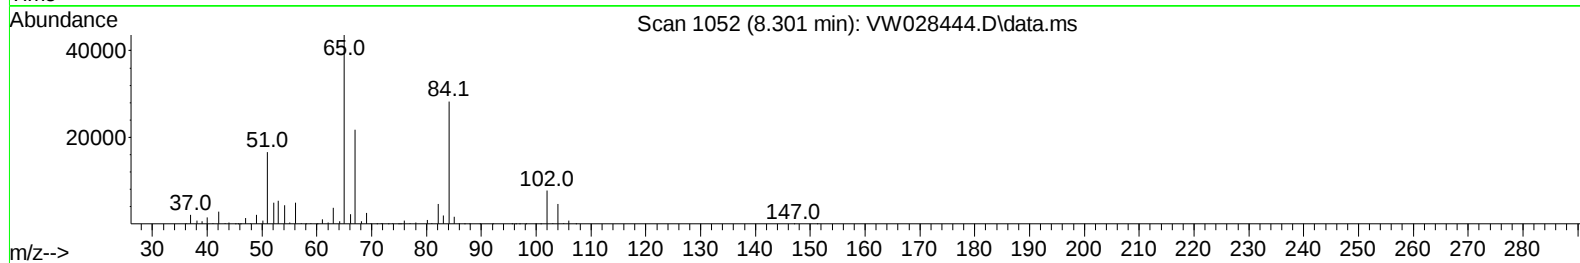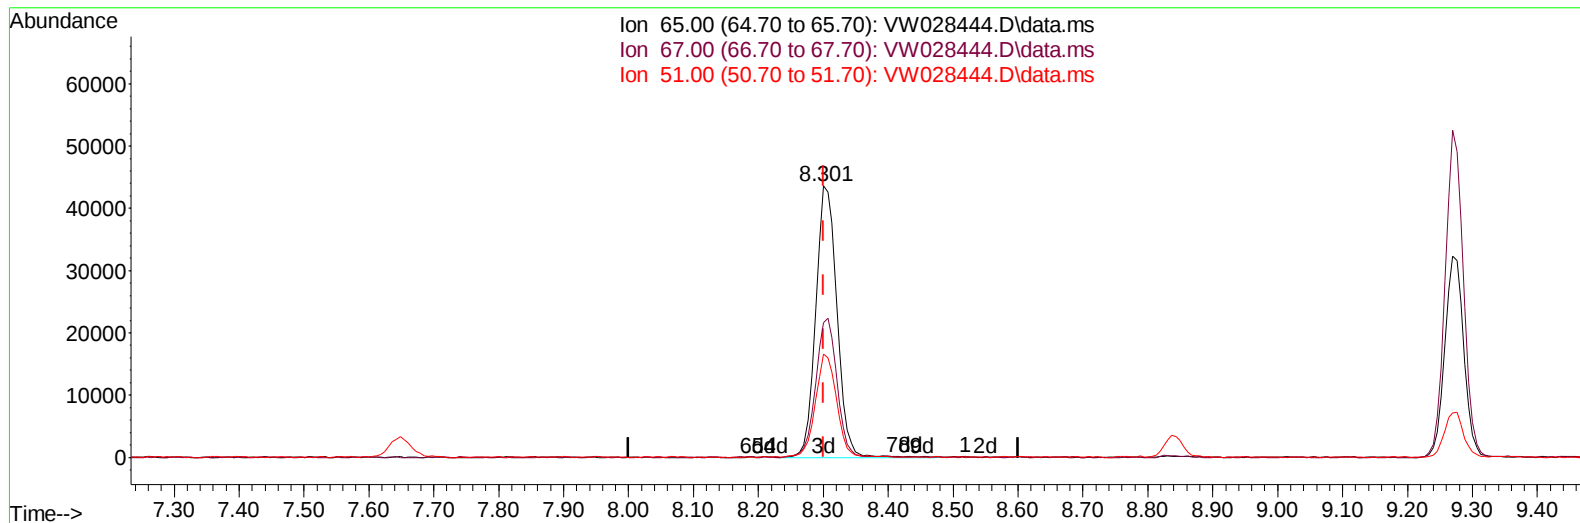

TIC: VW028444.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.301min (+ 0.000) 25.20 ug/L m

response 98869

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.10	0.05#
51.00	108.40	0.10#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041624\
 Data File : VW028444.D
 Acq On : 16 Apr 2024 11:10
 Operator : SY/MD
 Sample : VW0416SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK465

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/17/2024
 Supervised By :Mahesh Dadoda 04/17/2024

Quant Time: Apr 17 05:35:20 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 17 05:34:21 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		289373	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		262441	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		124547	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		89211	19.230	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	76.920%		
7) Chloroethane-d5	2.899	69		72036	20.487	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	81.960%		
11) 1,1-Dichloroethene-d2	4.027	65		38929	19.816	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	79.280%		
21) 2-Butanone-d5	7.075	46		46464	53.524	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	107.040%		
24) Chloroform-d	7.648	84		168716	22.344	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	89.360%		
26) 1,2-Dichloroethane-d4	8.301	65		98869m	25.195	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	100.800%		
32) Benzene-d6	8.276	84		338447	23.607	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	94.440%		
36) 1,2-Dichloropropane-d6	9.270	67		102469	24.045	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	96.160%		
41) Toluene-d8	10.319	98		304165	23.331	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	93.320%		
43) trans-1,3-Dichloroprop...	10.575	79		38830	22.915	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	91.680%		
47) 2-Hexanone-d5	10.922	63		30983	52.486	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	104.980%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		77892	25.906	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	103.640%		
66) 1,2-Dichlorobenzene-d4	13.848	152		96105	24.399	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	97.600%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041624\
Data File : VW028444.D
Acq On : 16 Apr 2024 11:10
Operator : SY/MD
Sample : VW0416SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK465

Manual IntegrationsAPPROVED

Quant Time: Apr 17 05:35:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 17 05:34:21 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/17/2024
Supervised By :Mahesh Dadoda 04/17/2024

