

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041724\
 Data File : VW028467.D
 Acq On : 17 Apr 2024 15:05
 Operator : SY/MD
 Sample : P2164-01
 Misc : 5.51g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0S99

Quant Time: Apr 18 02:21:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 18 02:19:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	565759	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	504655	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	225151	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	196366	21.650	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	86.600%		
7) Chloroethane-d5	2.899	69	155152	22.569	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	90.280%		
11) 1,1-Dichloroethene-d2	4.021	65	84862	22.094	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	88.360%		
21) 2-Butanone-d5	7.081	46	85869	50.593	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	101.180%		
24) Chloroform-d	7.648	84	343416	23.262	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	93.040%		
26) 1,2-Dichloroethane-d4	8.307	65	197679	25.766	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	103.080%		
32) Benzene-d6	8.276	84	688043	24.957	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	99.840%		
36) 1,2-Dichloropropane-d6	9.270	67	207095	25.272	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	101.080%		
41) Toluene-d8	10.319	98	621153	24.778	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	99.120%		
43) trans-1,3-Dichloroprop...	10.575	79	78997	24.244	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	96.960%		
47) 2-Hexanone-d5	10.922	63	60304	53.125	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	106.260%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	149451	25.849	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	103.400%		
66) 1,2-Dichlorobenzene-d4	13.848	152	188315	26.447	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	105.800%		
Target Compounds						Qvalue
16) Methylene chloride	4.923	84	44820	5.235	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041724\
Data File : VW028467.D
Acq On : 17 Apr 2024 15:05
Operator : SY/MD
Sample : P2164-01
Misc : 5.51g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0S99

Quant Time: Apr 18 02:21:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 18 02:19:47 2024
Response via : Initial Calibration

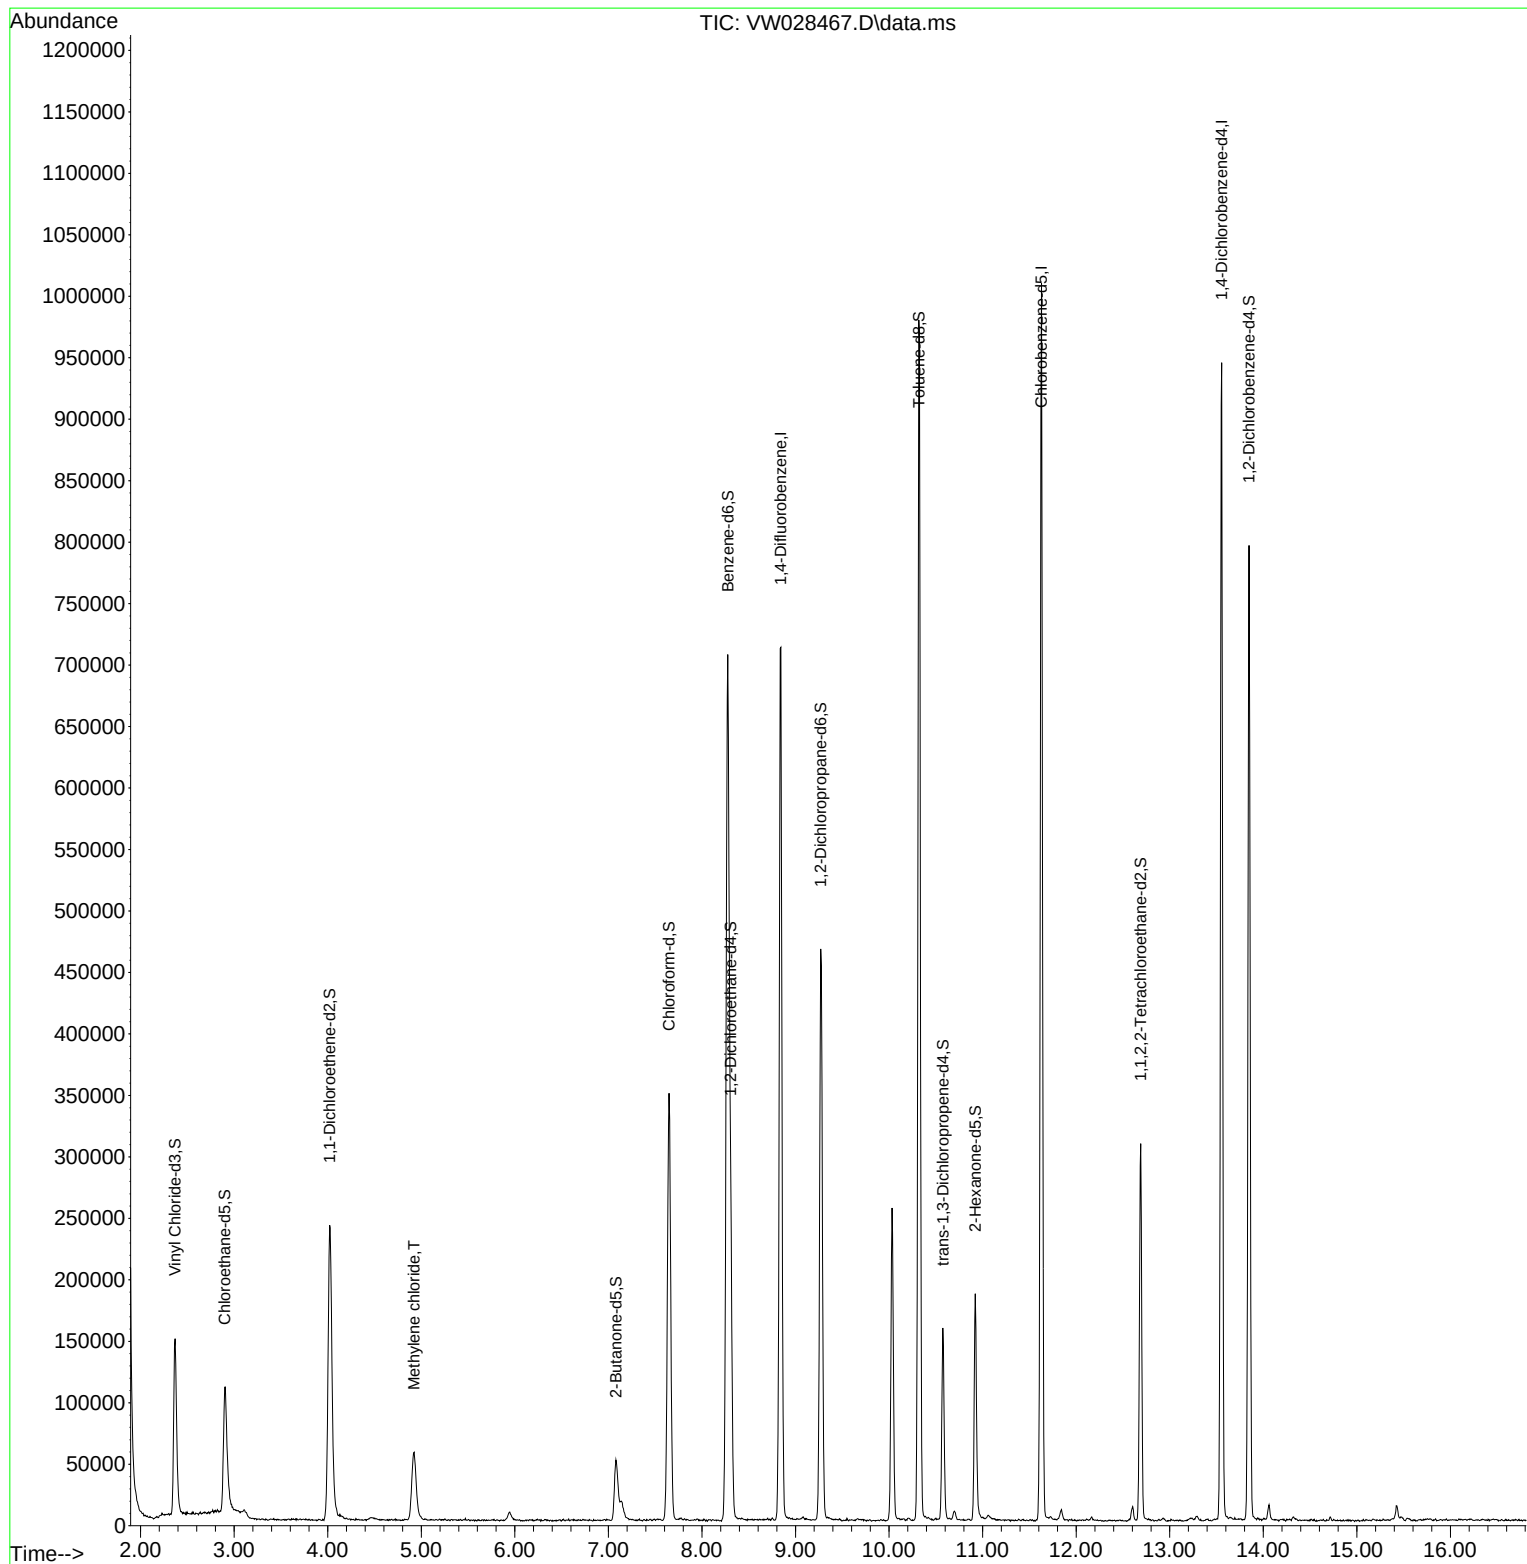

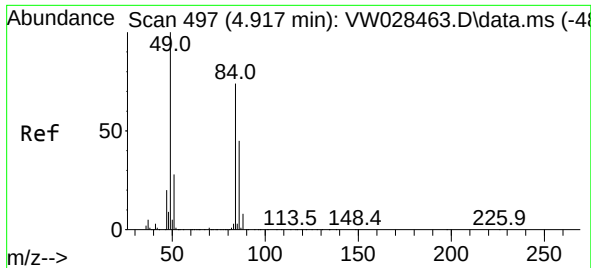

#16
Methylene chloride
Concen: 5.235 ug/L
RT: 4.923 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW028467.D
Acq: 17 Apr 2024 15:05

Instrument :
MSVOA_W
ClientSampleId :
C0S99

Tgt Ion: 84 Resp: 44820
Ion Ratio Lower Upper
84 100
86 61.9 44.2 82.0
49 124.3 95.0 176.4

