


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041824\
Data File : VW028477.D
Acq On : 18 Apr 2024 10:23
Operator : SY/MD
Sample : VW0418SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK467

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/19/2024
Supervised By :Mahesh Dadoda 04/19/2024

Quant Time: Apr 19 04:57:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 18 02:19:47 2024
Response via : Initial Calibration

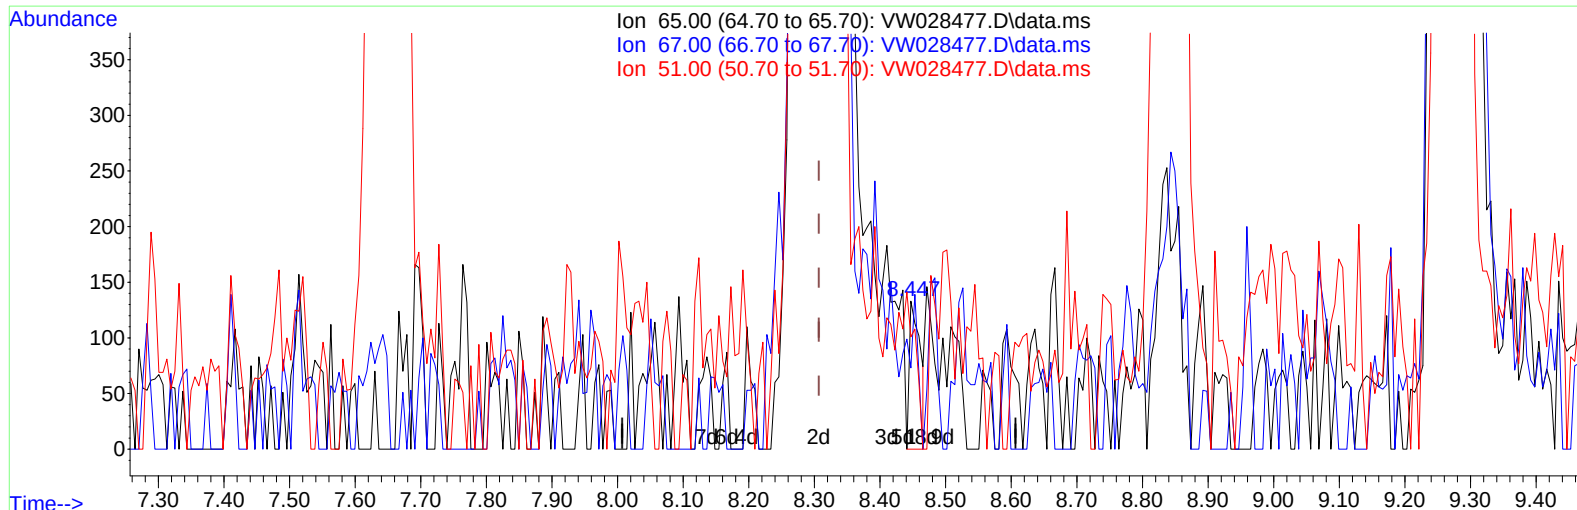




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041824\
 Data File : VW028477.D
 Acq On : 18 Apr 2024 10:23
 Operator : SY/MD
 Sample : VW0418SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK467

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/19/2024
 Supervised By :Mahesh Dadoda 04/19/2024

Quant Time: Apr 19 04:57:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 18 02:19:47 2024
 Response via : Initial Calibration

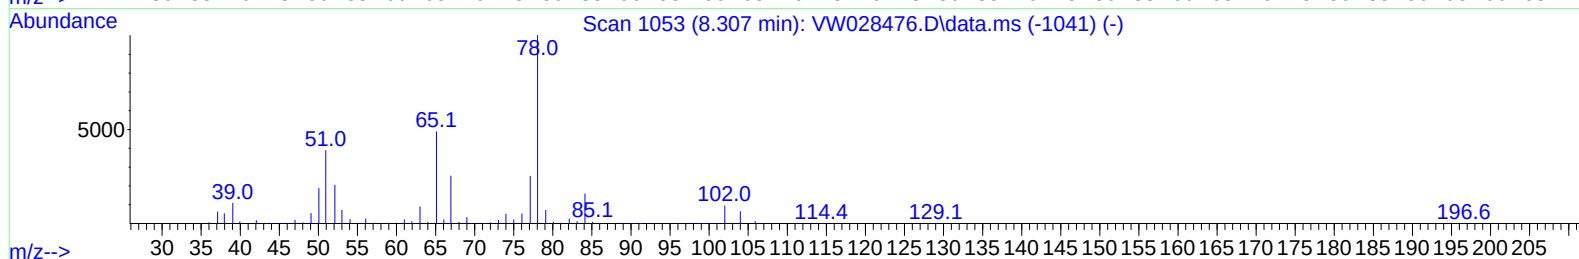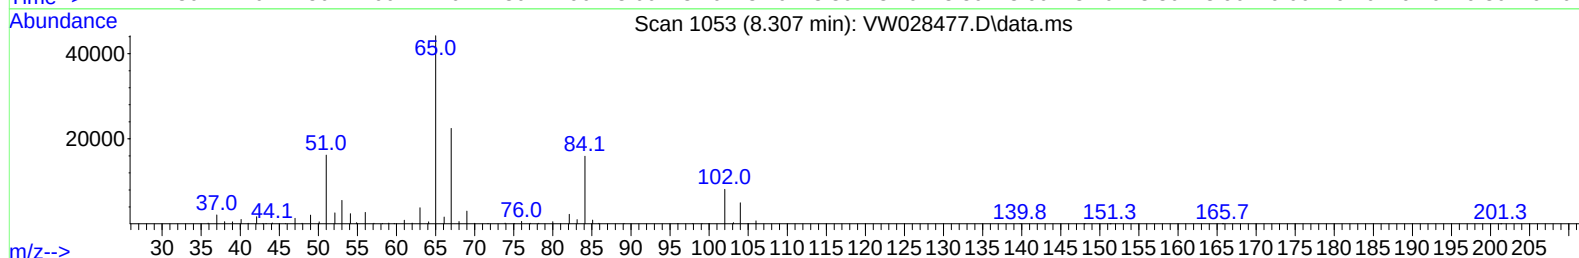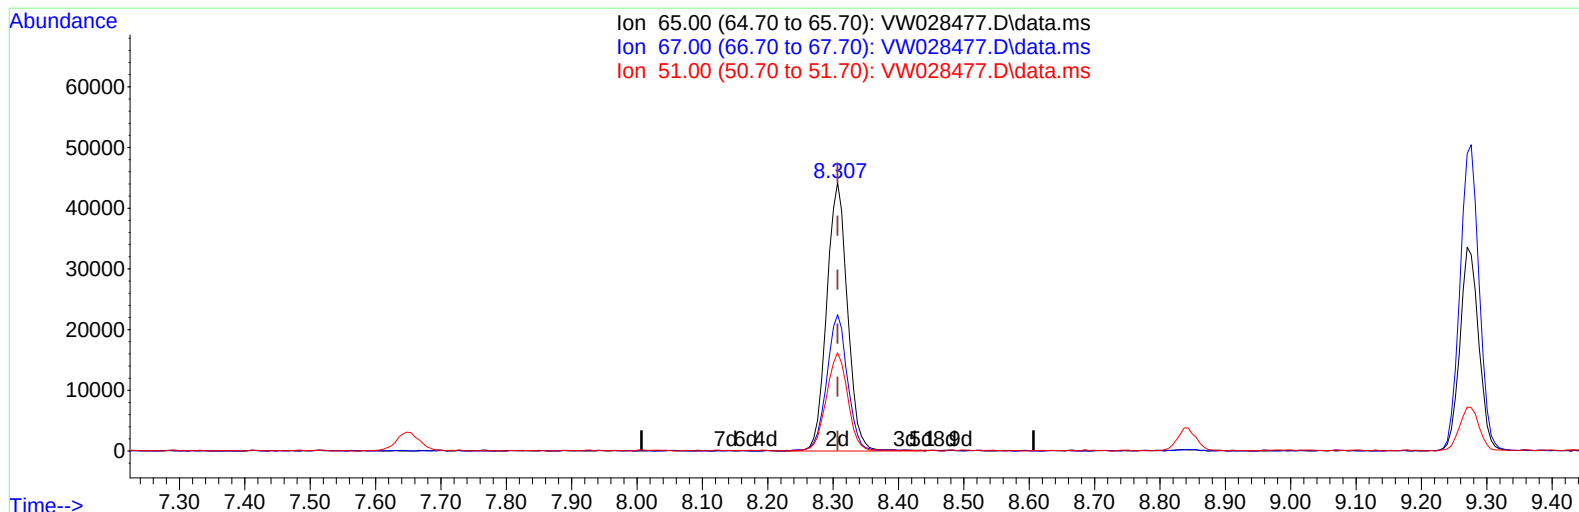

TIC: VW028477.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 22.61 ug/L m

response 97547

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.10	0.10#
51.00	108.40	0.15#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041824\
 Data File : VW028477.D
 Acq On : 18 Apr 2024 10:23
 Operator : SY/MD
 Sample : VW0418SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK467

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/19/2024
 Supervised By :Mahesh Dadoda 04/19/2024

Quant Time: Apr 19 04:57:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 18 02:19:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	318092	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	289592	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	129630	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	88819	17.417	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.680%
7) Chloroethane-d5	2.899	69	72013	18.632	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.520%
11) 1,1-Dichloroethene-d2	4.021	65	38195	17.687	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.760%
21) 2-Butanone-d5	7.081	46	43001	45.062	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.120%
24) Chloroform-d	7.648	84	171454	20.656	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.640%
26) 1,2-Dichloroethane-d4	8.307	65	97547m	22.614	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.440%
32) Benzene-d6	8.276	84	332129	20.994	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.960%
36) 1,2-Dichloropropane-d6	9.276	67	103153	21.936	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.760%
41) Toluene-d8	10.319	98	299516	20.821	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.280%
43) trans-1,3-Dichloroprop...	10.575	79	37625	20.122	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.480%
47) 2-Hexanone-d5	10.922	63	27909	42.846	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.700%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	75793	22.844	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.360%
66) 1,2-Dichlorobenzene-d4	13.848	152	97293	23.732	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.920%

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041824\
Data File : VW028477.D
Acq On : 18 Apr 2024 10:23
Operator : SY/MD
Sample : VW0418SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK467

Manual IntegrationsAPPROVED

Quant Time: Apr 19 04:57:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 18 02:19:47 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/19/2024
Supervised By :Mahesh Dadoda 04/19/2024

