

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041824\
 Data File : VW028480.D
 Acq On : 18 Apr 2024 12:24
 Operator : SY/MD
 Sample : P2164-01
 Misc : 4.56g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0S99RE

Quant Time: Apr 19 04:57:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 18 02:19:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	297913	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	277480	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	120569	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	98811	20.689	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.760%
7) Chloroethane-d5	2.899	69	79481	21.957	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.840%
11) 1,1-Dichloroethene-d2	4.021	65	42649	21.087	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	84.360%
21) 2-Butanone-d5	7.075	46	44918	50.260	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.520%
24) Chloroform-d	7.648	84	176411	22.693	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.760%
26) 1,2-Dichloroethane-d4	8.307	65	103162	25.536	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.160%
32) Benzene-d6	8.276	84	348107	22.964	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.840%
36) 1,2-Dichloropropane-d6	9.270	67	108767	24.139	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.560%
41) Toluene-d8	10.325	98	307823	22.332	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.320%
43) trans-1,3-Dichloroprop...	10.575	79	40476	22.592	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.360%
47) 2-Hexanone-d5	10.922	63	29805	47.754	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.500%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	79334	24.955	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.840%
66) 1,2-Dichlorobenzene-d4	13.848	152	94410	24.760	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.040%
Target Compounds						
13) Acetone	4.125	43	4534	4.132	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041824\
Data File : VW028480.D
Acq On : 18 Apr 2024 12:24
Operator : SY/MD
Sample : P2164-01
Misc : 4.56g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0S99RE

Quant Time: Apr 19 04:57:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 18 02:19:47 2024
Response via : Initial Calibration

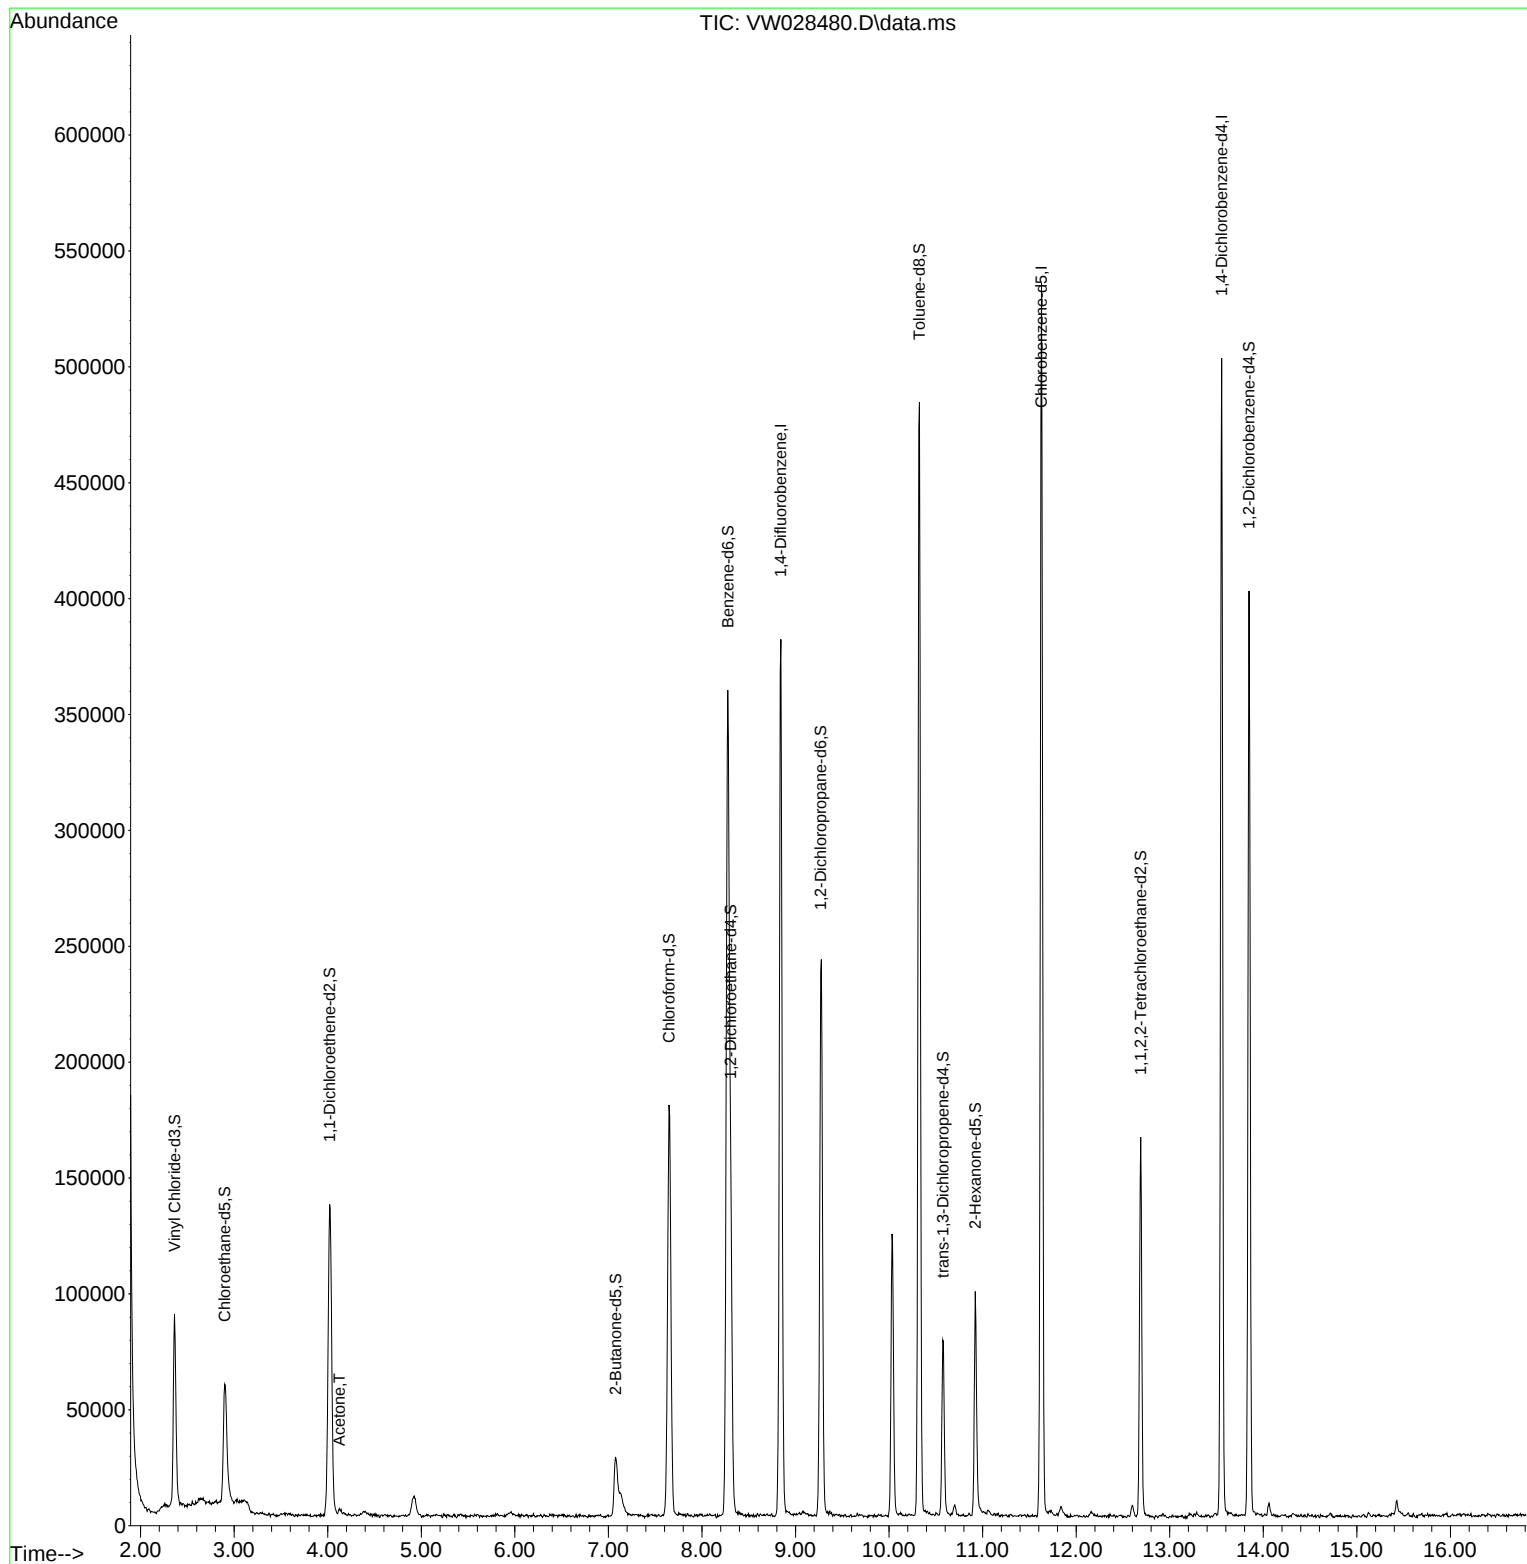

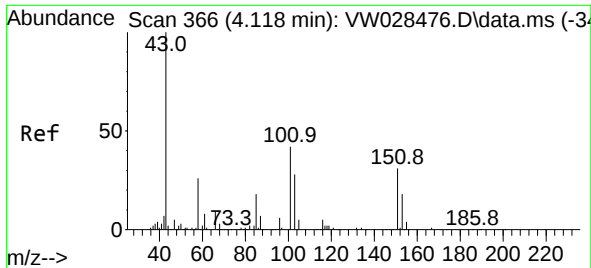

#13

Acetone

Concen: 4.132 ug/L

RT: 4.125 min Scan# 3

Delta R.T. 0.006 min

Lab File: VW028480.D


Acq: 18 Apr 2024 12:24

Instrument :

MSVOA_W

ClientSampleId :

C0S99RE

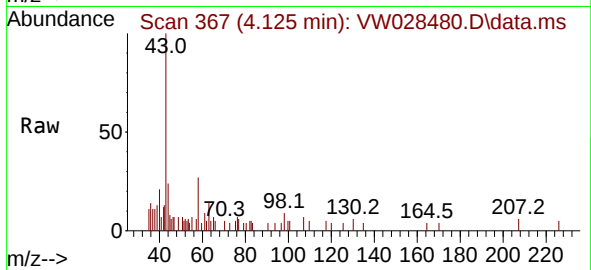

Tgt Ion: 43 Resp: 4534

Ion Ratio Lower Upper

43 100

58 22.1 0.0 53.4

