

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
 Data File : VW022585.D
 Acq On : 20 Apr 2022 13:35
 Operator : SY/VA
 Sample : N2469-05
 Misc : 3.30g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Apr 21 01:20:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 21 01:19:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	286146	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	214267	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	65447	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	81059	12.814	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	51.240%
7) Chloroethane-d5	2.891	69	62872	15.859	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	63.440%
11) 1,1-Dichloroethene-d2	4.019	63	90315	11.008	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	44.040%#
21) 2-Butanone-d5	7.208	46	309	0.280	ug/L	0.12
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.560%#
24) Chloroform-d	7.653	84	172260	19.260	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	77.040%
26) 1,2-Dichloroethane-d4	8.378	65	185	0.036	ug/L	0.07
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.160%#
32) Benzene-d6	8.275	84	296003	22.611	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.440%
36) 1,2-Dichloropropane-d6	9.274	67	93990	24.810	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.240%
41) Toluene-d8	10.323	98	229160	17.874	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	71.480%
43) trans-1,3-Dichloroprop...	10.579	79	30707	17.175	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	68.720%
47) 2-Hexanone-d5	10.927	63	35186	49.921	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.840%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	74999	23.283	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.120%
66) 1,2-Dichlorobenzene-d4	13.853	152	43043	18.568	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	74.280%#
Target Compounds					Qvalue	
13) Acetone	4.129	43	4542	6.040	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
Data File : VW022585.D
Acq On : 20 Apr 2022 13:35
Operator : SY/VA
Sample : N2469-05
Misc : 3.30g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Apr 21 01:20:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 21 01:19:16 2022
Response via : Initial Calibration

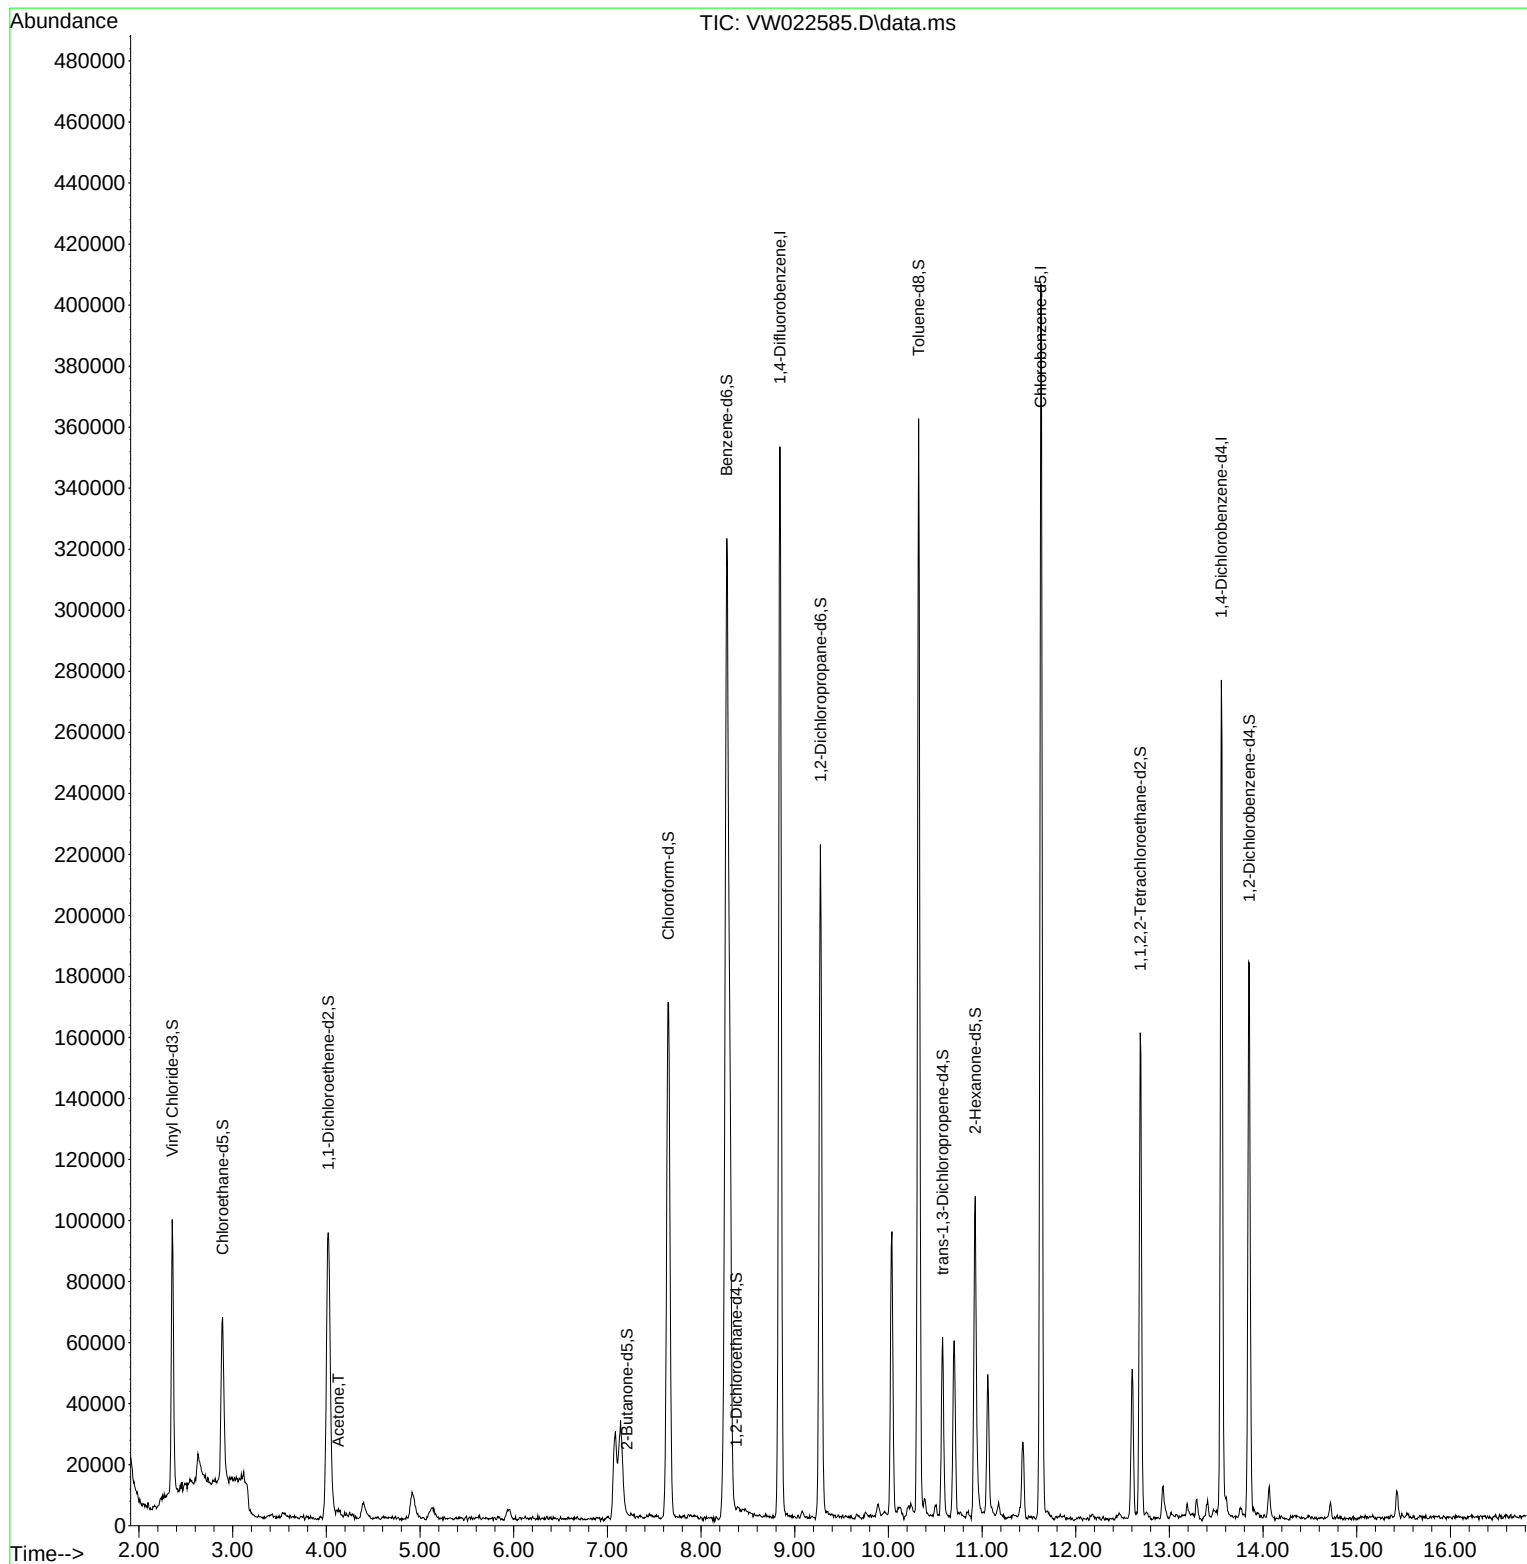

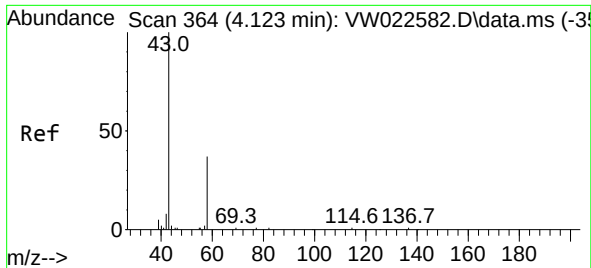

#13
 Acetone
 Concen: 6.040 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW022585.D
 Acq: 20 Apr 2022 13:35

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 43 Resp: 4542
 Ion Ratio Lower Upper
 43 100
 58 22.1 0.0 57.0

