

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
 Data File : VW022586.D
 Acq On : 20 Apr 2022 13:59
 Operator : SY/VA
 Sample : N2469-06
 Misc : 3.20g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Apr 21 01:20:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 21 01:19:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	336537	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	231395	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	57033	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	101777	13.680	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	54.720%
7) Chloroethane-d5	2.885	69	76752	16.461	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.840%
11) 1,1-Dichloroethene-d2	4.013	63	113022	11.713	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	46.840%
21) 2-Butanone-d5	7.080	46	51368	39.548	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.100%
24) Chloroform-d	7.647	84	208072	19.781	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.120%
26) 1,2-Dichloroethane-d4	8.384	65	273	0.045	ug/L	0.08
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.200%#
32) Benzene-d6	8.275	84	359806	25.451	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.800%
36) 1,2-Dichloropropane-d6	9.274	67	108925	26.624	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	106.480%
41) Toluene-d8	10.323	98	285964	20.653	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.600%
43) trans-1,3-Dichloroprop...	10.579	79	31588	16.360	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	65.440%
47) 2-Hexanone-d5	10.921	63	38335	50.363	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.720%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	64668	18.590	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	74.360%
66) 1,2-Dichlorobenzene-d4	13.853	152	35503	17.575	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	70.280%#
Target Compounds					Qvalue	
13) Acetone	4.123	43	25226	28.524	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
Data File : VW022586.D
Acq On : 20 Apr 2022 13:59
Operator : SY/VA
Sample : N2469-06
Misc : 3.20g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Apr 21 01:20:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 21 01:19:16 2022
Response via : Initial Calibration

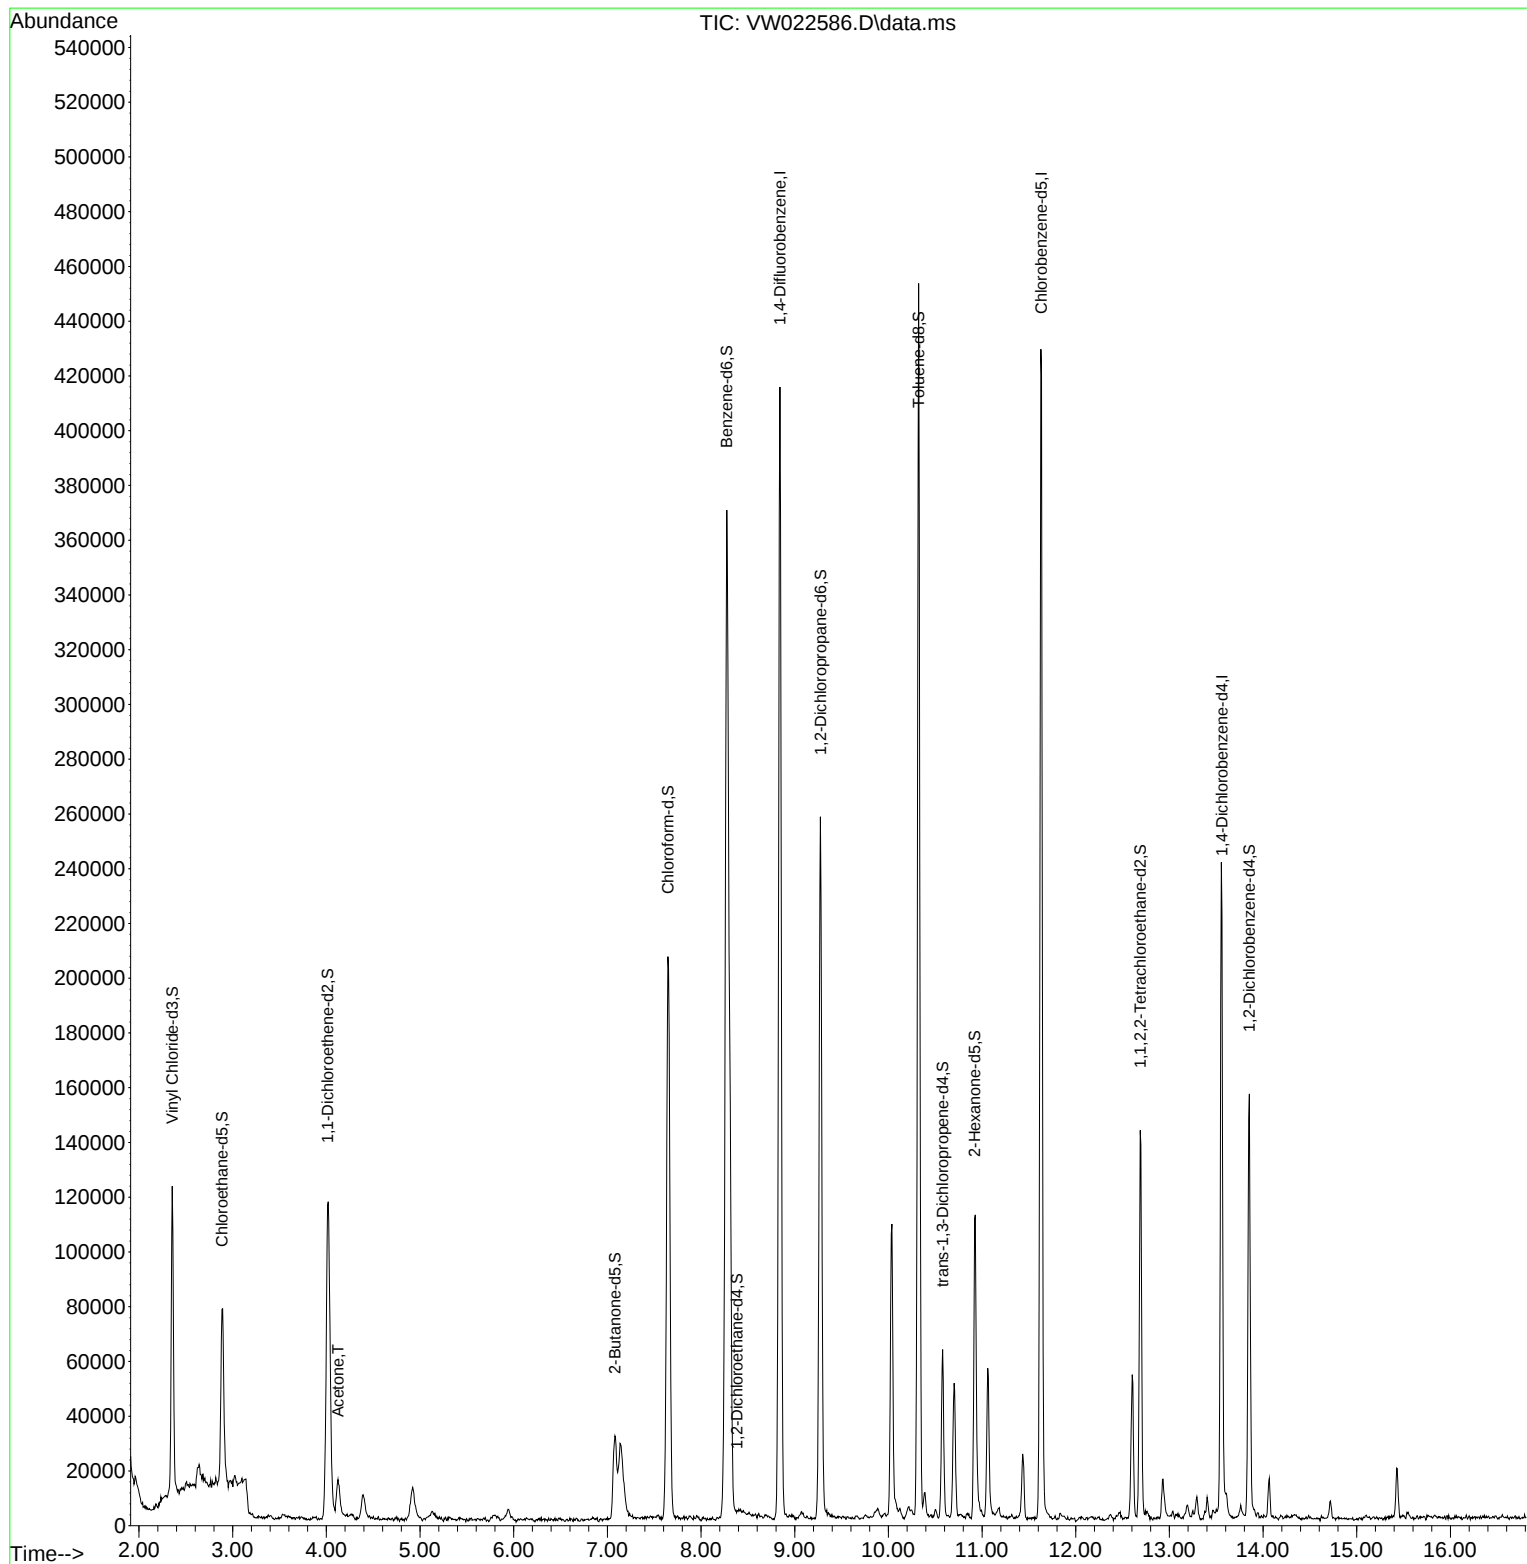

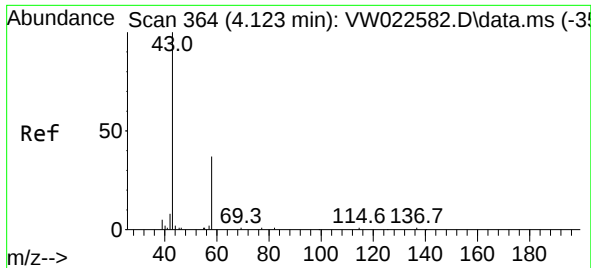

#13

Acetone

Concen: 28.524 ug/L

RT: 4.123 min Scan# 30

Delta R.T. -0.000 min


Lab File: VW022586.D

Acq: 20 Apr 2022 13:59

Instrument :

MSVOA_W

ClientSampleId :

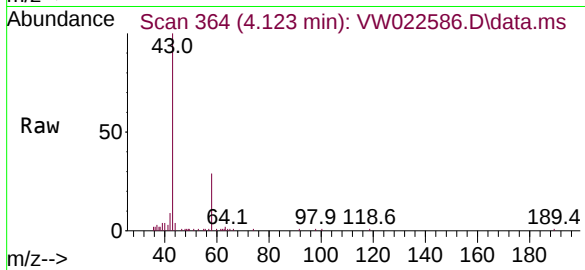

Tgt Ion: 43 Resp: 25226

Ion Ratio Lower Upper

43 100

58 28.9 0.0 57.0

