




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
Data File : VW022583.D
Acq On : 20 Apr 2022 10:57
Operator : SY/VA
Sample : VW0420SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK483

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/21/2022
Supervised By :Mahesh Dadoda 04/26/2022

Quant Time: Apr 21 01:19:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 21 01:19:16 2022
Response via : Initial Calibration

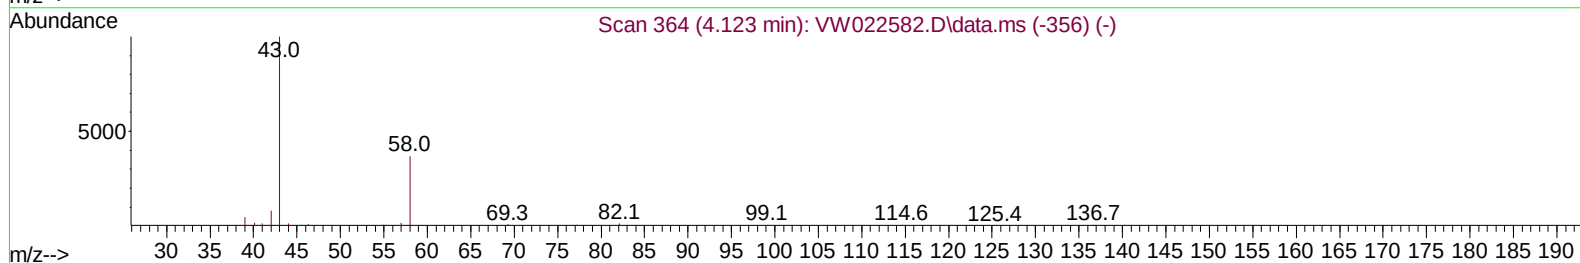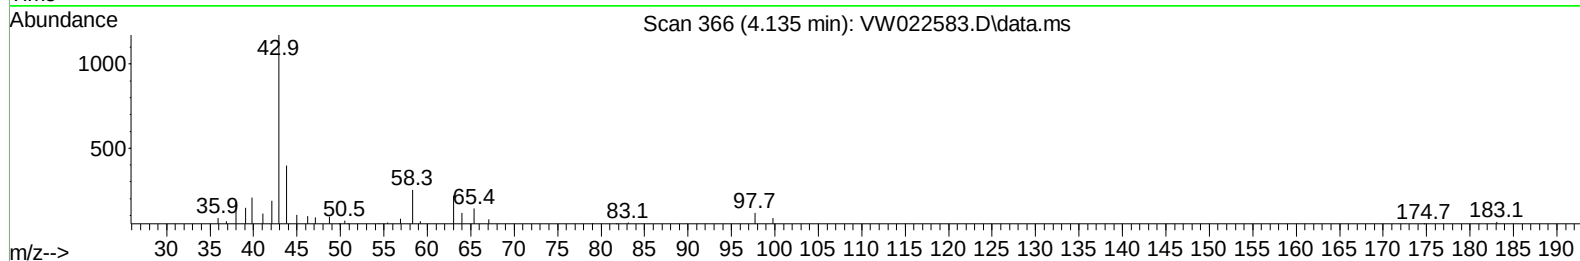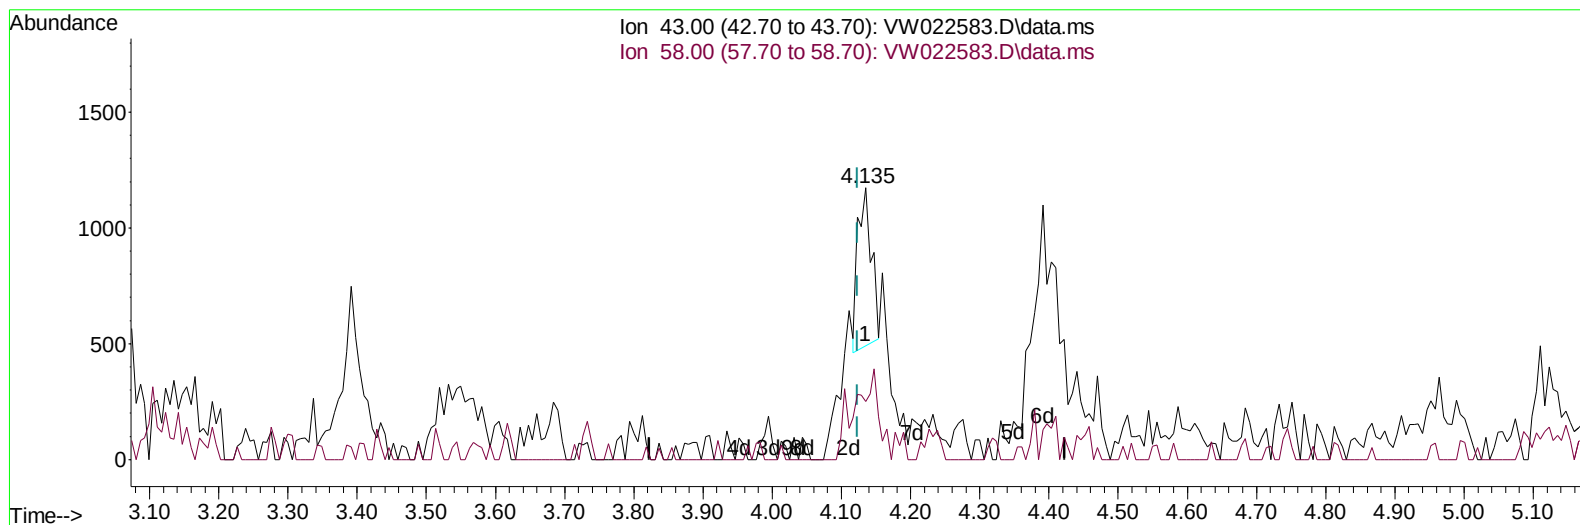

TIC: VW022583.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 1.14 ug/L

response 932

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	38.73
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
 Data File : VW022583.D
 Acq On : 20 Apr 2022 10:57
 Operator : SY/VA
 Sample : VW0420SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK483

Manual IntegrationsAPPROVED

Quant Time: Apr 21 01:19:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 21 01:19:16 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/21/2022
 Supervised By :Mahesh Dadoda 04/26/2022

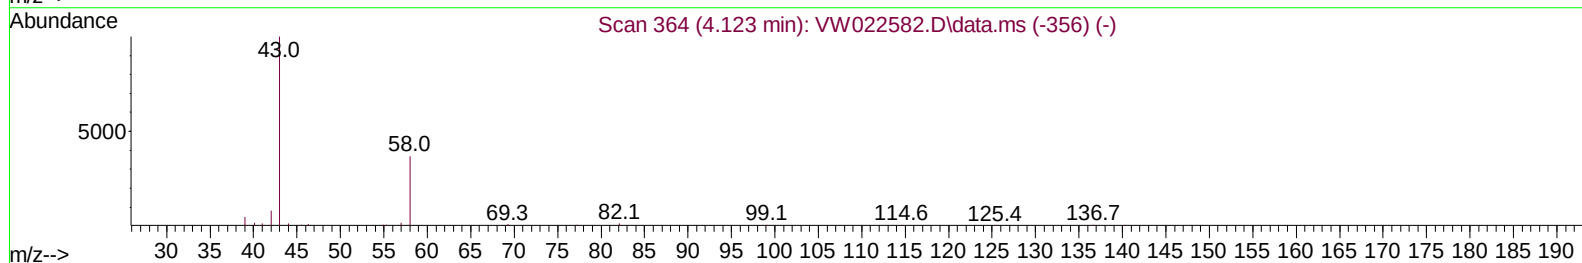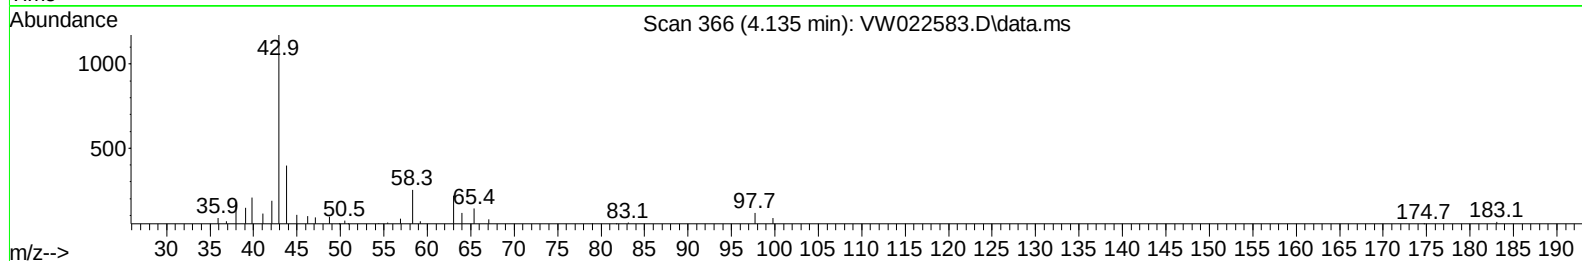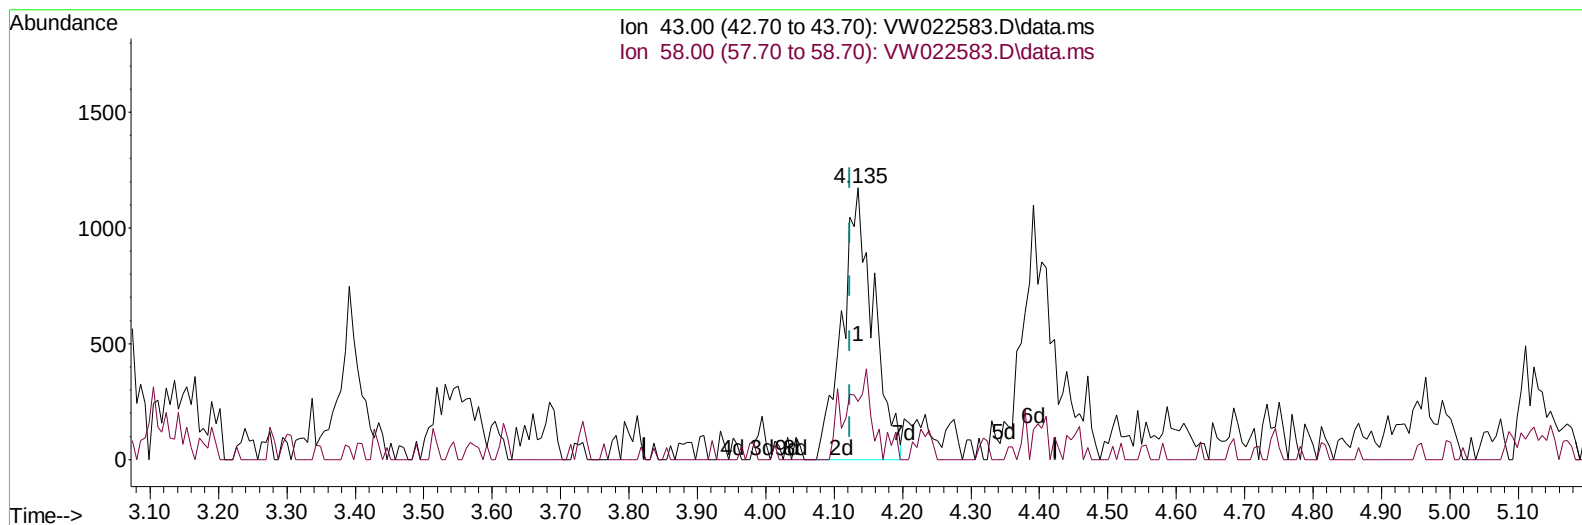

TIC: VW022583.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 4.57 ug/L m

response 3728

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	9.68
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
 Data File : VW022583.D
 Acq On : 20 Apr 2022 10:57
 Operator : SY/VA
 Sample : VW0420SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK483

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/21/2022
 Supervised By :Mahesh Dadoda 04/26/2022

Quant Time: Apr 21 01:19:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 21 01:19:16 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		310248	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		294638	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		154077	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		148330	21.627	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	86.520%	
7) Chloroethane-d5	2.891	69		94605	22.009	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	88.040%	
11) 1,1-Dichloroethene-d2	4.019	63		171630	19.293	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	77.160%	
21) 2-Butanone-d5	7.080	46		53641	44.797	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	89.600%	
24) Chloroform-d	7.653	84		240122	24.762	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	99.040%	
26) 1,2-Dichloroethane-d4	8.305	65		133879	24.163	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	96.640%	
32) Benzene-d6	8.275	84		482395	26.798	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	107.200%	
36) 1,2-Dichloropropane-d6	9.274	67		132539	25.442	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	101.760%	
41) Toluene-d8	10.323	98		457632	25.957	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	103.840%	
43) trans-1,3-Dichloroprop...	10.579	79		53391	21.717	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	86.880%	
47) 2-Hexanone-d5	10.920	63		41929	43.261	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	86.520%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		104079	23.497	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	94.000%	
66) 1,2-Dichlorobenzene-d4	13.853	152		150008	27.487	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	109.960%	
Target Compounds							
13) Acetone	4.135	43		3728m	4.573	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
Data File : VW022583.D
Acq On : 20 Apr 2022 10:57
Operator : SY/VA
Sample : VW0420SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK483

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/21/2022
Supervised By :Mahesh Dadoda 04/26/2022

Quant Time: Apr 21 01:19:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 21 01:19:16 2022
Response via : Initial Calibration

