




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
 Data File : VW022589.D
 Acq On : 20 Apr 2022 15:11
 Operator : SY/VA
 Sample : N2470-06
 Misc : 6.39g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFG9

Manual IntegrationsAPPROVED

Quant Time: Apr 21 01:21:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 21 01:19:16 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/21/2022
 Supervised By :Mahesh Dadoda 04/26/2022

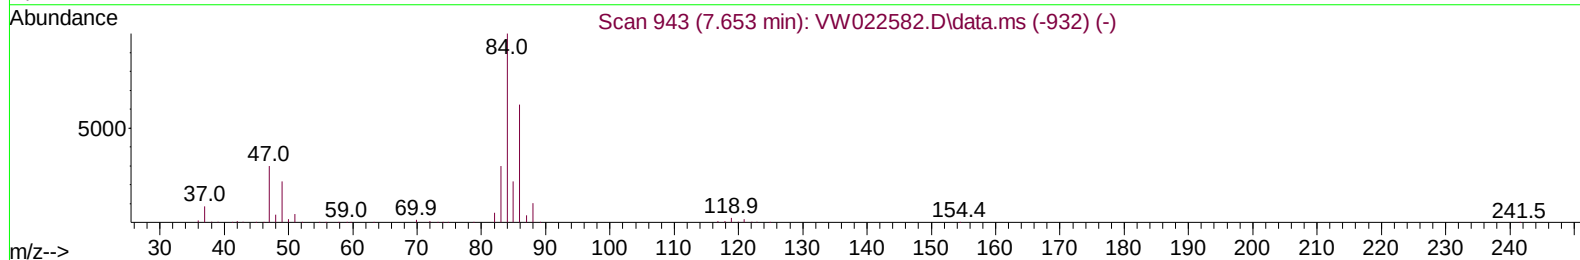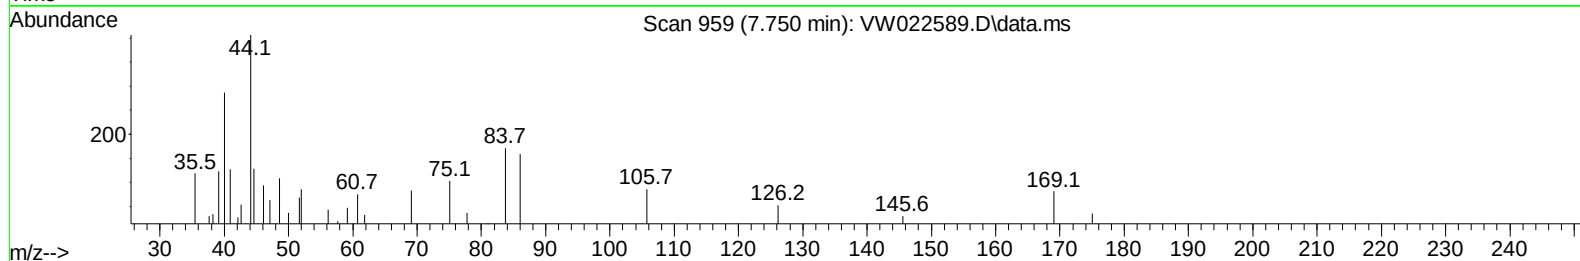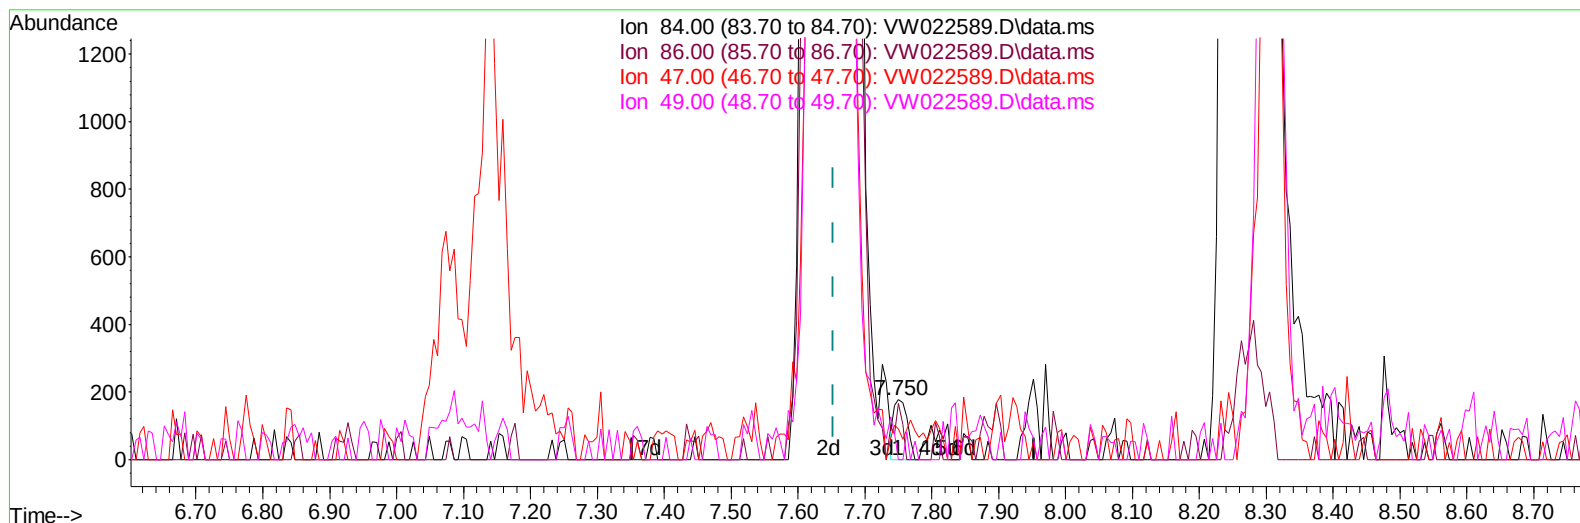

TIC: VW022589.D\data.ms

(24) Chloroform-d (S)

7.750min (+ 0.097) 0.02 ug/L

response 252

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.80	64.29
47.00	51.50	46.03
49.00	31.80	29.76




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
 Data File : VW022589.D
 Acq On : 20 Apr 2022 15:11
 Operator : SY/VA
 Sample : N2470-06
 Misc : 6.39g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFG9

Manual IntegrationsAPPROVED

Quant Time: Apr 21 01:21:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 21 01:19:16 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/21/2022
 Supervised By :Mahesh Dadoda 04/26/2022

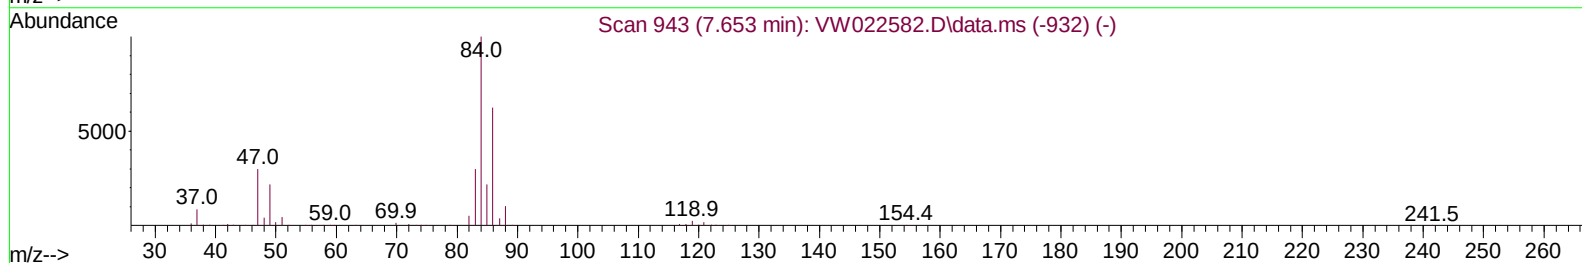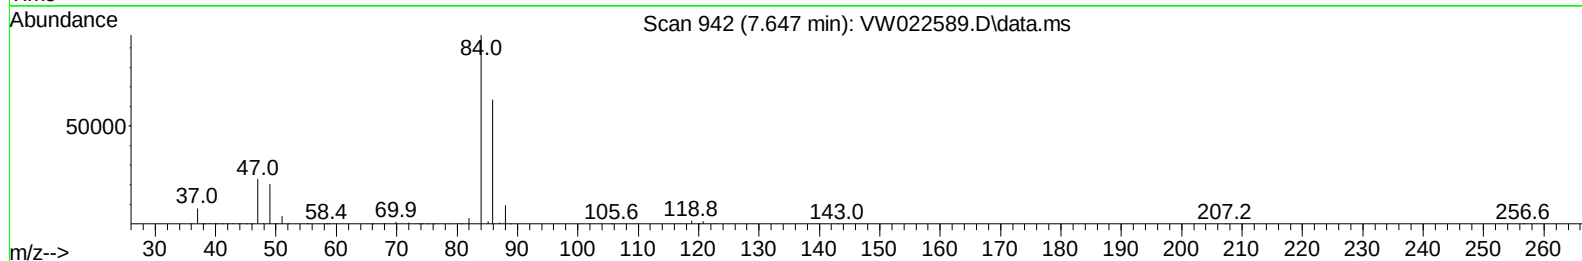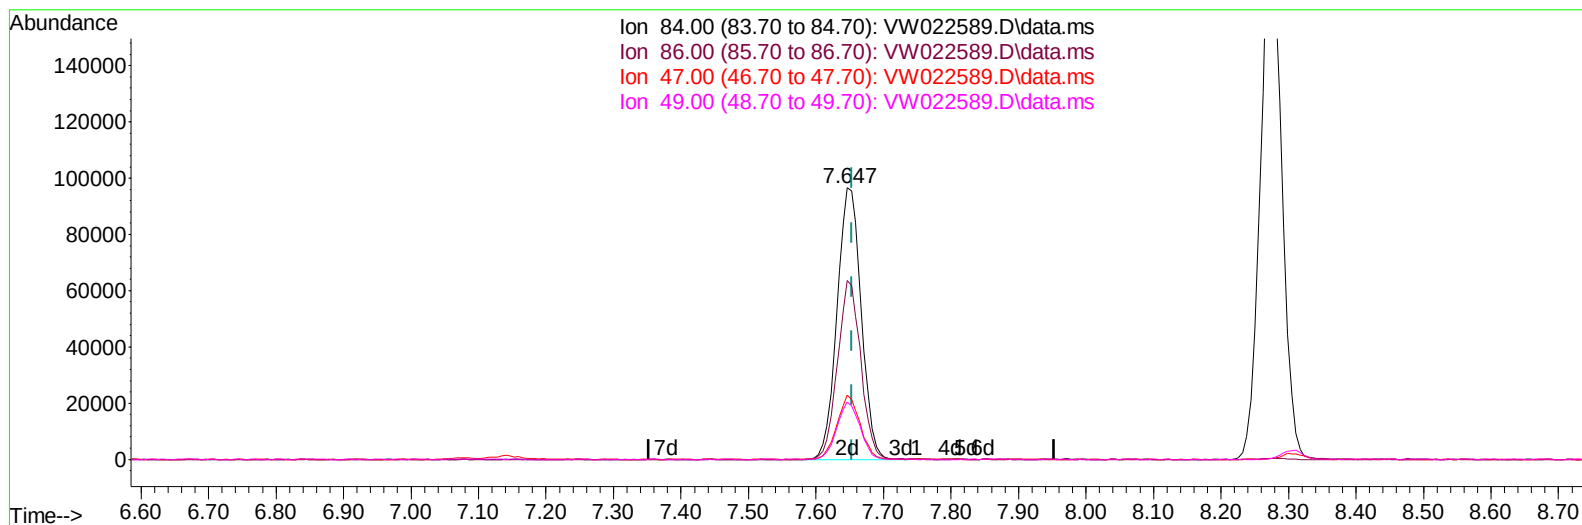

TIC: VW022589.D\data.ms

(24) Chloroform-d (S)

7.647min (-0.006) 20.89 ug/L m

response 239375

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.80	0.07#
47.00	51.50	0.05#
49.00	31.80	0.03#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
 Data File : VW022589.D
 Acq On : 20 Apr 2022 15:11
 Operator : SY/VA
 Sample : N2470-06
 Misc : 6.39g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFG9

Manual IntegrationsAPPROVED

Quant Time: Apr 21 01:21:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 21 01:19:16 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/21/2022
 Supervised By :Mahesh Dadoda 04/26/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		366670	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		342931	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		164769	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		104565	12.900	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	51.600%		
7) Chloroethane-d5	2.885	69		81402	16.023	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	64.080%		
11) 1,1-Dichloroethene-d2	4.019	63		121134	11.522	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	46.080%		
21) 2-Butanone-d5	7.080	46		63687	45.002	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	90.000%		
24) Chloroform-d	7.647	84		239375m	20.886	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	83.560%		
26) 1,2-Dichloroethane-d4	8.305	65		132913	20.297	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	81.200%		
32) Benzene-d6	8.275	84		408959	19.519	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	78.080%		
36) 1,2-Dichloropropane-d6	9.274	67		130896	21.589	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	86.360%		
41) Toluene-d8	10.323	98		368967	17.981	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	71.920%		
43) trans-1,3-Dichloroprop...	10.579	79		50034	17.485	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	69.960%		
47) 2-Hexanone-d5	10.927	63		51871	45.982	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	91.960%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		120948	23.460	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	93.840%		
66) 1,2-Dichlorobenzene-d4	13.853	152		135201	23.166	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	92.680%		
Target Compounds							
13) Acetone	4.129	43		11945	12.397	ug/L	Qvalue 73

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
Data File : VW022589.D
Acq On : 20 Apr 2022 15:11
Operator : SY/VA
Sample : N2470-06
Misc : 6.39g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFFG9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/21/2022
Supervised By :Mahesh Dadoda 04/26/2022

Quant Time: Apr 21 01:21:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 21 01:19:16 2022
Response via : Initial Calibration

