




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
 Data File : VW022596.D
 Acq On : 20 Apr 2022 17:59
 Operator : SY/VA
 Sample : VIBLK430
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK430

Manual IntegrationsAPPROVED

Quant Time: Apr 21 01:22:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 21 01:19:16 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/21/2022
 Supervised By :Mahesh Dadoda 04/26/2022

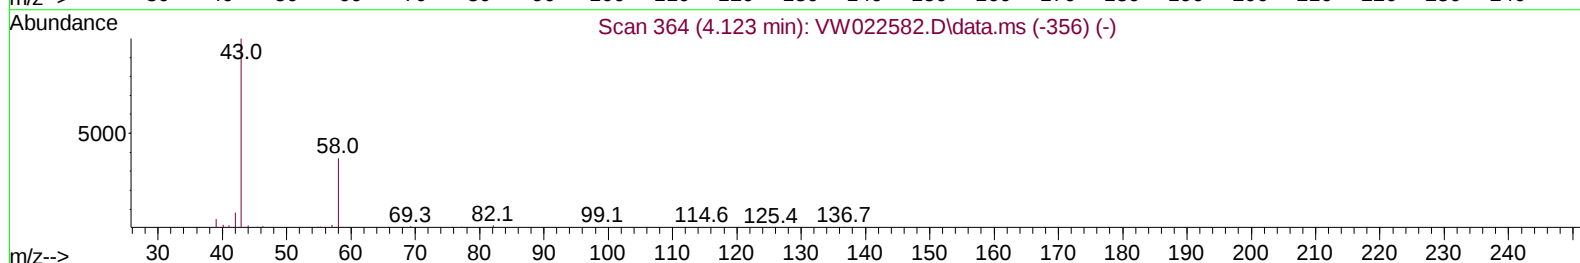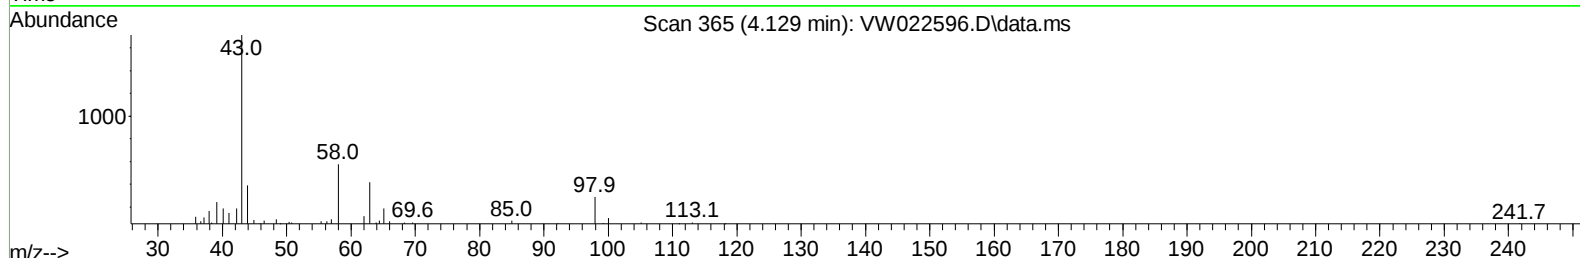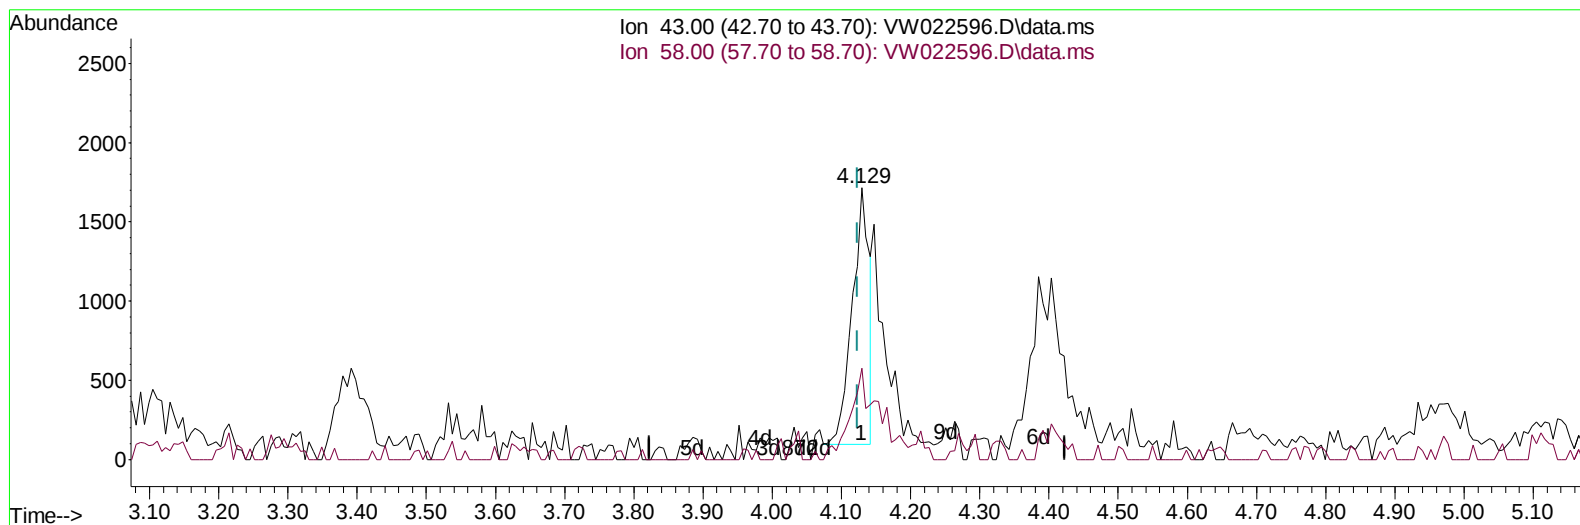

TIC: VW022596.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 3.41 ug/L

response 2751

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	29.41
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
 Data File : VW022596.D
 Acq On : 20 Apr 2022 17:59
 Operator : SY/VA
 Sample : VIBLK430
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK430

Manual IntegrationsAPPROVED

Quant Time: Apr 21 01:22:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 21 01:19:16 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/21/2022
 Supervised By :Mahesh Dadoda 04/26/2022

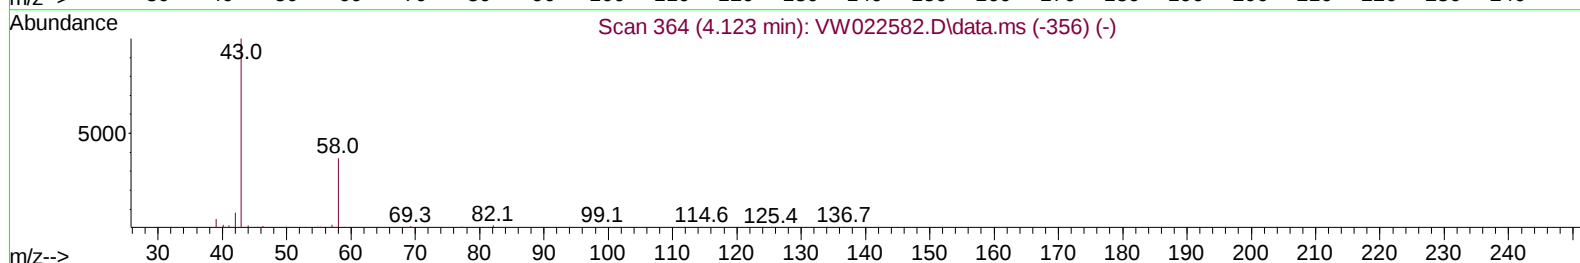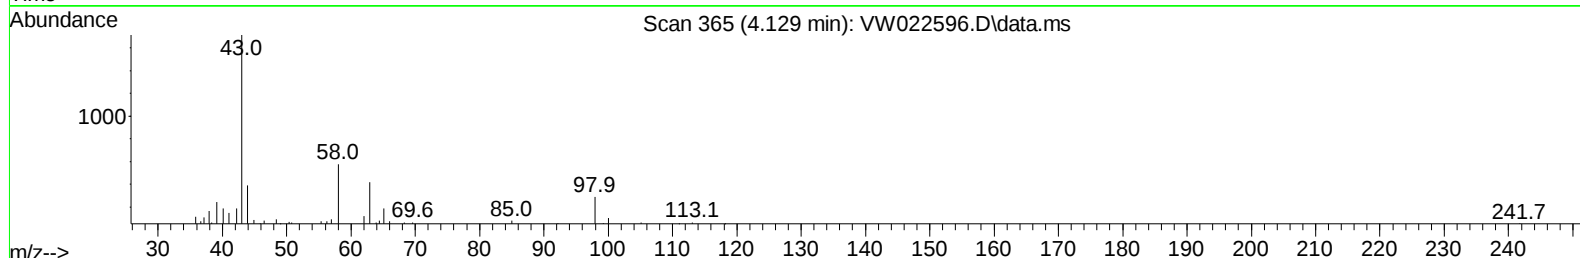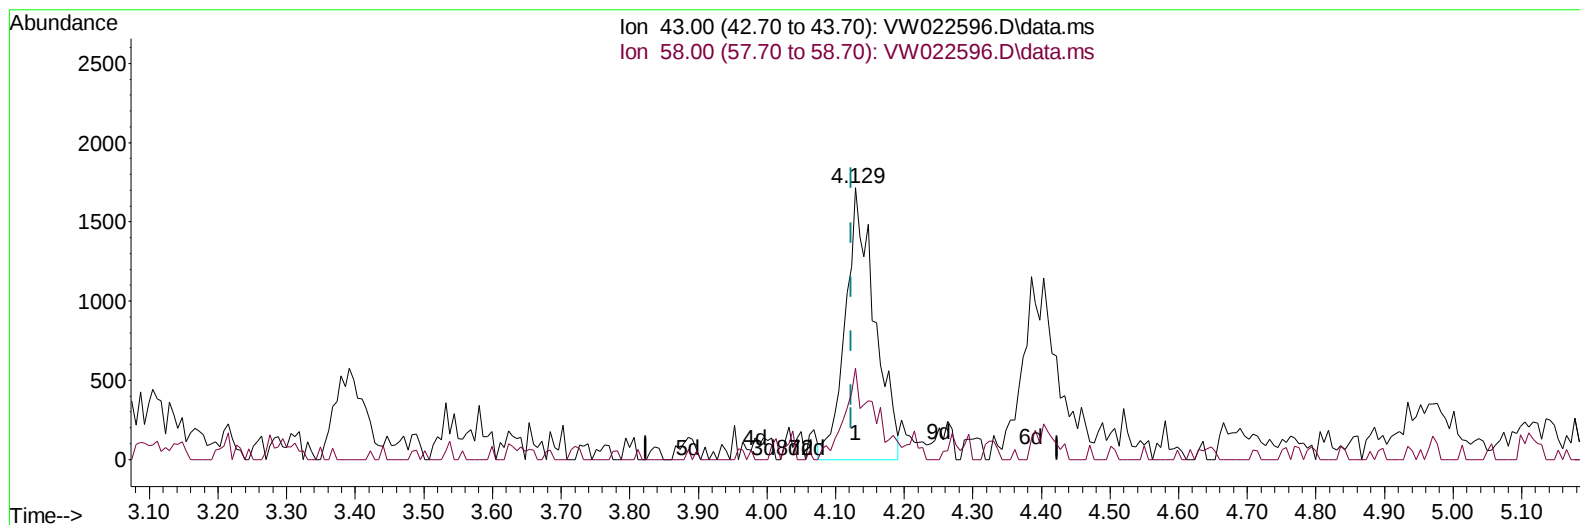

TIC: VW022596.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 6.30 ug/L m

response 5073

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	15.95
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
 Data File : VW022596.D
 Acq On : 20 Apr 2022 17:59
 Operator : SY/VA
 Sample : VIBLK430
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK430

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/21/2022
 Supervised By :Mahesh Dadoda 04/26/2022

Quant Time: Apr 21 01:22:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 21 01:19:16 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		306665	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		296575	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		154630	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		299541	44.184	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	= 176.720%#		
7) Chloroethane-d5	2.892	69		207363	48.805	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	= 195.200%#		
11) 1,1-Dichloroethene-d2	4.019	63		328764	37.389	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	= 149.560%#		
21) 2-Butanone-d5	7.080	46		113391	95.802	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	= 191.600%#		
24) Chloroform-d	7.647	84		464856	48.497	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	= 194.000%#		
26) 1,2-Dichloroethane-d4	8.305	65		262938	48.010	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	= 192.040%#		
32) Benzene-d6	8.275	84		930839	51.372	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	= 205.480%#		
36) 1,2-Dichloropropane-d6	9.275	67		263152	50.185	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	= 200.760%#		
41) Toluene-d8	10.323	98		902297	50.845	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	= 203.360%#		
43) trans-1,3-Dichloroprop...	10.579	79		114046	46.085	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	= 184.360%#		
47) 2-Hexanone-d5	10.921	63		97065	99.494	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	= 198.980%#		
56) 1,1,2,2-Tetrachloroeth...	12.689	84		219787	49.296	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	= 197.200%#		
66) 1,2-Dichlorobenzene-d4	13.853	152		286376	52.287	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	= 209.160%#		
Target Compounds							
13) Acetone	4.129	43		5073m	6.295	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
Data File : VW022596.D
Acq On : 20 Apr 2022 17:59
Operator : SY/VA
Sample : VIBLK430
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK430

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/21/2022
Supervised By :Mahesh Dadoda 04/26/2022

Quant Time: Apr 21 01:22:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 21 01:19:16 2022
Response via : Initial Calibration

