

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
 Data File : VW022584.D
 Acq On : 20 Apr 2022 13:11
 Operator : SY/VA
 Sample : N2469-04
 Misc : 5.46g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFG4

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/21/2022
 Supervised By : Mahesh Dadoda 04/26/2022

Quant Time: Apr 21 01:20:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 21 01:19:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	373784	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	284972	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	79141	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	108680	13.152	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	52.600%		
7) Chloroethane-d5	2.891	69	78441	15.147	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	60.600%		
11) 1,1-Dichloroethene-d2	4.013	63	130344	12.162	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	48.640%		
21) 2-Butanone-d5	7.074	46	60127	41.678	ug/L	-0.01
Spiked Amount 50.000	Range 20 - 135		Recovery =	83.360%		
24) Chloroform-d	7.647	84	240304	20.568	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	82.280%		
26) 1,2-Dichloroethane-d4	8.305	65	132994m	19.923	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	79.680%		
32) Benzene-d6	8.275	84	409120	23.498	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	94.000%		
36) 1,2-Dichloropropane-d6	9.274	67	130800	25.960	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	103.840%		
41) Toluene-d8	10.323	98	329906	19.347	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	77.400%		
43) trans-1,3-Dichloroprop...	10.573	79	40276	16.938	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	67.760%		
47) 2-Hexanone-d5	10.920	63	39207	41.824	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	83.640%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	88663	20.696	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	82.800%		
66) 1,2-Dichlorobenzene-d4	13.853	152	55761	19.892	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	79.560%		
Target Compounds					Qvalue	
13) Acetone	4.123	43	4041	4.114	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
Data File : VW022584.D
Acq On : 20 Apr 2022 13:11
Operator : SY/VA
Sample : N2469-04
Misc : 5.46g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BFFG4

Quant Time: Apr 21 01:20:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 21 01:19:16 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 04/21/2022
Supervised By : Mahesh Dadoda 04/26/2022

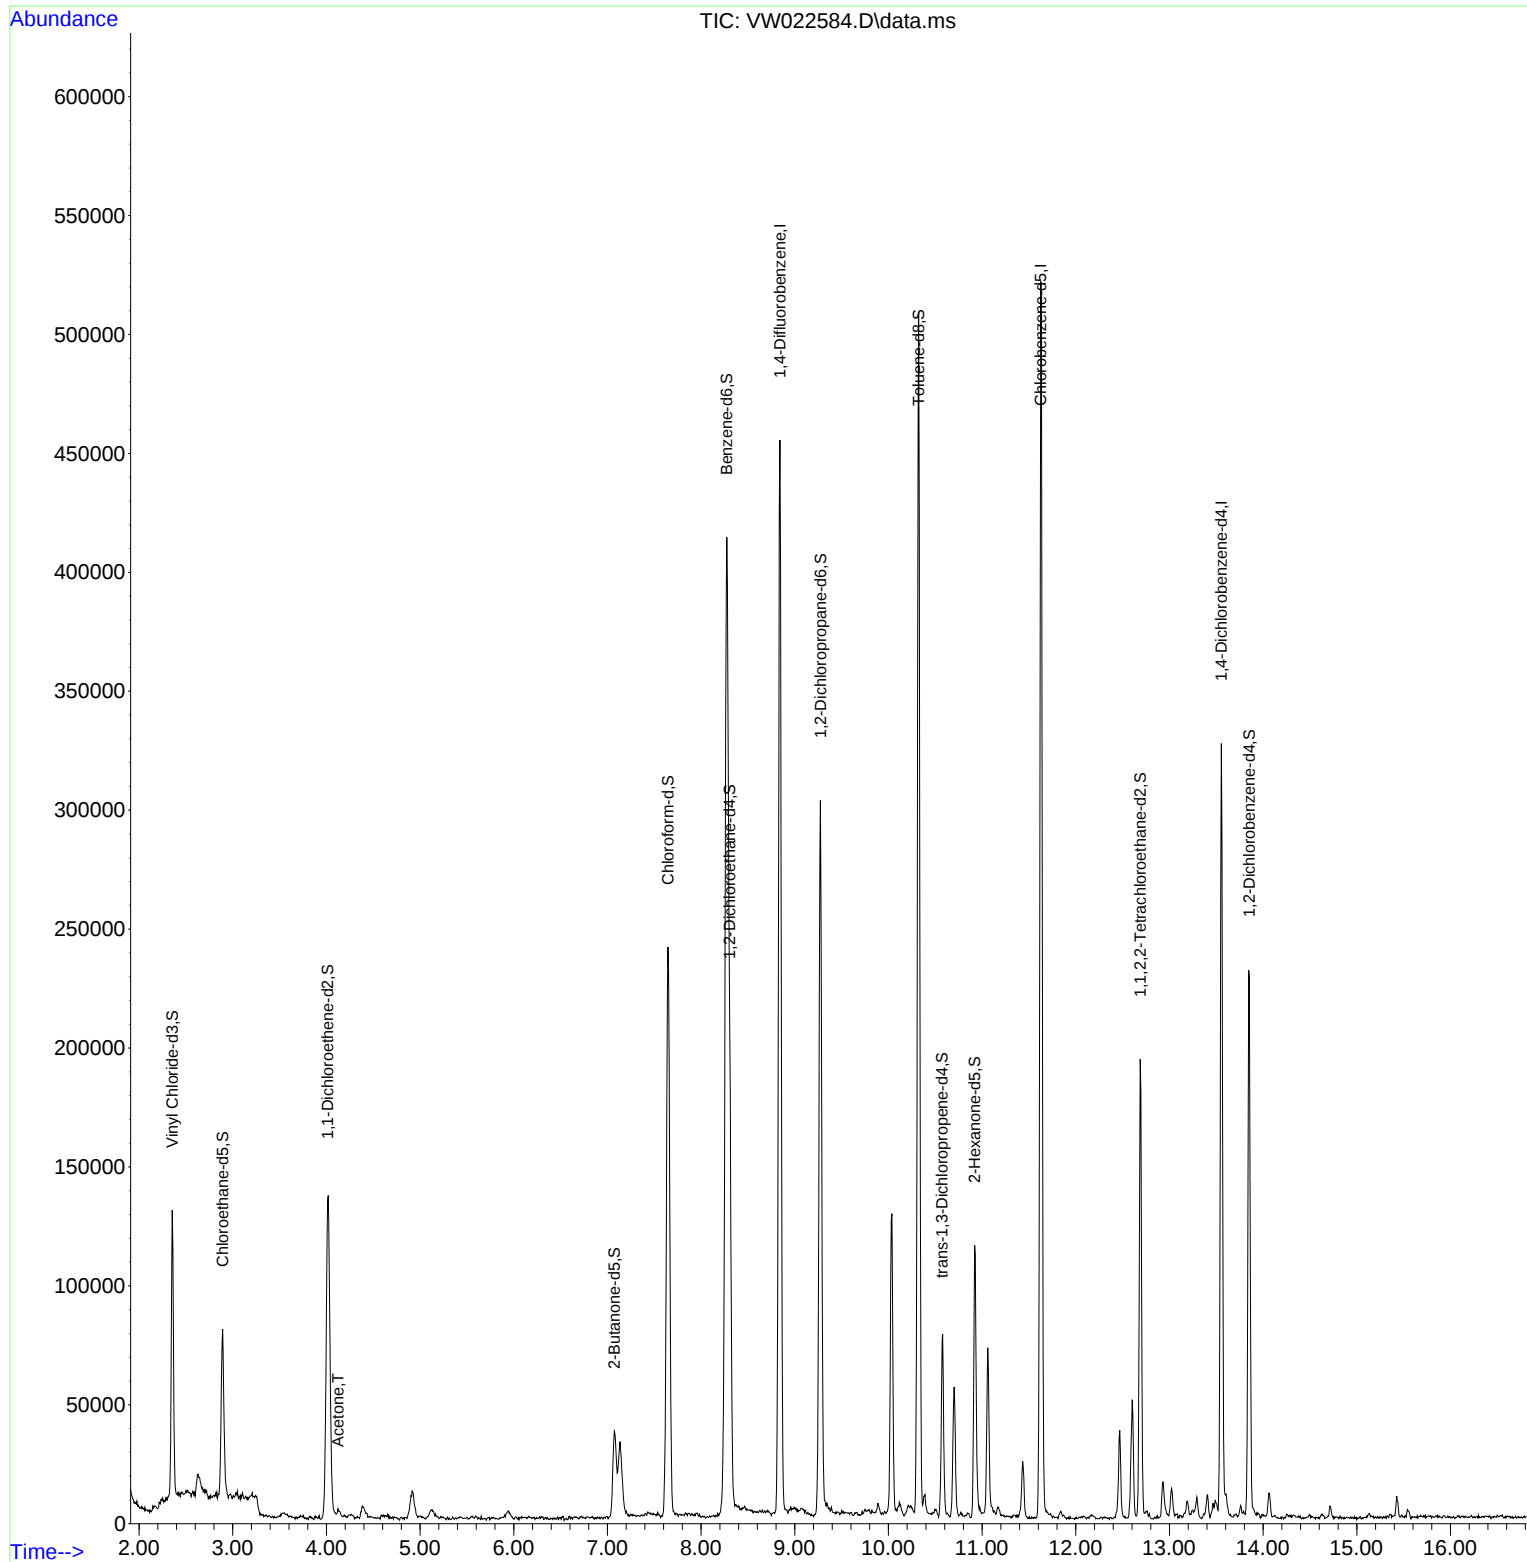

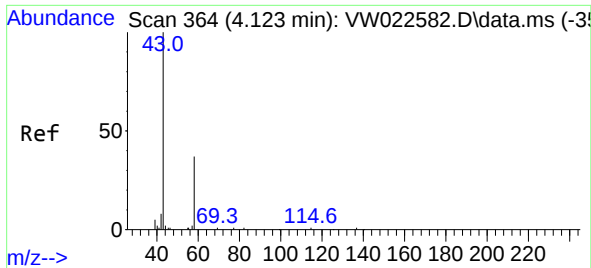

#13
Acetone
Concen: 4.114 ug/L
RT: 4.123 min Scan# 30
Delta R.T. -0.000 min
Lab File: VW022584.D
Acq: 20 Apr 2022 13:11

Instrument :
MSVOA_W
ClientSampleId :
BFFG4

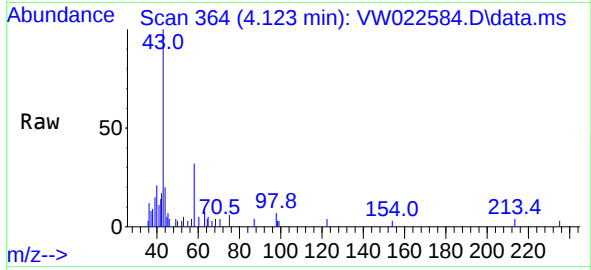

Tgt Ion: 43 Resp: 404
Ion Ratio Lower Upper
43 100
58 22.9 0.0 57.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/21/2022
Supervised By :Mahesh Dadoda 04/26/2022

