

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
 Data File : VW022585.D
 Acq On : 20 Apr 2022 13:35
 Operator : SY/VA
 Sample : N2469-05
 Misc : 3.30g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFG7

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/21/2022
 Supervised By : Mahesh Dadoda 04/26/2022

Quant Time: Apr 21 01:20:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 21 01:19:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	286146	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	214267	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	65447	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	81059	12.814	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	51.240%		
7) Chloroethane-d5	2.891	69	62872	15.859	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	63.440%		
11) 1,1-Dichloroethene-d2	4.019	63	90315	11.008	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	44.040%#		
21) 2-Butanone-d5	7.080	46	47840m	43.317	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	86.640%		
24) Chloroform-d	7.653	84	172260	19.260	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	77.040%		
26) 1,2-Dichloroethane-d4	8.305	65	103421m	20.238	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	80.960%		
32) Benzene-d6	8.275	84	296003	22.611	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	90.440%		
36) 1,2-Dichloropropane-d6	9.274	67	93990	24.810	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	99.240%		
41) Toluene-d8	10.323	98	229160	17.874	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	71.480%		
43) trans-1,3-Dichloroprop...	10.579	79	30707	17.175	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	68.720%		
47) 2-Hexanone-d5	10.927	63	35186	49.921	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	99.840%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	74999	23.283	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	93.120%		
66) 1,2-Dichlorobenzene-d4	13.853	152	43043	18.568	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	74.280%#		
Target Compounds					Qvalue	
13) Acetone	4.129	43	4542	6.040	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
Data File : VW022585.D
Acq On : 20 Apr 2022 13:35
Operator : SY/VA
Sample : N2469-05
Misc : 3.30g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BFFG7

Quant Time: Apr 21 01:20:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 21 01:19:16 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/21/2022
Supervised By :Mahesh Dadoda 04/26/2022

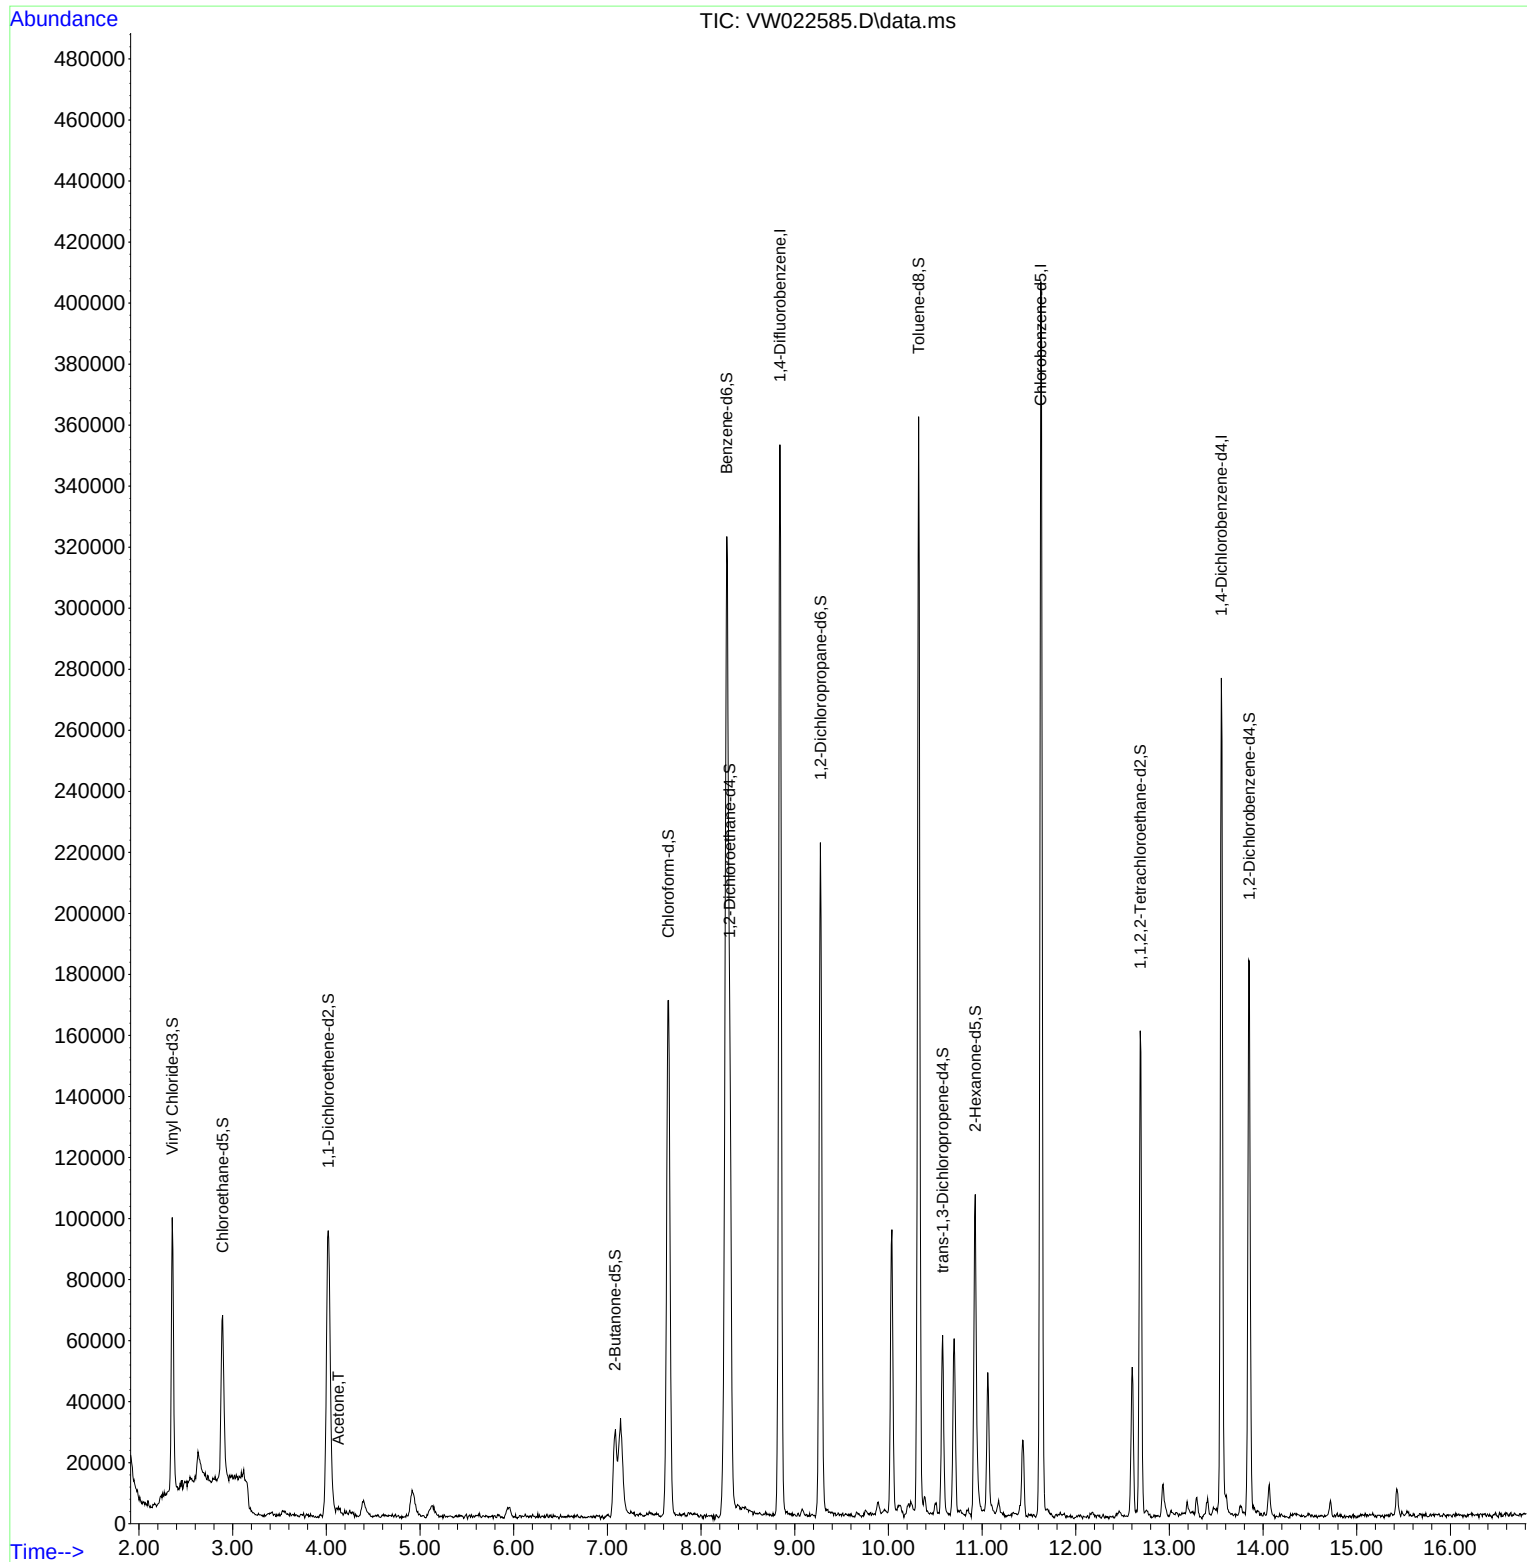

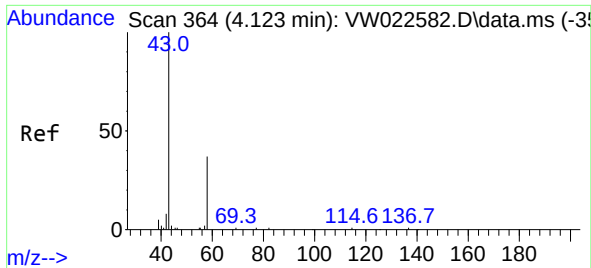

#13

Acetone

Concen: 6.040 ug/L

RT: 4.129 min Scan# 30

Delta R.T. 0.006 min

Lab File: VW022585.D


Acq: 20 Apr 2022 13:35

Instrument :

MSVOA_W

ClientSampleId :

BFFG7

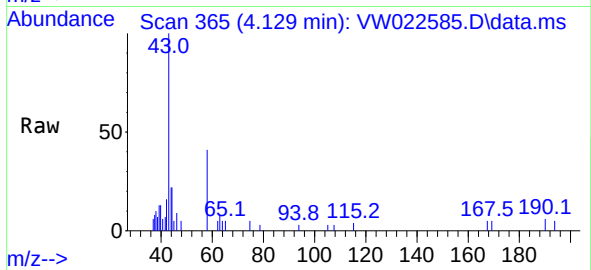

Tgt Ion: 43 Resp: 454

Ion Ratio Lower Upper

43 100

58 22.1 0.0 57.0

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 04/21/2022

Supervised By :Mahesh Dadoda 04/26/2022

