

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
 Data File : VW022591.D
 Acq On : 20 Apr 2022 16:00
 Operator : SY/VA
 Sample : VIBLK429
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK429

Quant Time: Apr 21 01:21:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 21 01:19:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	296896	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	287802	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	156450	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	151448	23.074	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.280%
7) Chloroethane-d5	2.885	69	96536	23.468	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.880%
11) 1,1-Dichloroethene-d2	4.019	63	160511	18.855	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.400%
21) 2-Butanone-d5	7.080	46	58252	50.835	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.680%
24) Chloroform-d	7.647	84	233911	25.206	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.840%
26) 1,2-Dichloroethane-d4	8.305	65	135539	25.563	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.240%
32) Benzene-d6	8.275	84	473928	26.953	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	107.800%
36) 1,2-Dichloropropane-d6	9.275	67	133325	26.201	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	104.800%
41) Toluene-d8	10.323	98	454315	26.381	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	105.520%
43) trans-1,3-Dichloroprop...	10.579	79	53737	22.377	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.520%
47) 2-Hexanone-d5	10.921	63	47295	49.956	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.920%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	114170	26.388	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.560%
66) 1,2-Dichlorobenzene-d4	13.847	152	145968	26.341	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.360%
Target Compounds					Qvalue	
13) Acetone	4.123	43	3747	4.803	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
Data File : VW022591.D
Acq On : 20 Apr 2022 16:00
Operator : SY/VA
Sample : VIBLK429
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK429

Quant Time: Apr 21 01:21:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 21 01:19:16 2022
Response via : Initial Calibration

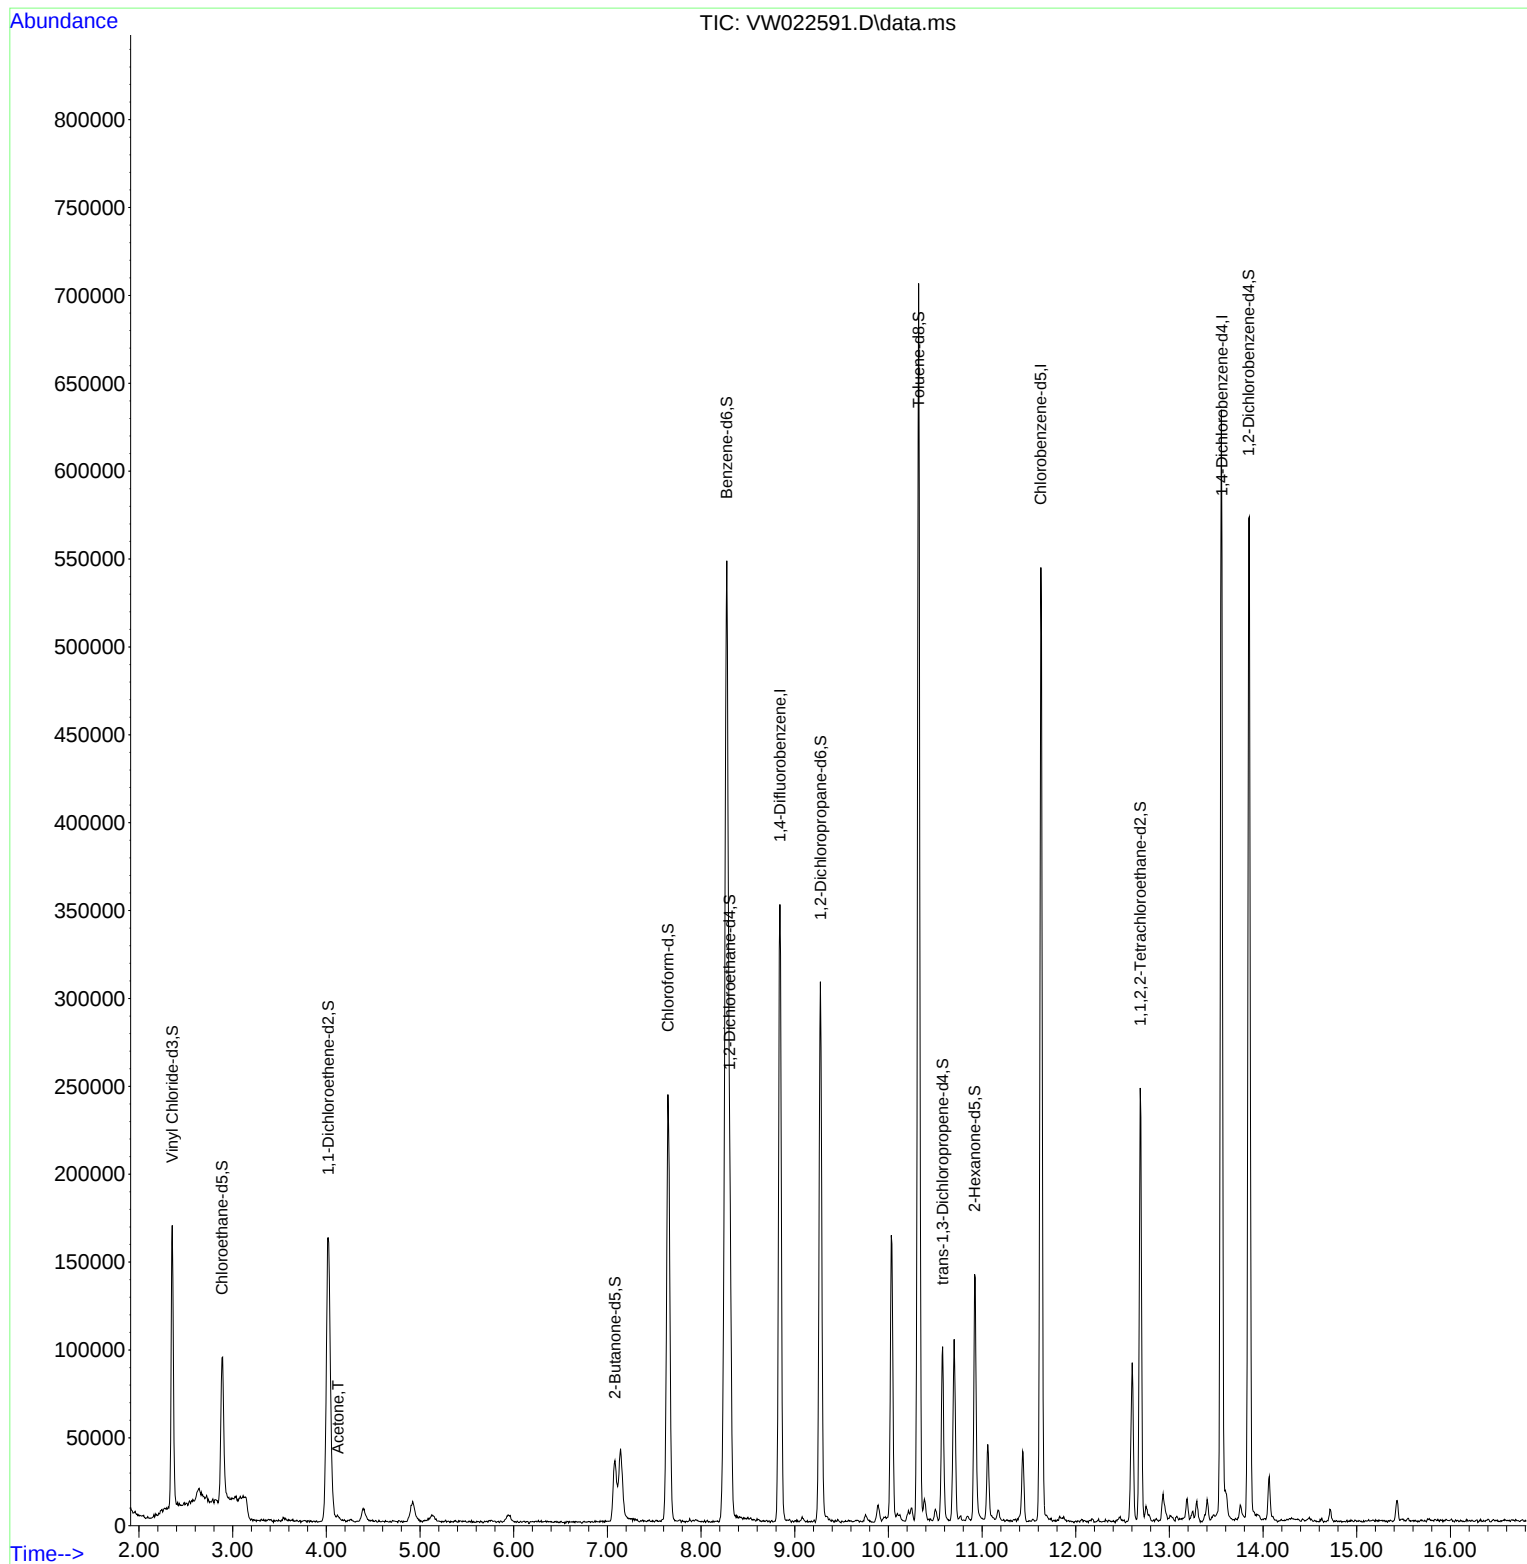

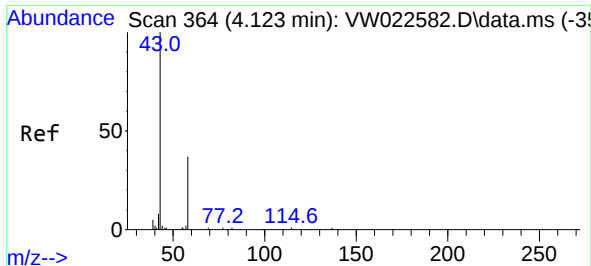

#13
 Acetone
 Concen: 4.803 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW022591.D
 Acq: 20 Apr 2022 16:00

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK429

Tgt Ion: 43 Resp: 3747
 Ion Ratio Lower Upper
 43 100
 58 22.7 0.0 57.0

