

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
 Data File : VW022593.D
 Acq On : 20 Apr 2022 16:48
 Operator : SY/VA
 Sample : N2469-05RE
 Misc : 3.44g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFG7RE

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/21/2022
 Supervised By :Mahesh Dadoda 04/26/2022

Quant Time: Apr 21 01:21:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 21 01:19:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	292443	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	231581	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	77046	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	91147	14.098	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	56.400%		
7) Chloroethane-d5	2.885	69	70139	17.311	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	69.240%		
11) 1,1-Dichloroethene-d2	4.019	63	97530	11.631	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	46.520%		
21) 2-Butanone-d5	7.080	46	56830	50.350	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	100.700%		
24) Chloroform-d	7.647	84	194673	21.297	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	85.200%		
26) 1,2-Dichloroethane-d4	8.305	65	115464m	22.108	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	88.440%		
32) Benzene-d6	8.275	84	331858	23.455	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	93.840%		
36) 1,2-Dichloropropane-d6	9.274	67	104510	25.525	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	102.080%		
41) Toluene-d8	10.323	98	262997	18.979	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	75.920%		
43) trans-1,3-Dichloroprop...	10.579	79	33277	17.221	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	68.880%		
47) 2-Hexanone-d5	10.927	63	42876	56.283	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	112.560%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	87442	25.116	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	100.480%		
66) 1,2-Dichlorobenzene-d4	13.847	152	56308	20.633	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	82.520%		
Target Compounds					Qvalue	
13) Acetone	4.123	43	9673	12.587	ug/L	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042022\
Data File : VW022593.D
Acq On : 20 Apr 2022 16:48
Operator : SY/VA
Sample : N2469-05RE
Misc : 3.44g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BFFG7RE

Quant Time: Apr 21 01:21:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 21 01:19:16 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/21/2022
Supervised By :Mahesh Dadoda 04/26/2022

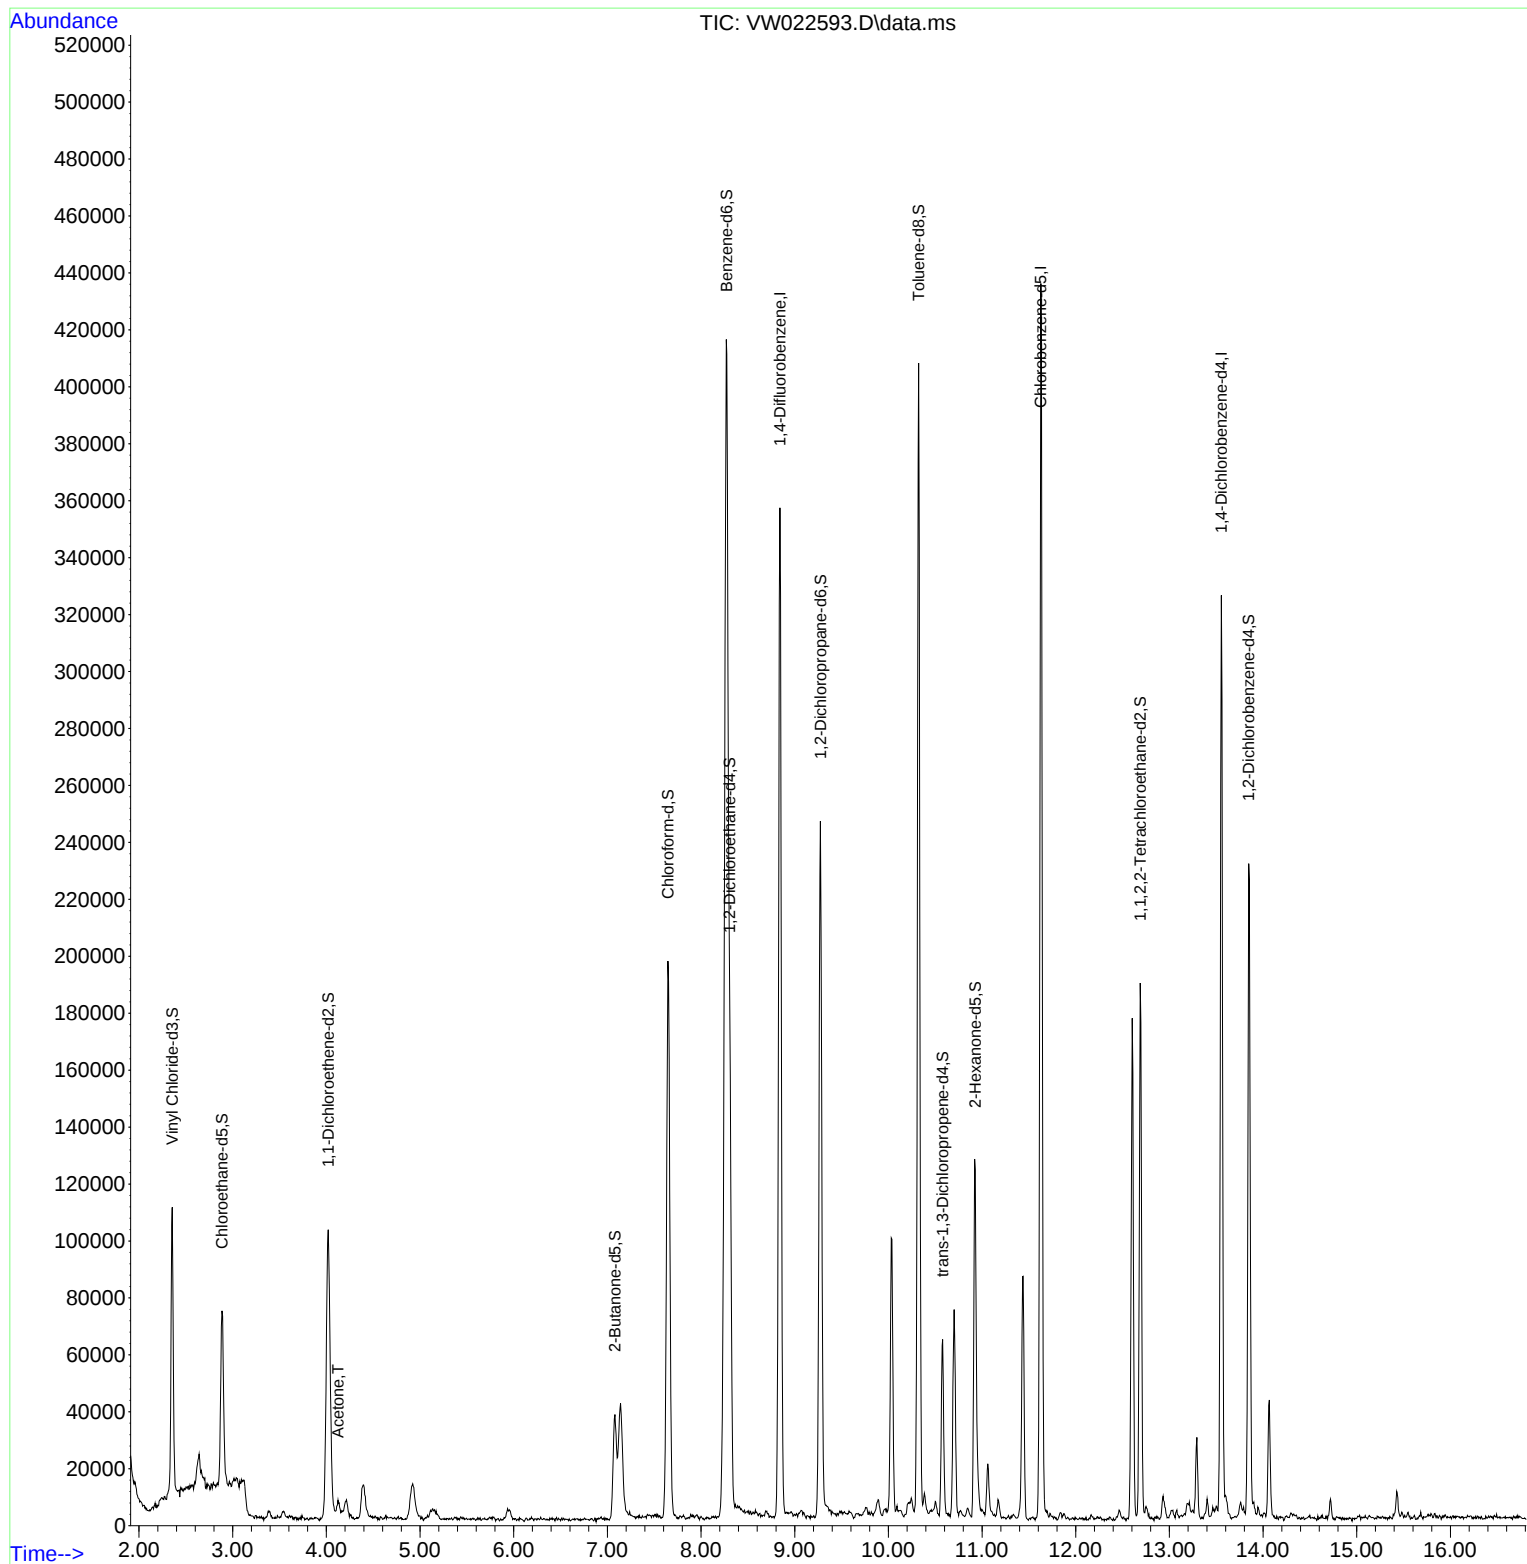

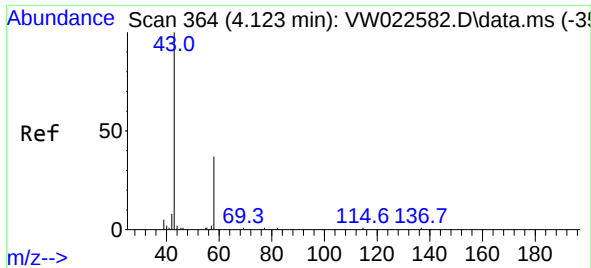

#13
Acetone
Concen: 12.587 ug/L
RT: 4.123 min Scan# 30
Delta R.T. -0.000 min
Lab File: VW022593.D
Acq: 20 Apr 2022 16:48

Instrument :
MSVOA_W
ClientSampleId :
BFFG7RE

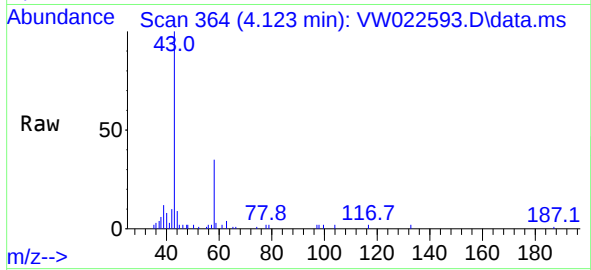

Tgt Ion: 43 Resp: 967
Ion Ratio Lower Upper
43 100
58 35.8 0.0 57.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/21/2022
Supervised By :Mahesh Dadoda 04/26/2022

