

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042023\
 Data File : VW025595.D
 Acq On : 20 Apr 2023 10:53
 Operator : SY/MD
 Sample : VW0420SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK483

Quant Time: Apr 21 01:47:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 21 01:47:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	687117	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	601474	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	269051	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	195944	17.524	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.080%
7) Chloroethane-d5	2.899	69	154063	19.353	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.400%
11) 1,1-Dichloroethene-d2	4.253	63	147	0.007	ug/L	0.23
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.040%#
21) 2-Butanone-d5	7.075	46	137166	54.989	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.980%
24) Chloroform-d	7.807	84	160	0.008	ug/L	0.16
Spiked Amount	25.000	Range	40 - 150	Recovery	=	0.040%#
26) 1,2-Dichloroethane-d4	8.471	65	152	0.015	ug/L	0.16
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.080%#
32) Benzene-d6	8.276	84	862832	22.154	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.600%
36) 1,2-Dichloropropane-d6	9.270	67	276694	22.785	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.160%
41) Toluene-d8	10.325	98	742928	21.838	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.360%
43) trans-1,3-Dichloroprop...	10.575	79	101278	22.245	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.000%
47) 2-Hexanone-d5	10.922	63	88324	53.212	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.420%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	209402	25.548	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.200%
66) 1,2-Dichlorobenzene-d4	13.848	152	231658	25.063	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.240%
Target Compounds						Qvalue
16) Methylene chloride	4.923	84	26358	2.413	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042023\
Data File : VW025595.D
Acq On : 20 Apr 2023 10:53
Operator : SY/MD
Sample : VW0420SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK483

Quant Time: Apr 21 01:47:49 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 21 01:47:12 2023
Response via : Initial Calibration

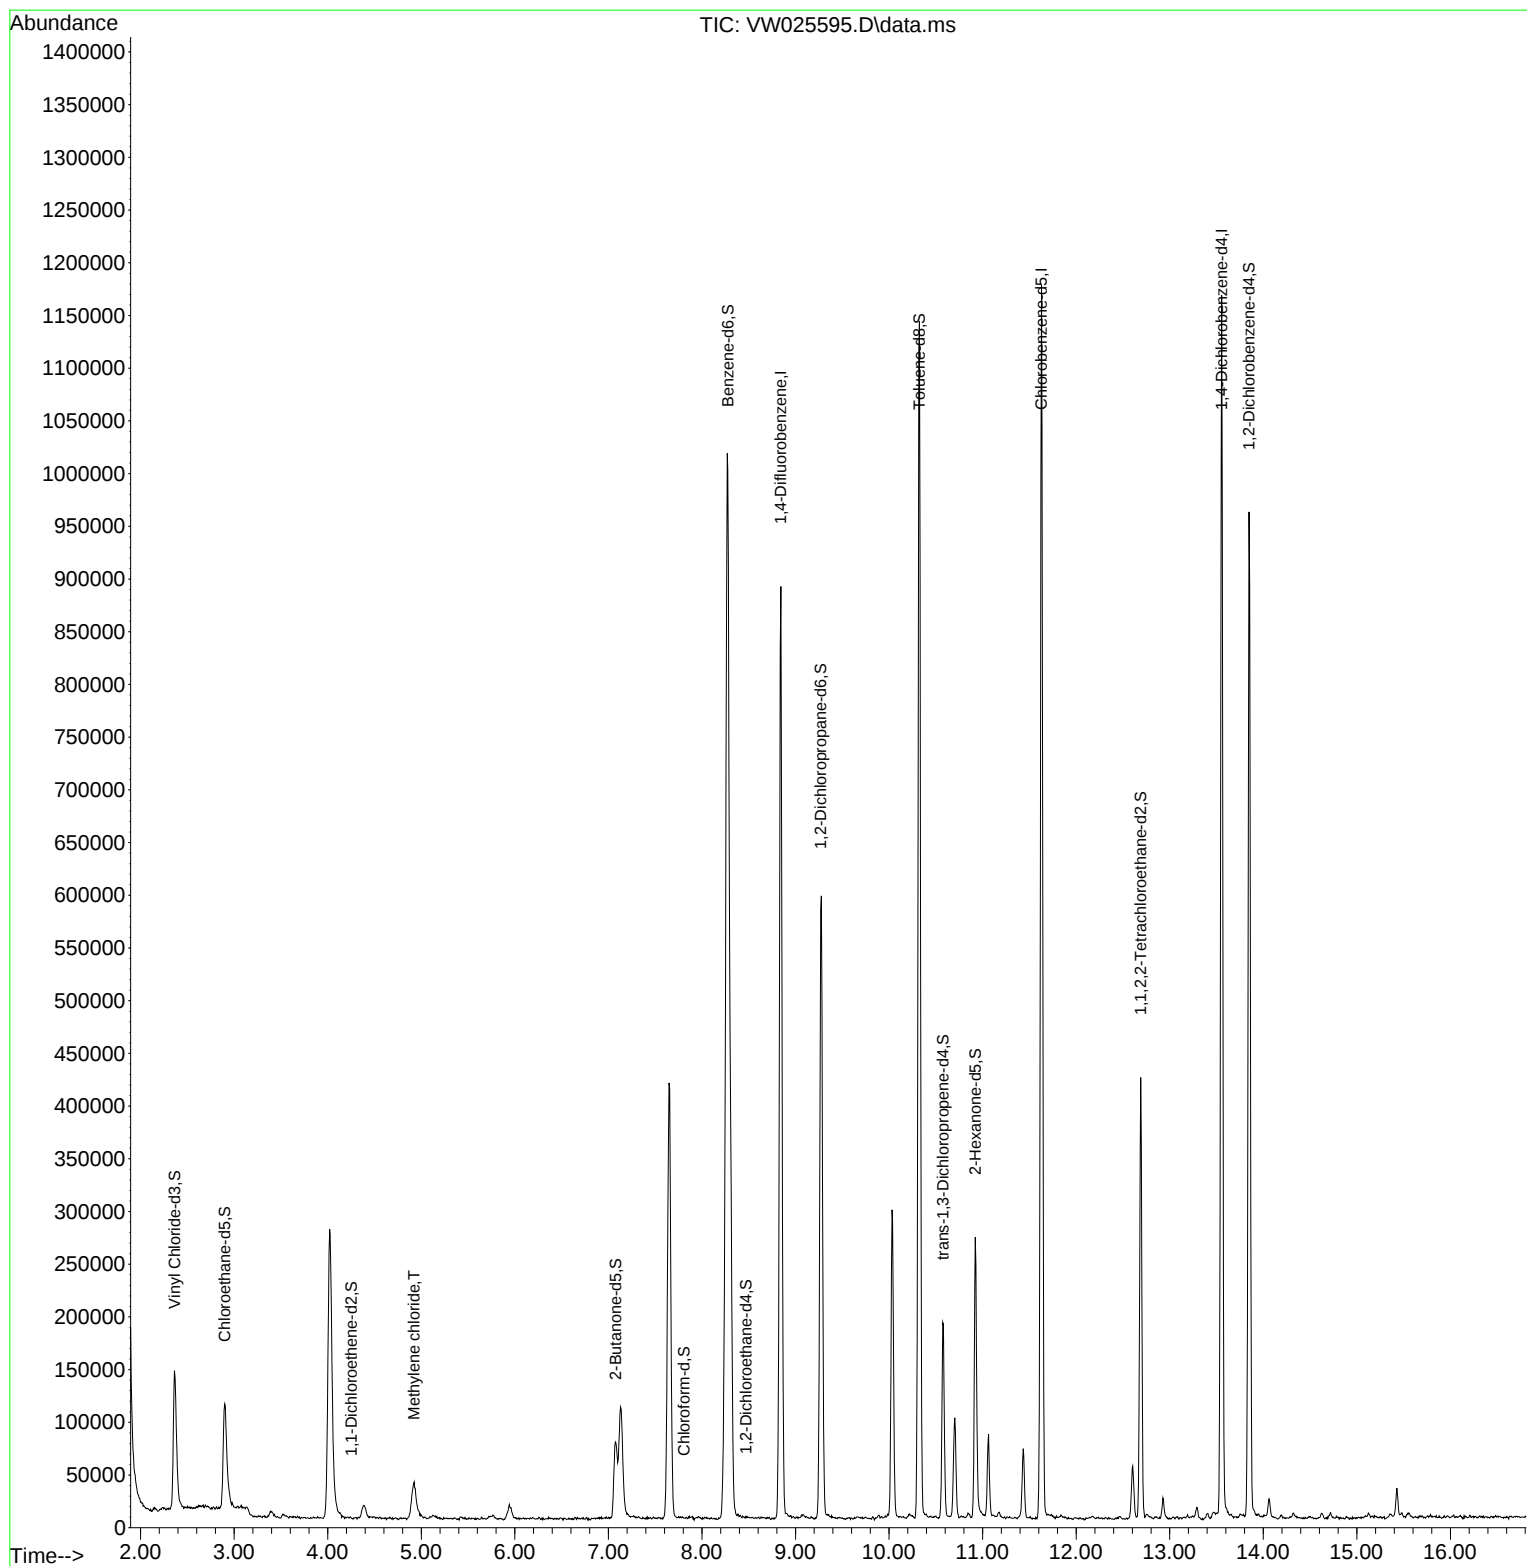

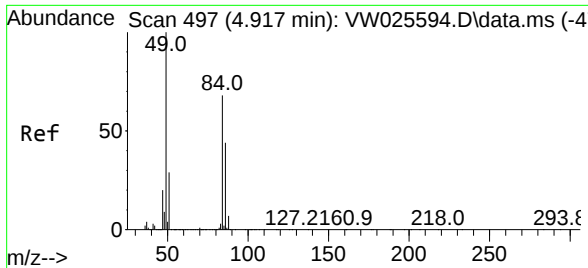

#16
Methylene chloride
Concen: 2.413 ug/L
RT: 4.923 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW025595.D
Acq: 20 Apr 2023 10:53

Instrument :
MSVOA_W
ClientSampleId :
VBLK483

Tgt Ion:	84	Resp:	26358
Ion	Ratio	Lower	Upper
84	100		
86	62.1	44.9	83.3
49	139.9	101.4	188.4

