

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042023\
 Data File : VW025601.D
 Acq On : 20 Apr 2023 13:17
 Operator : SY/MD
 Sample : 02418-13RE
 Misc : 5.48g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 EW8Z7RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/21/2023
 Supervised By :Mahesh Dadoda 04/22/2023

04/21/2023
 Supervised By :Mahesh
 Dadoda

Quant Time: Apr 21 01:49:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 21 01:47:12 2023
 Response via : Initial Calibration

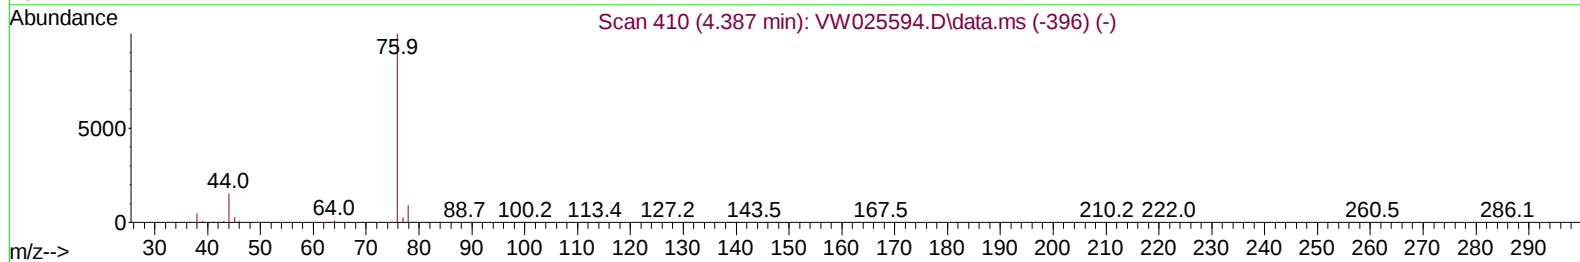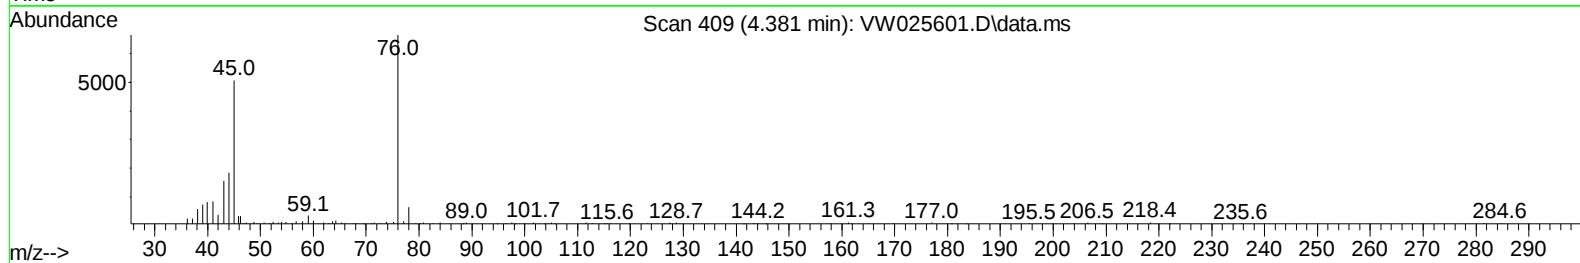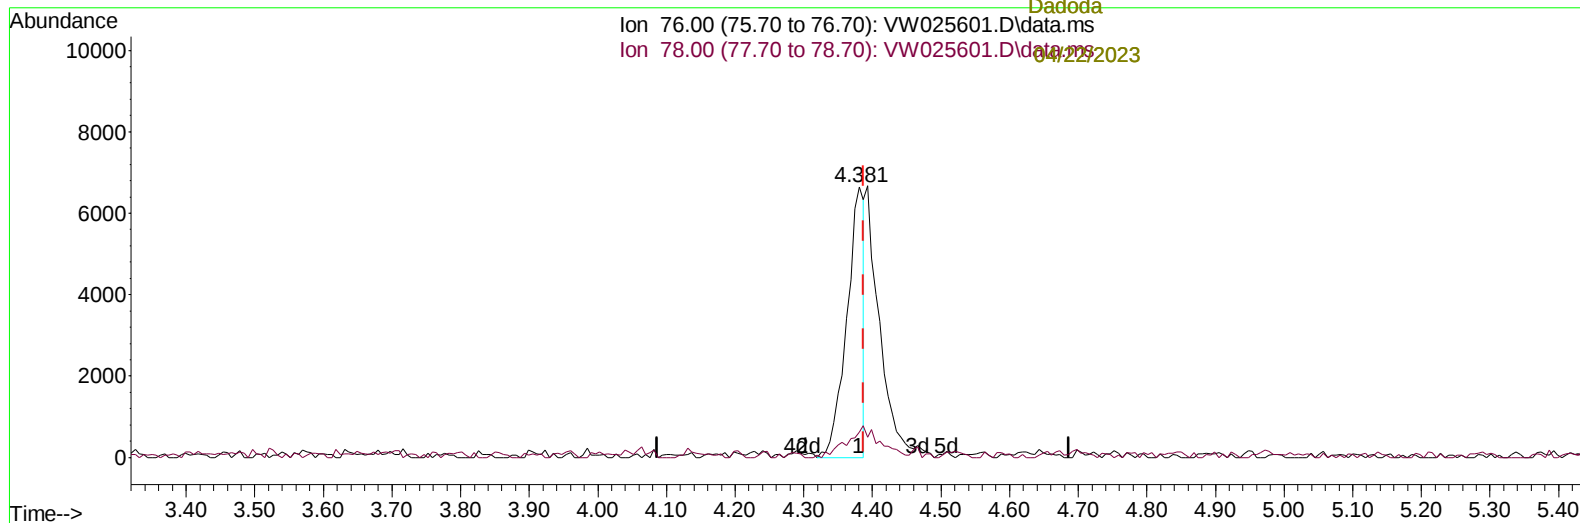

TIC: VW025601.D\data.ms

(14) Carbon disulfide (T)

4.381min (-0.006) 0.37 ug/L

response 11697

Ion	Exp%	Act%
76.00	100.00	100.00
78.00	8.90	9.35
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042023\
 Data File : VW025601.D
 Acq On : 20 Apr 2023 13:17
 Operator : SY/MD
 Sample : 02418-13RE
 Misc : 5.48g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 EW8Z7RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/21/2023
 Supervised By :Mahesh Dadoda 04/22/2023

04/21/2023
 Supervised By :Mahesh
 Dadoda

Quant Time: Apr 21 01:49:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 21 01:47:12 2023
 Response via : Initial Calibration

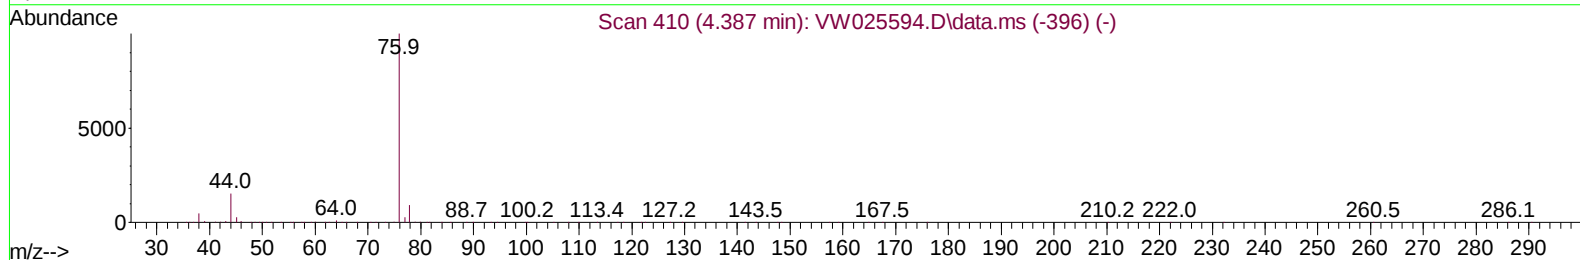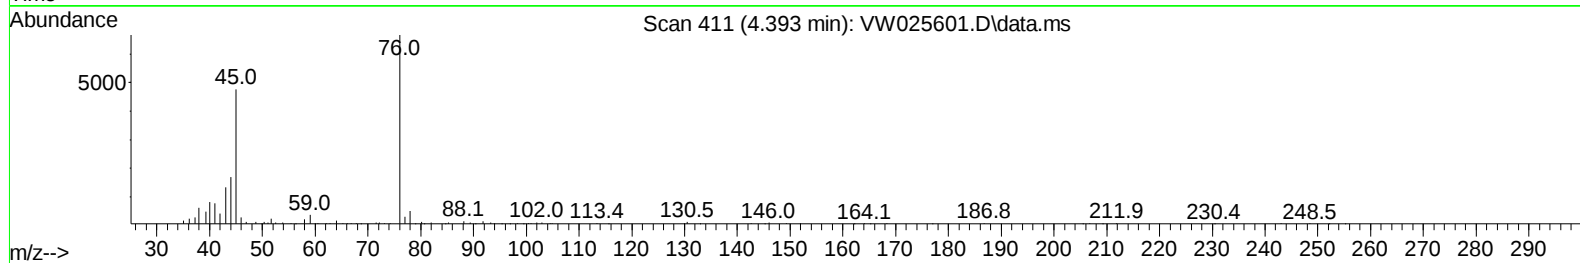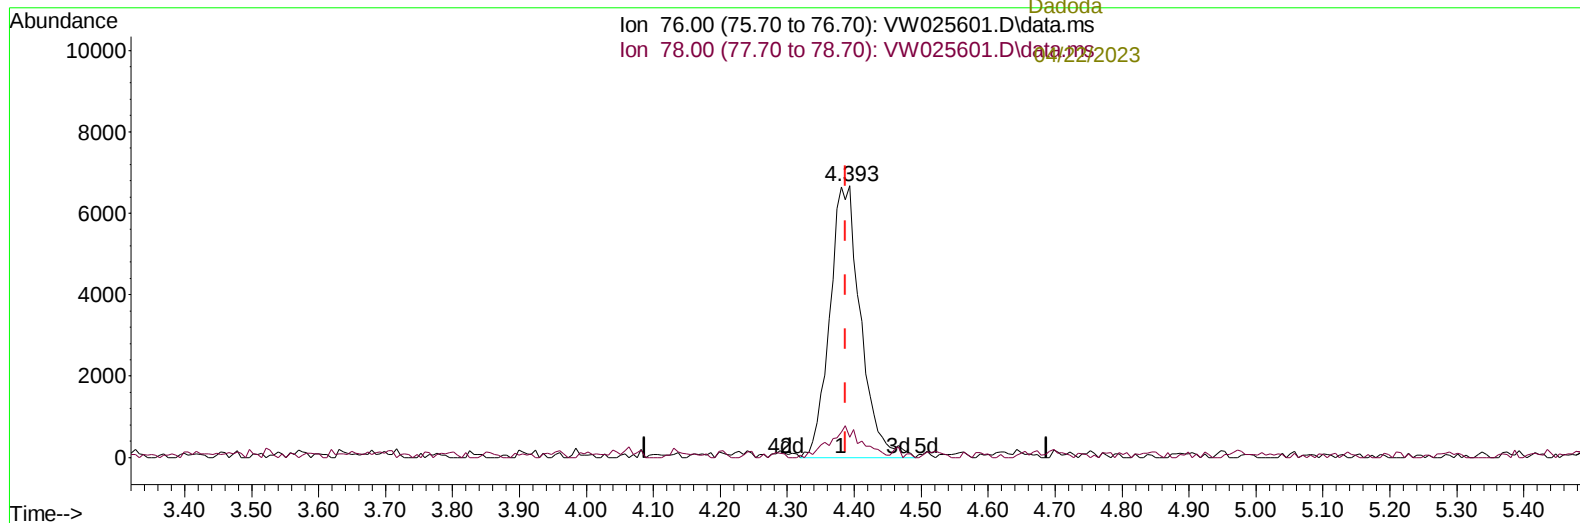

TIC: VW025601.D\data.ms

(14) Carbon disulfide (T)

4.393min (+ 0.006) 0.67 ug/L m

response 21268

Ion	Exp%	Act%
76.00	100.00	100.00
78.00	8.90	7.51
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042023\
 Data File : VW025601.D
 Acq On : 20 Apr 2023 13:17
 Operator : SY/MD
 Sample : 02418-13RE
 Misc : 5.48g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 EW8Z7RE

Manual IntegrationsAPPROVED

Quant Time: Apr 21 01:49:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 21 01:47:12 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/21/2023
 Supervised By :Mahesh Dadoda 04/22/2023

04/21/2023
 Supervised By :Mahesh
 Dadoda

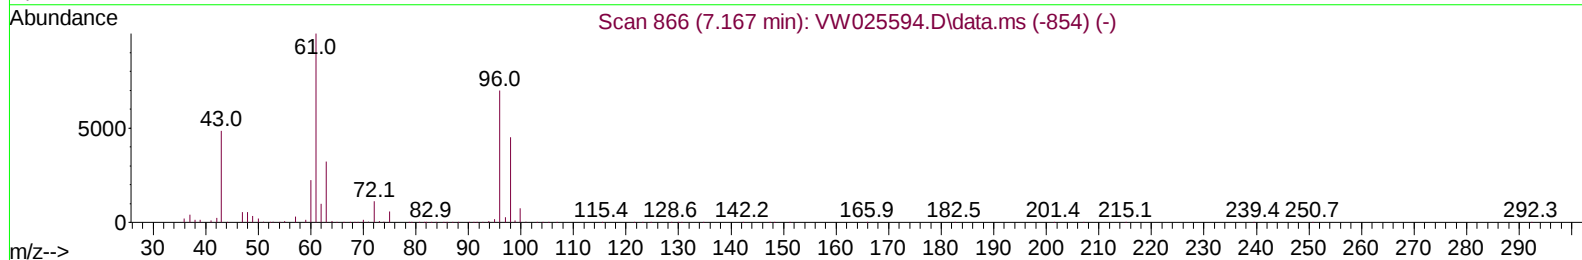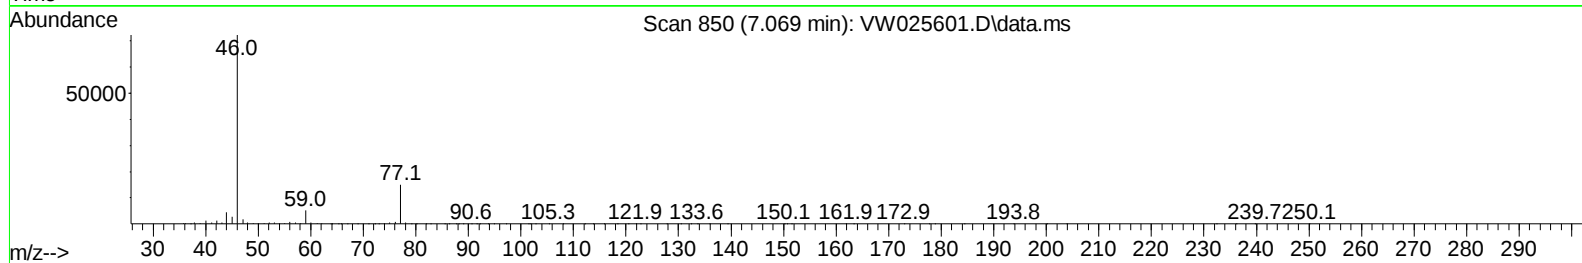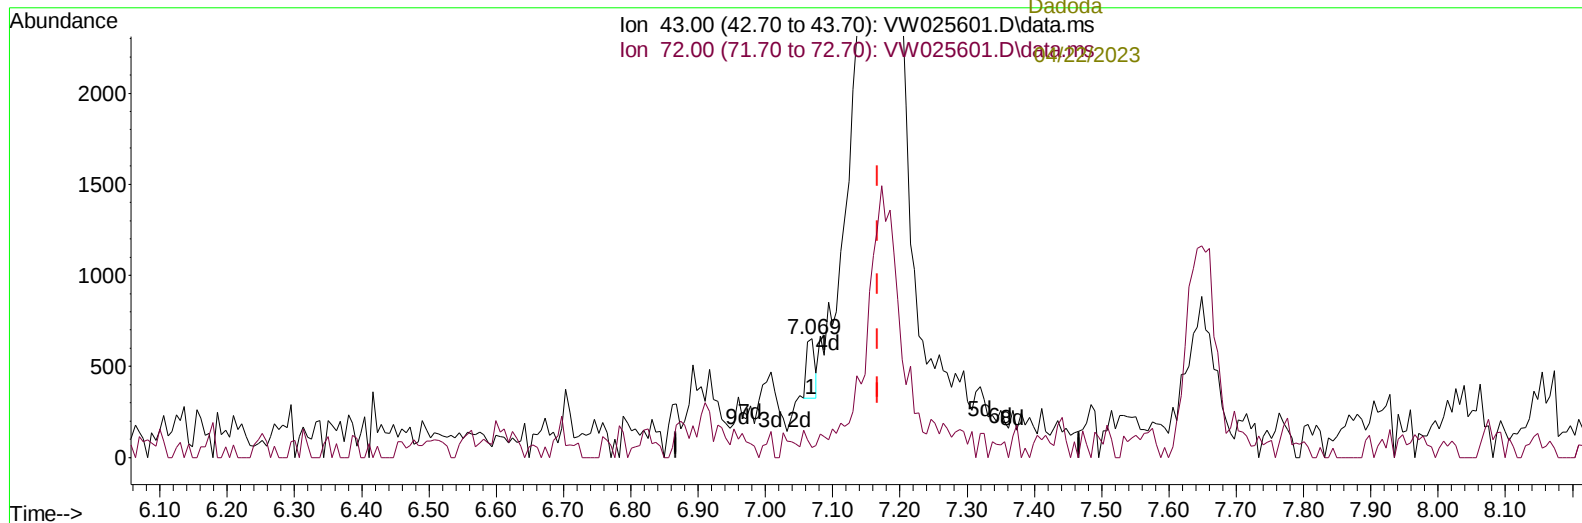

TIC: VW025601.D\data.ms

(22) 2-Butanone (T)

7.069min (-0.097) 0.10 ug/L

response	285	
Ion	Exp%	Act%
43.00	100.00	100.00
72.00	24.00	23.51
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042023\
 Data File : VW025601.D
 Acq On : 20 Apr 2023 13:17
 Operator : SY/MD
 Sample : 02418-13RE
 Misc : 5.48g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 EW8Z7RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/21/2023
 Supervised By :Mahesh Dadoda 04/22/2023

04/21/2023
 Supervised By :Mahesh
 Dadoda

Quant Time: Apr 21 01:49:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 21 01:47:12 2023
 Response via : Initial Calibration

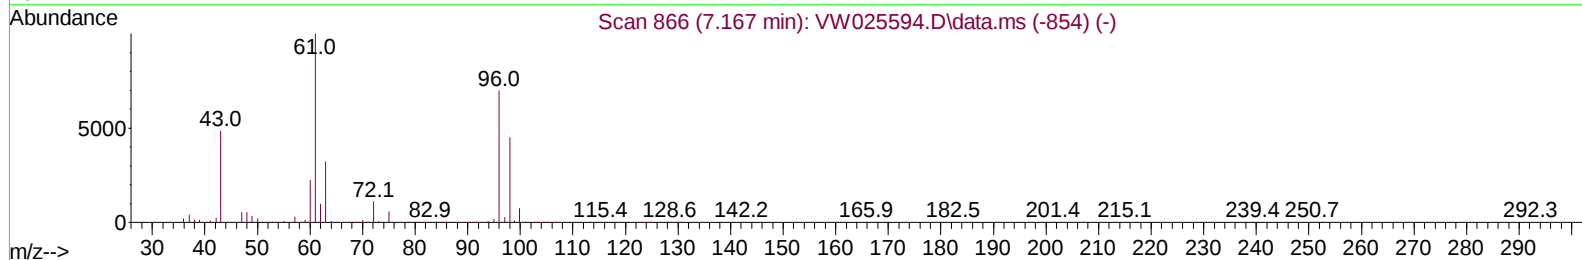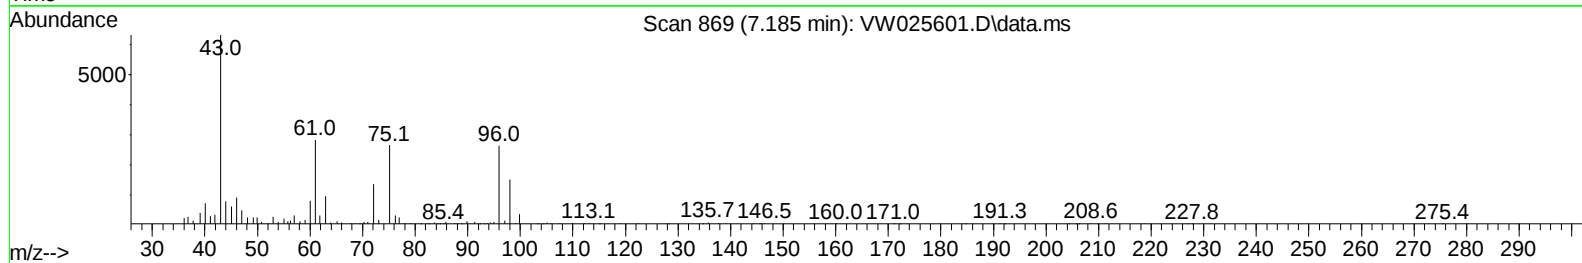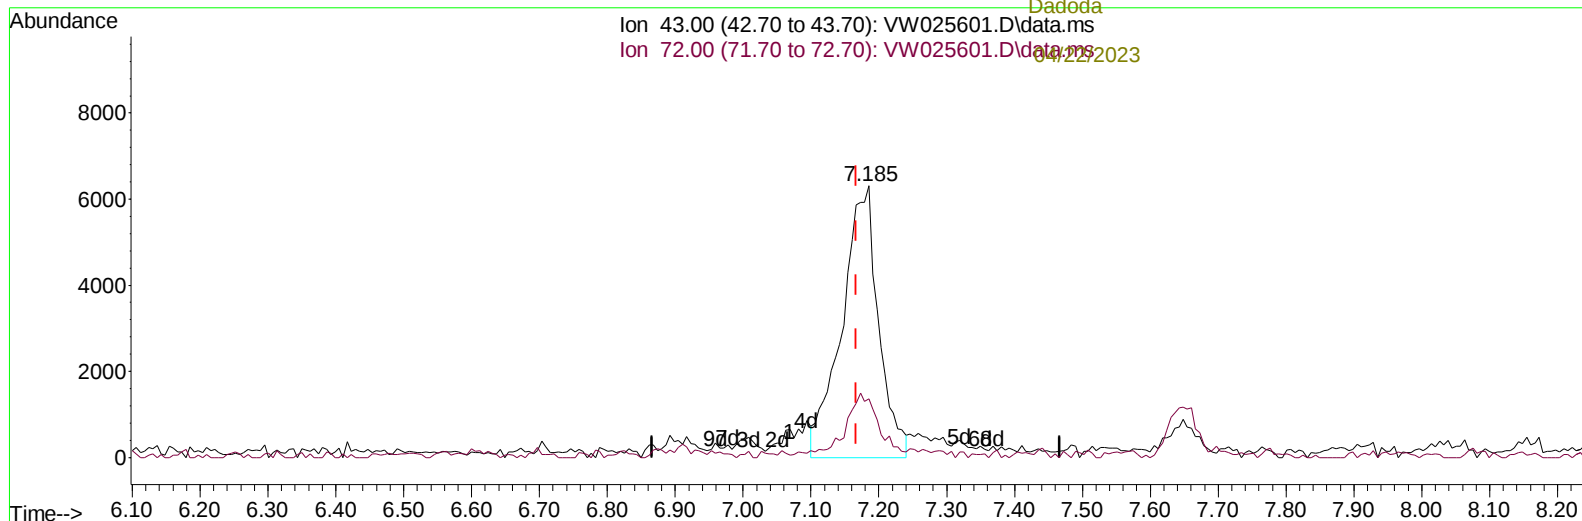

TIC: VW025601.D\data.ms

(22) 2-Butanone (T)

7.185min (+ 0.018) 8.36 ug/L m

response 23545

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	24.00	0.28#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042023\
 Data File : VW025601.D
 Acq On : 20 Apr 2023 13:17
 Operator : SY/MD
 Sample : 02418-13RE
 Misc : 5.48g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8Z7RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/21/2023
 Supervised By :Mahesh Dadoda 04/22/2023

Quant Time: Apr 21 01:49:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 21 01:47:12 2023
 Response via : Initial Calibration

04/21/2023
 Supervised By :Mahesh
 Dadoda

04/22/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----04/22/2023						
Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	644544	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	349592	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	63537	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	199654	19.035	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	76.160%	
7) Chloroethane-d5	2.893	69	181076	24.248	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	97.000%	
11) 1,1-Dichloroethene-d2	4.021	63	328081	15.467	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	61.880%	
21) 2-Butanone-d5	7.075	46	206062	88.066	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	176.140%#	
24) Chloroform-d	7.648	84	489790	27.064	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	108.240%	
26) 1,2-Dichloroethane-d4	8.301	65	270014	28.679	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	114.720%	
32) Benzene-d6	8.276	84	932261	41.184	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	164.720%#	
36) 1,2-Dichloropropane-d6	9.270	67	333550	47.258	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	189.040%#	
41) Toluene-d8	10.325	98	631408	31.932	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	127.720%	
43) trans-1,3-Dichloroprop...	10.575	79	69371	26.215	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	104.880%	
47) 2-Hexanone-d5	10.922	63	106513	110.405	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	220.820%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	226576	47.561	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	190.240%#	
66) 1,2-Dichlorobenzene-d4	13.855	152	78147	35.801	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	143.200%#	
Target Compounds						
					Qvalue	
13) Acetone	4.118	43	64076	32.356	ug/L	98
14) Carbon disulfide	4.393	76	21268m	0.674	ug/L	
16) Methylene chloride	4.917	84	32208	3.144	ug/L	99
20) cis-1,2-Dichloroethene	7.173	96	8729	0.882	ug/L #	93
22) 2-Butanone	7.185	43	23545m	8.363	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042023\
Data File : VW025601.D
Acq On : 20 Apr 2023 13:17
Operator : SY/MD
Sample : 02418-13RE
Misc : 5.48g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW8Z7RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/21/2023
Supervised By :Mahesh Dadoda 04/22/2023

04/21/2023
Supervised By :Mahesh
Dadoda

04/22/2023

