

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042023\
 Data File : VW025605.D
 Acq On : 20 Apr 2023 14:52
 Operator : SY/MD
 Sample : 02418-14
 Misc : 4.64g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8Z8

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/21/2023
 Supervised By : Mahesh Dadoda 04/22/2023

Quant Time: Apr 21 01:50:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 21 01:47:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	682852	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	472016	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	120695	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	200318	18.027	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	72.120%		
7) Chloroethane-d5	2.899	69	185036	23.389	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	93.560%		
11) 1,1-Dichloroethene-d2	4.027	63	345292m	15.366	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	61.480%		
21) 2-Butanone-d5	7.075	46	130149	52.502	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	105.000%		
24) Chloroform-d	7.648	84	513497	26.783	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	107.120%		
26) 1,2-Dichloroethane-d4	8.307	65	291726	29.247	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	117.000%		
32) Benzene-d6	8.276	84	956033	31.280	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	125.120%		
36) 1,2-Dichloropropane-d6	9.276	67	336654	35.326	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	141.320%#		
41) Toluene-d8	10.325	98	724541	27.138	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	108.560%		
43) trans-1,3-Dichloroprop...	10.575	79	92324	25.840	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	103.360%		
47) 2-Hexanone-d5	10.922	63	82032	62.976	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	125.960%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	223881	34.806	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	139.240%#		
66) 1,2-Dichlorobenzene-d4	13.848	152	118115	28.486	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	113.960%		
Target Compounds					Qvalue	
13) Acetone	4.125	43	7879	3.755	ug/L	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042023\
Data File : VW025605.D
Acq On : 20 Apr 2023 14:52
Operator : SY/MD
Sample : 02418-14
Misc : 4.64g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW8Z8

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 04/21/2023
Supervised By : Mahesh Dadoda 04/22/2023


Quant Time: Apr 21 01:50:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 21 01:47:12 2023
Response via : Initial Calibration

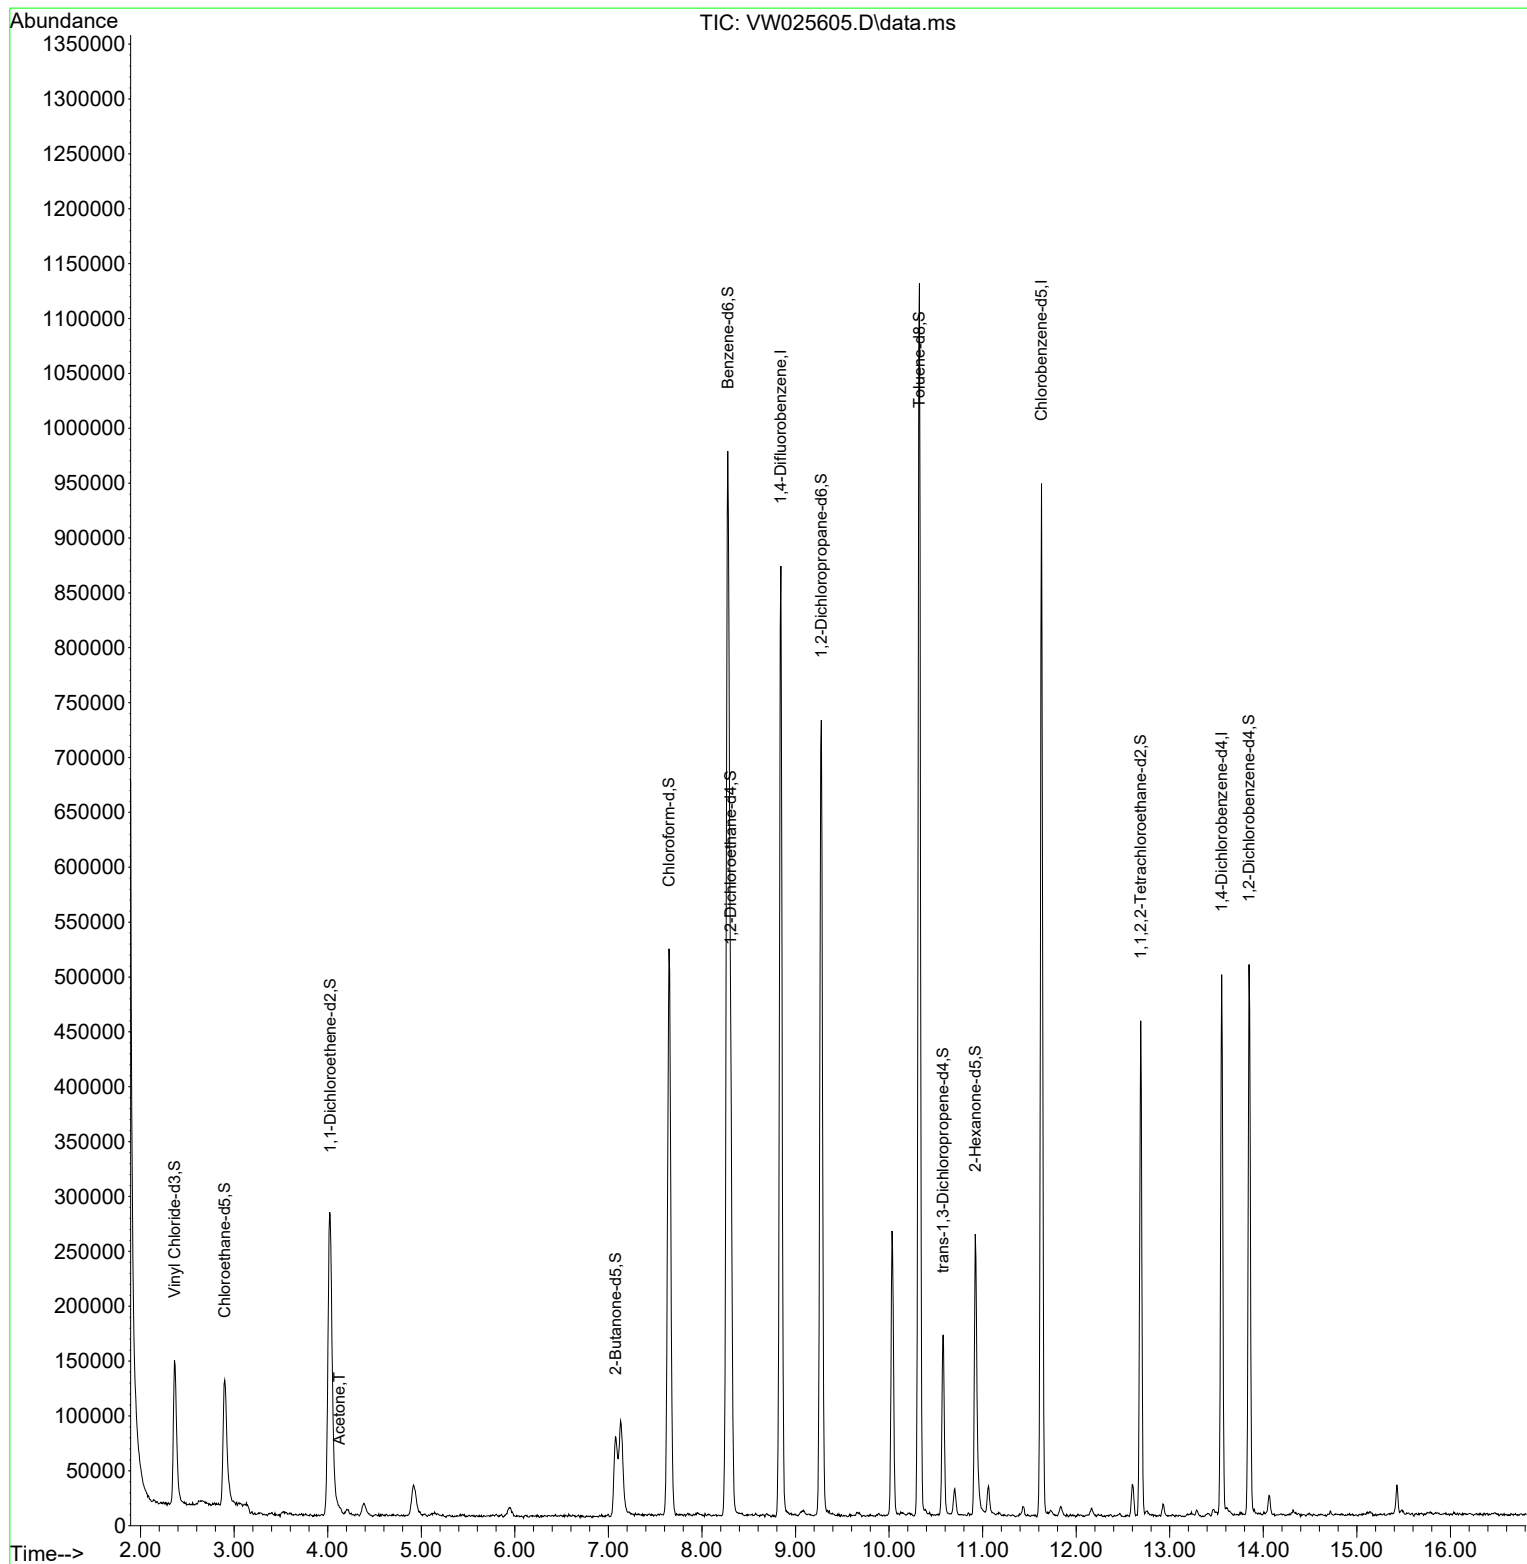

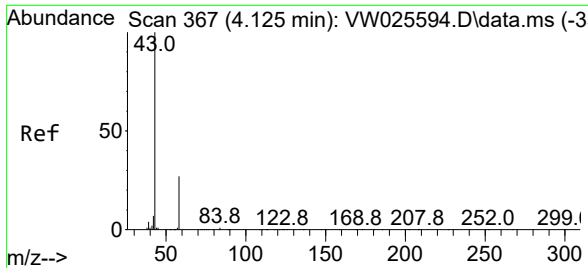

#13
 Acetone
 Concen: 3.755 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW025605.D
 Acq: 20 Apr 2023 14:52

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8Z8

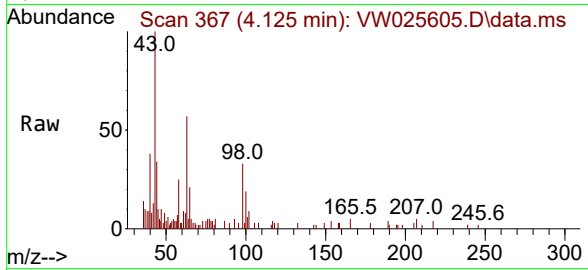

Tgt Ion: 43 Resp: 7879
 Ion Ratio Lower Upper
 43 100
 58 13.8 0.0 57.4

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/21/2023
 Supervised By :Mahesh Dadoda 04/22/2023

