

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042319\
Quantitation Report (QT Reviewed)


Data File : VW010098.D
Acq On : 23 Apr 2019 14:36
Operator : SY/VA
Sample : K2456-16
Misc : 5.03G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAHN6

Manual Integrations
APPROVED

MMDadoda
4/25/2019 9:22:08 AM

Quant Time: Apr 24 04:38:05 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM041519S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 24 03:51:20 2019
Response via : Initial Calibration

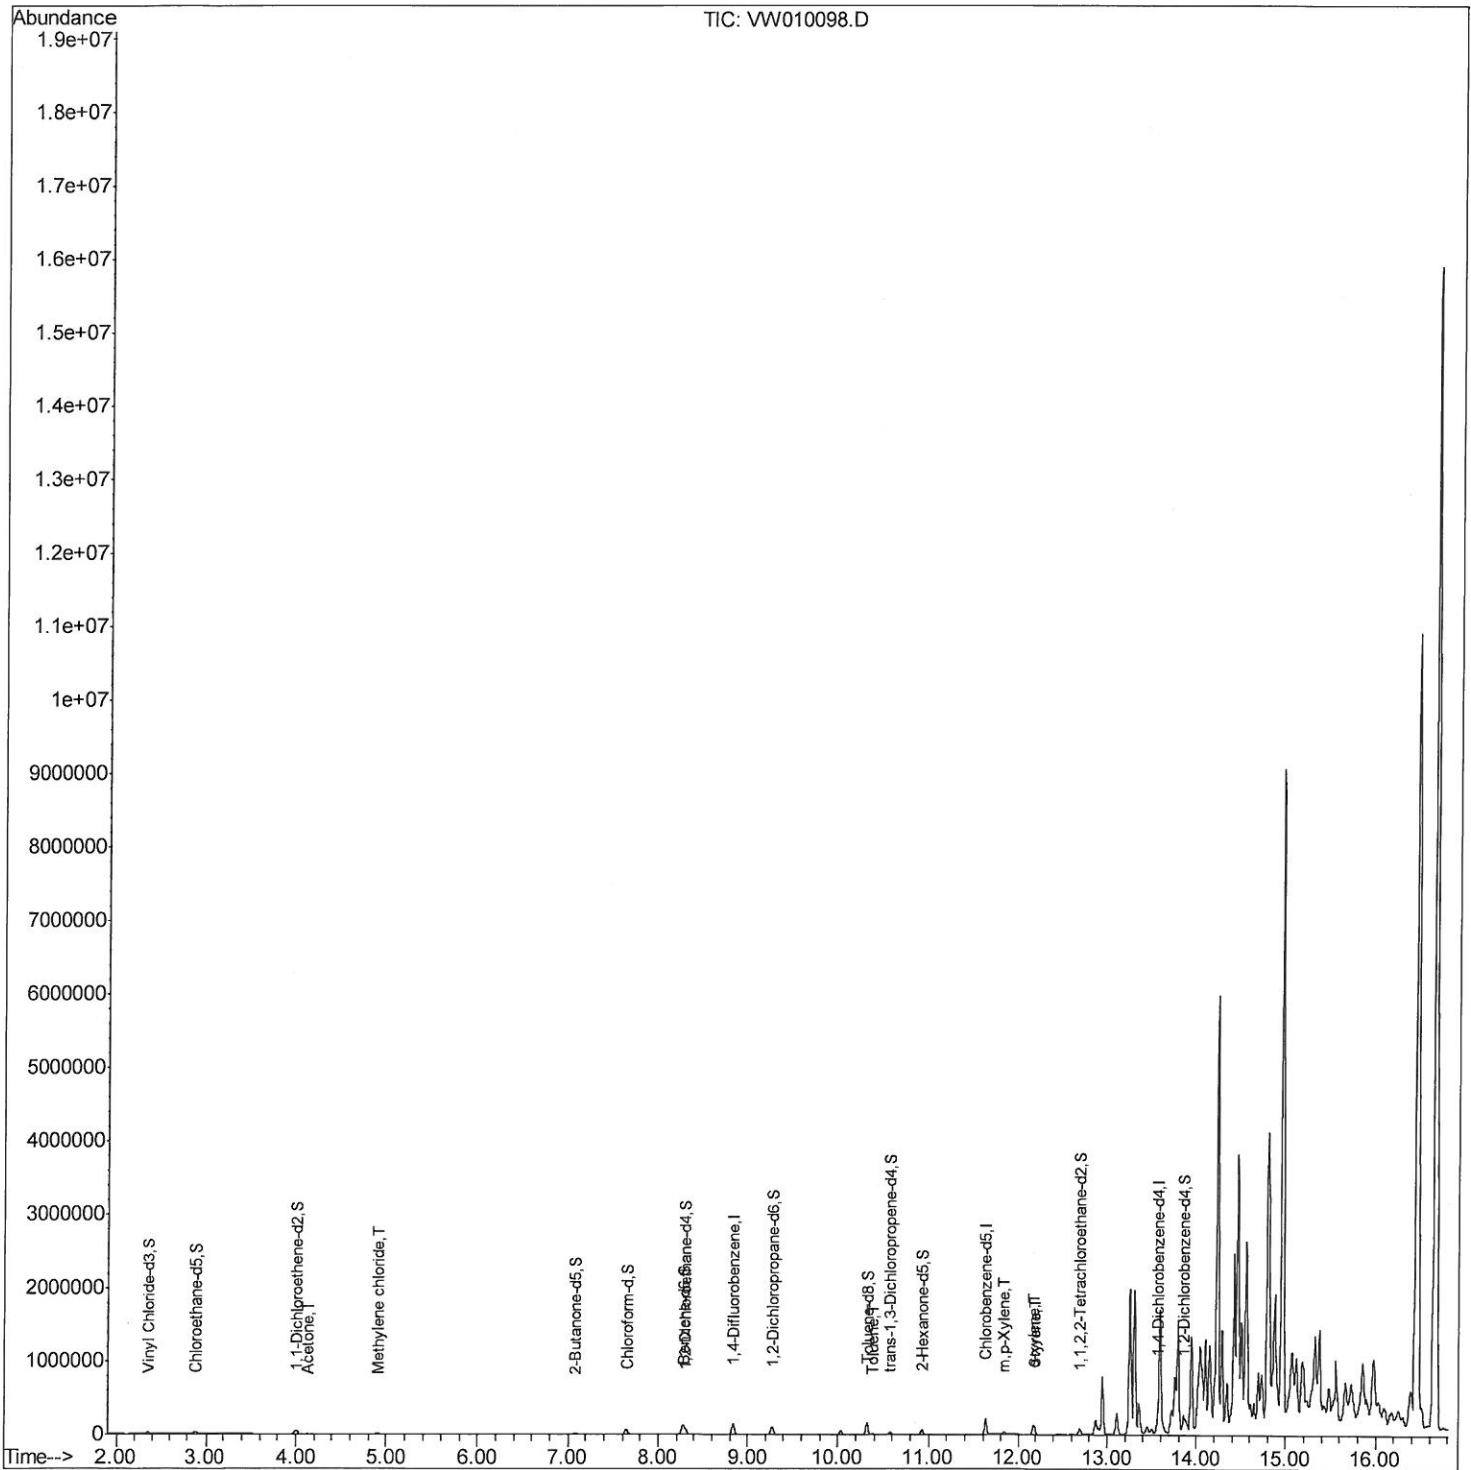

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042319\
Quantitation Report (Qedit)




Data File : VW010098.D
Acq On : 23 Apr 2019 14:36
Operator : SY/VA
Sample : K2456-16
Misc : 5.03G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAHN6

Manual Integrations
APPROVED

MMDadoda
4/25/2019 9:22:08 AM

Quant Time: Apr 24 04:37:41 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM041519S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 24 03:51:20 2019
Response via : Initial Calibration

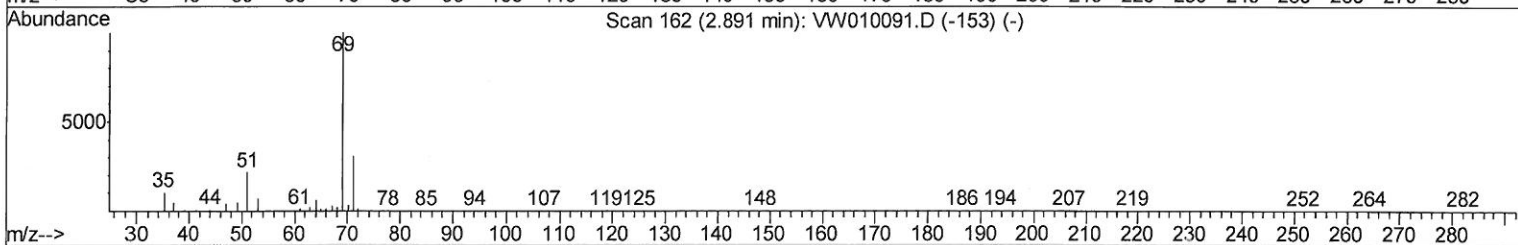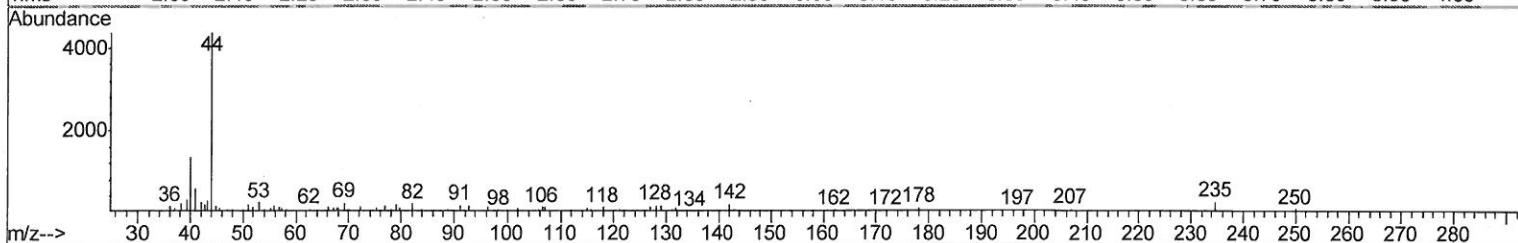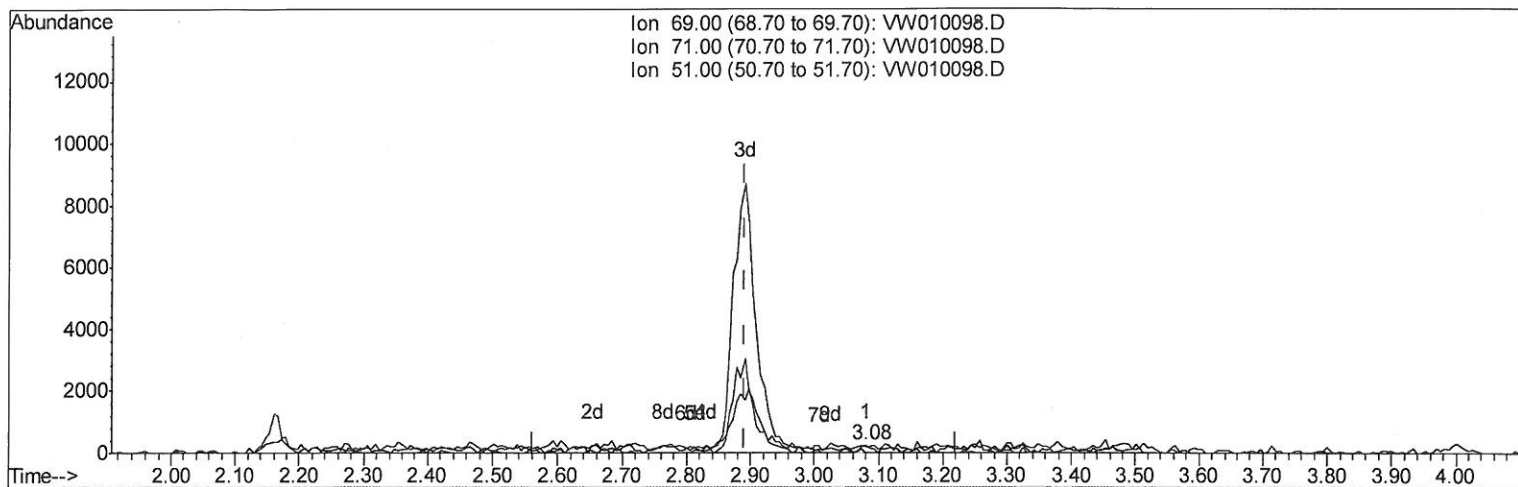

TIC: VW010098.D

(7) Chloroethane-d5 (S)
3.081min (+0.189) 0.25ug/L
response 281

Ion	Exp%	Act%
69.00	100	100
71.00	32.70	26.33
51.00	29.10	41.28
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042319\
Quantitation Report (Qedit)




Data File : VW010098.D
Acq On : 23 Apr 2019 14:36
Operator : SY/VA
Sample : K2456-16
Misc : 5.03G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAHN6

Manual Integrations
APPROVED

MMDadoda
4/25/2019 9:22:08 AM

Quant Time: Apr 24 04:37:41 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM041519S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 24 03:51:20 2019
Response via : Initial Calibration

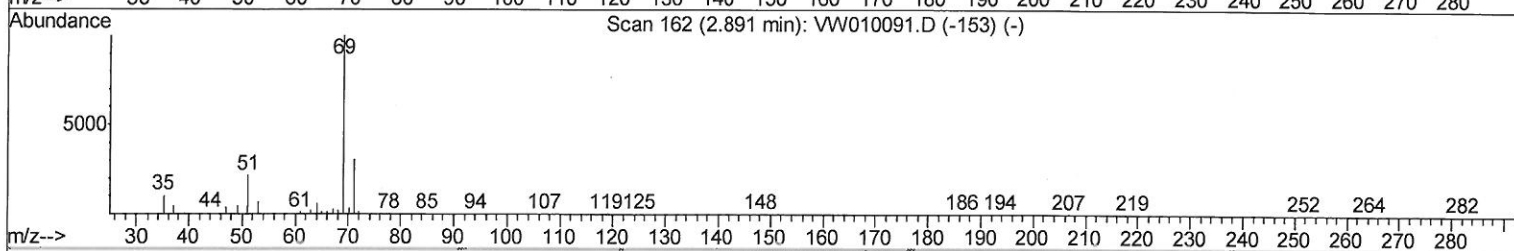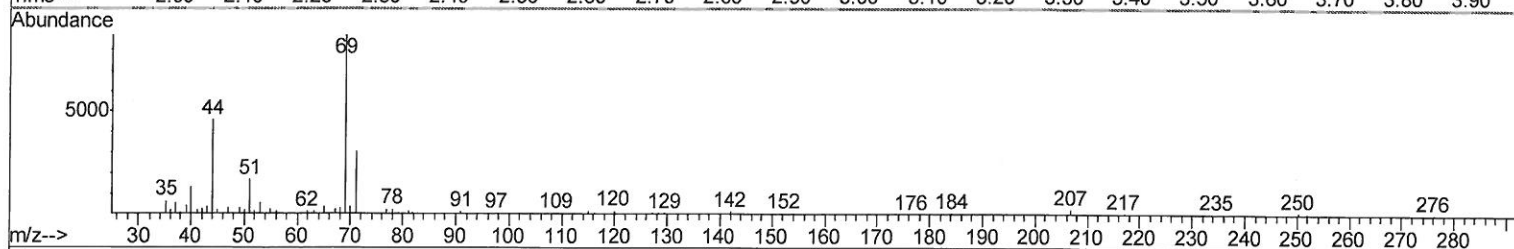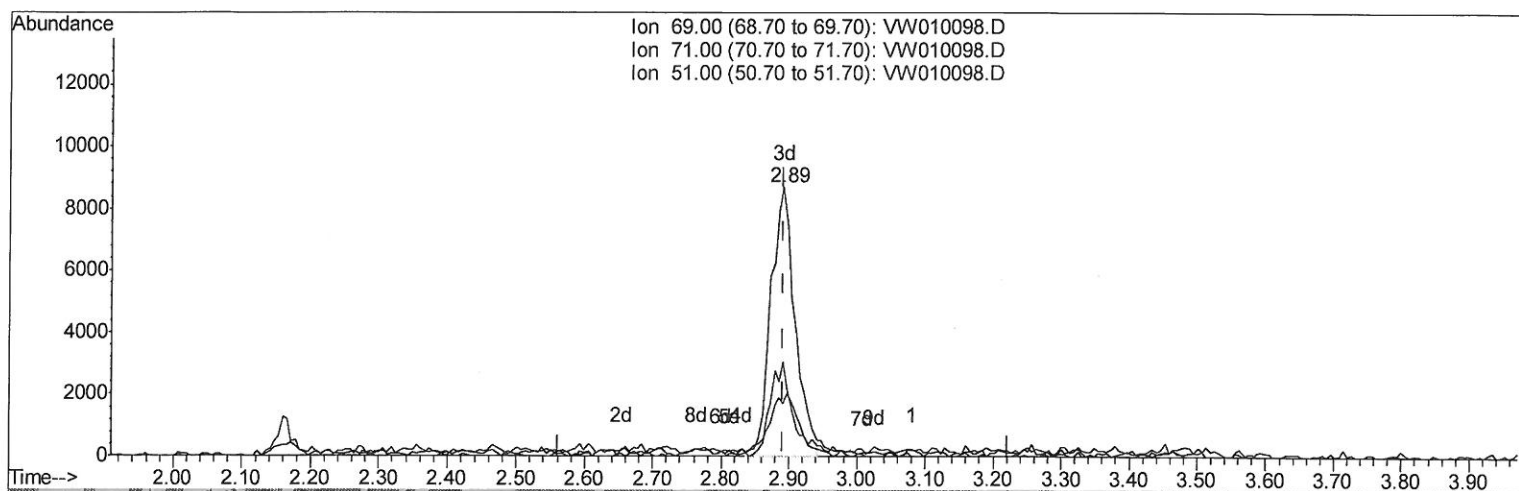

TIC: VW010098.D

(7) Chloroethane-d5 (S)

2.892min (+0.000) 18.80ug/L m

response 21317

Ion	Exp%	Act%
69.00	100	100
71.00	32.70	0.35#
51.00	29.10	0.54#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042319\
Quantitation Report (QT Reviewed)

Data File : VW010098.D
Acq On : 23 Apr 2019 14:36
Operator : SY/VA
Sample : K2456-16
Misc : 5.03G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAHN6

Manual Integrations
APPROVED

MMDadoda
4/25/2019 9:22:08 AM

Quant Time: Apr 24 04:38:05 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM041519S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 24 03:51:20 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	118430	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	110107	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	35698	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	23338	20.85	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.40%
7) Chloroethane-d5	2.89	69	21317m	18.80	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.20%
10) 1,1-Dichloroethene-d2	4.00	63	50511	16.27	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.08%
20) 2-Butanone-d5	7.08	46	29496m	48.72	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.44%
24) Chloroform-d	7.64	84	69701	20.36	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.44%
26) 1,2-Dichloroethane-d4	8.31	65	47028	22.14	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.56%
29) Benzene-d6	8.27	84	134100	22.16	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.64%
33) 1,2-Dichloropropane-d6	9.27	67	44916	23.30	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.20%
37) Toluene-d8	10.32	98	106770	19.34	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.36%
38) trans-1,3-Dichloropropene-	10.58	79	17999	19.70	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.80%
39) 2-Hexanone-d5	10.93	63	17927	41.98	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.96%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	36033	19.99	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.96%
61) 1,2-Dichlorobenzene-d4	13.86	152	27690	20.63	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	82.52%

04/25/19SY

Target Compounds

					Qvalue
13) Acetone	4.12	43	11945	22.188	ug/L 96
16) Methylene chloride	4.91	84	9357	4.364	ug/L 85
44) Toluene	10.39	91	8356	1.214	ug/L 95
54) m,p-Xylene	11.84	106	7227	2.569	ug/L 85
55) o-xylene	12.16	106	17603	6.524	ug/L 97
56) Styrene	12.19	104	42350	8.966	ug/L 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed