

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042523\
 Data File : VW025670.D
 Acq On : 25 Apr 2023 09:51
 Operator : SY/MD
 Sample : VW0425SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK486

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/26/2023
 Supervised By :Mahesh Dadoda 04/26/2023

04/26/2023
 Supervised By :Mahesh
 Dadoda

Quant Time: Apr 26 01:13:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 26 01:13:04 2023
 Response via : Initial Calibration

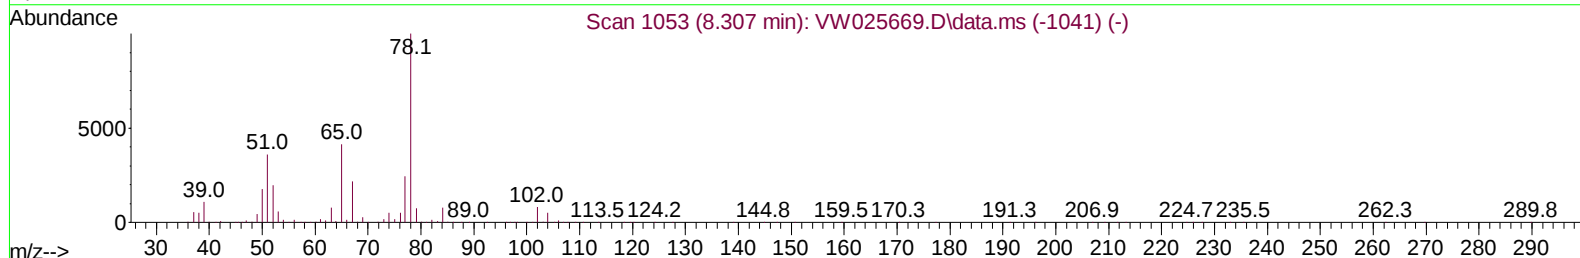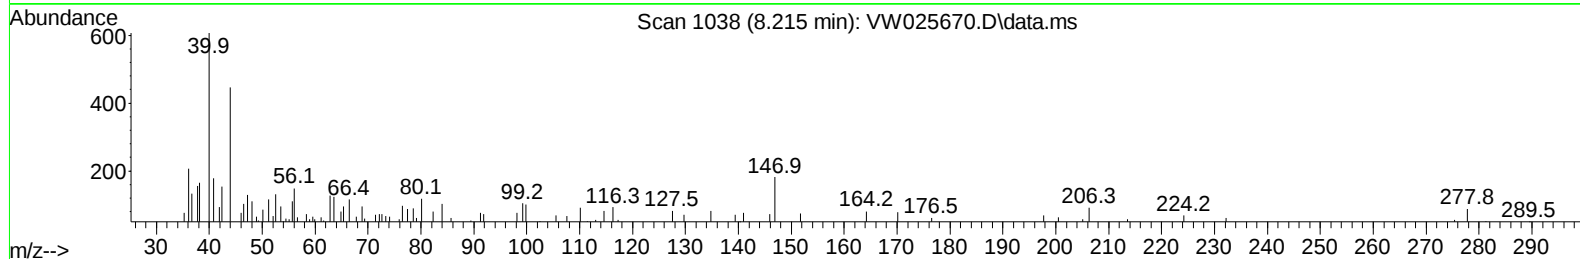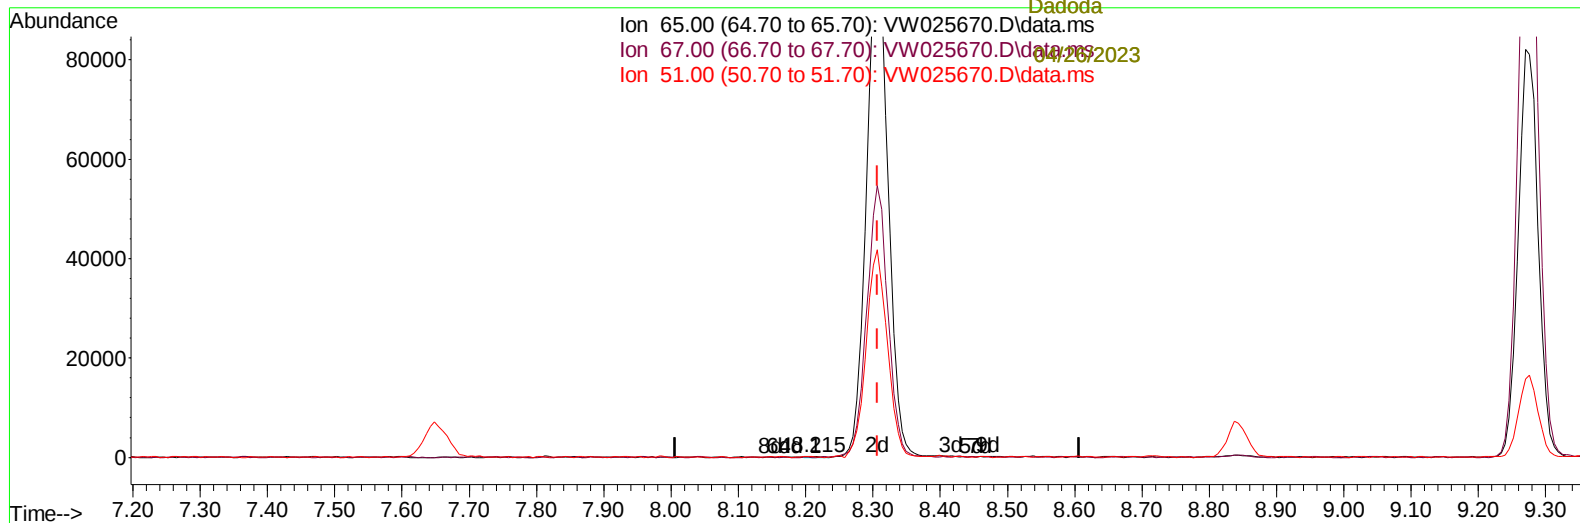

TIC: VW025670.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.215min (-0.091) 0.02 ug/L

response 202

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.50	65.35
51.00	124.00	136.14
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042523\
 Data File : VW025670.D
 Acq On : 25 Apr 2023 09:51
 Operator : SY/MD
 Sample : VW0425SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK486

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/26/2023
 Supervised By :Mahesh Dadoda 04/26/2023

Quant Time: Apr 26 01:13:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 26 01:13:04 2023
 Response via : Initial Calibration

04/26/2023
 Supervised By :Mahesh
 Dadoda

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----04/26/2023						
Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	652964	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	585480	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	280329	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	179367	16.881	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	67.520%	
7) Chloroethane-d5	2.899	69	146669	19.388	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	77.560%	
11) 1,1-Dichloroethene-d2	4.027	63	303242	14.112	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	56.440%	
21) 2-Butanone-d5	7.075	46	133586	56.355	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	112.720%	
24) Chloroform-d	7.648	84	401509	21.900	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	87.600%	
26) 1,2-Dichloroethane-d4	8.307	65	224238m	23.510	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	94.040%	
32) Benzene-d6	8.276	84	810127	21.369	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	85.480%	
36) 1,2-Dichloropropane-d6	9.276	67	260622	22.048	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	88.200%	
41) Toluene-d8	10.325	98	693820	20.951	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	83.800%	
43) trans-1,3-Dichloroprop...	10.575	79	94080	21.229	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	84.920%	
47) 2-Hexanone-d5	10.922	63	90666	56.115	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	112.240%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	204314	25.609	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	102.440%	
66) 1,2-Dichlorobenzene-d4	13.855	152	216138	22.443	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	89.760%	
Target Compounds						
16) Methylene chloride	4.923	84	32527	3.134	ug/L	Qvalue 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042523\
Data File : VW025670.D
Acq On : 25 Apr 2023 09:51
Operator : SY/MD
Sample : VW0425SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK486

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/26/2023
Supervised By :Mahesh Dadoda 04/26/2023

04/26/2023
Supervised By :Mahesh
Dadoda

04/26/2023

