




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042523\
 Data File : VW025673.D
 Acq On : 25 Apr 2023 11:03
 Operator : SY/MD
 Sample : 02479-02
 Misc : 4.63g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW943

Manual IntegrationsAPPROVED

Quant Time: Apr 26 01:14:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 26 01:13:04 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/26/2023
 Supervised By :Mahesh Dadoda 04/26/2023

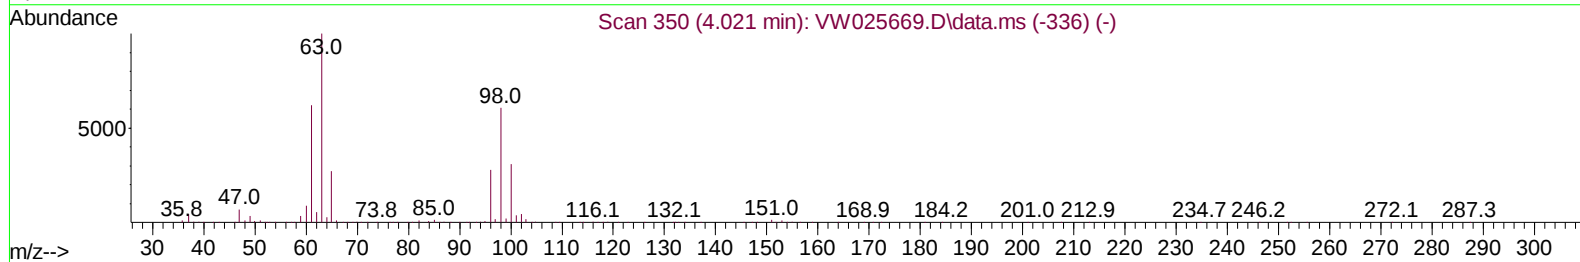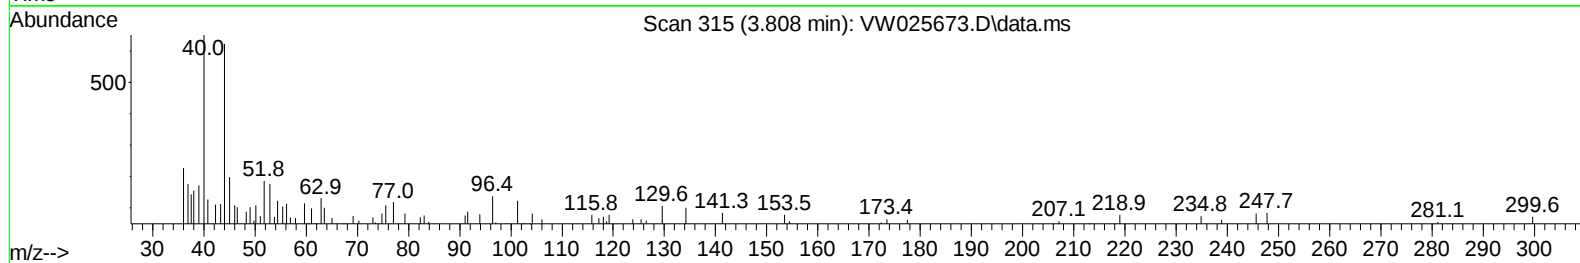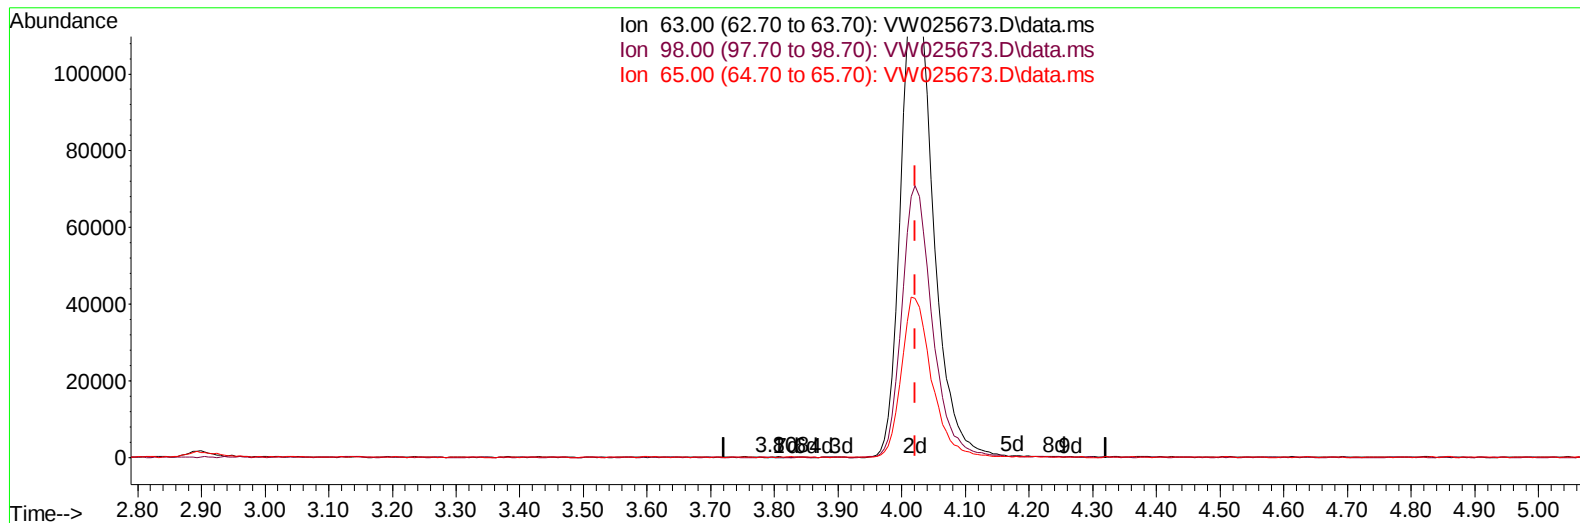

TIC: VW025673.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.808min (-0.213) 0.01 ug/L

response 153

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.70	66.67
65.00	23.30	21.57
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042523\
 Data File : VW025673.D
 Acq On : 25 Apr 2023 11:03
 Operator : SY/MD
 Sample : 02479-02
 Misc : 4.63g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW943

Manual IntegrationsAPPROVED

Quant Time: Apr 26 01:14:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 26 01:13:04 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/26/2023
 Supervised By :Mahesh Dadoda 04/26/2023

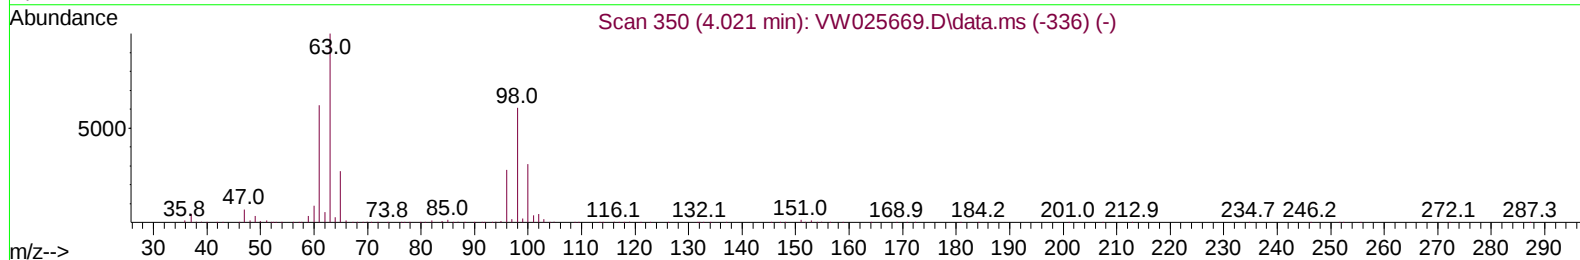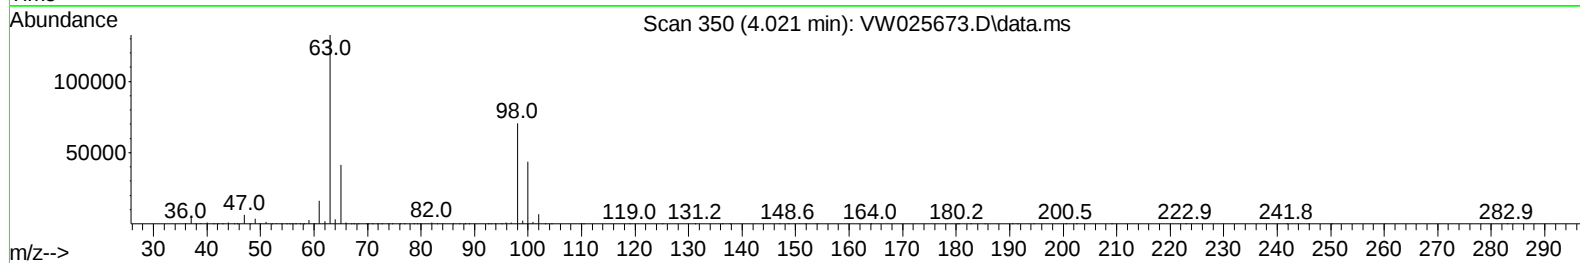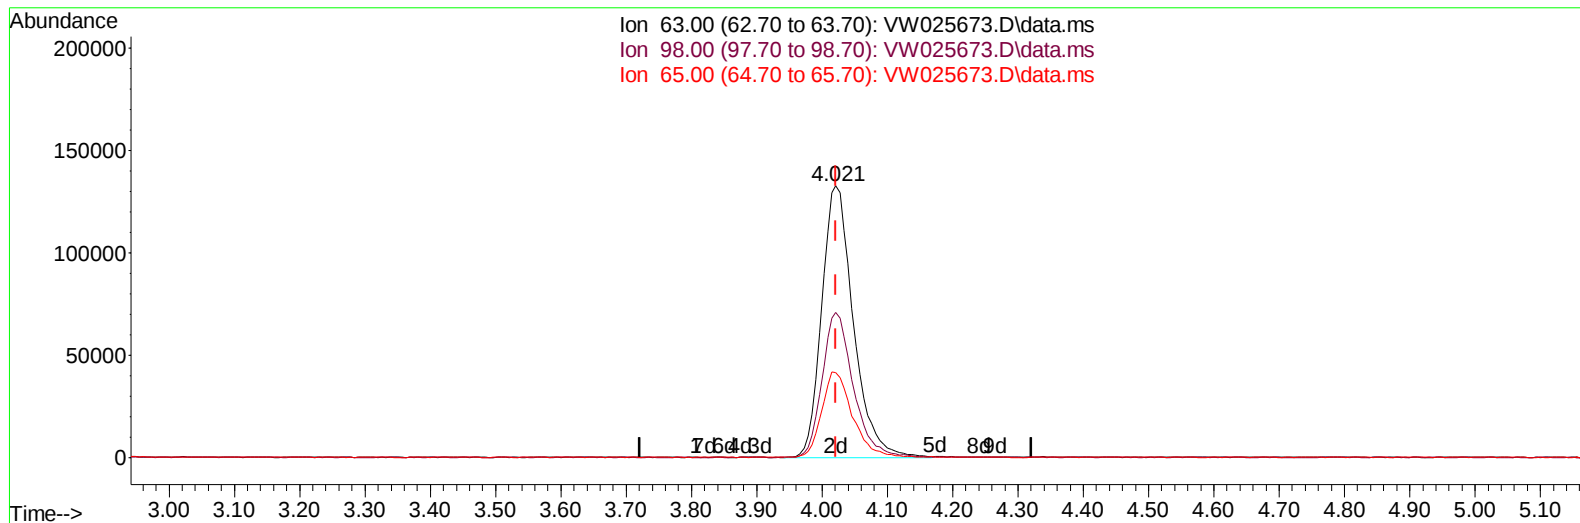

TIC: VW025673.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.021min (+ 0.000) 16.30 ug/L m

response 445097

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.70	0.02#
65.00	23.30	0.01#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042523\
 Data File : VW025673.D
 Acq On : 25 Apr 2023 11:03
 Operator : SY/MD
 Sample : 02479-02
 Misc : 4.63g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW943

Manual IntegrationsAPPROVED

Quant Time: Apr 26 01:14:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 26 01:13:04 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/26/2023
 Supervised By :Mahesh Dadoda 04/26/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		829924	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		308096	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		32082	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		277042	20.514	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	82.040%		
7) Chloroethane-d5	2.899	69		265011	27.561	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	110.240%		
11) 1,1-Dichloroethene-d2	4.021	63		445097m	16.297	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	65.200%		
21) 2-Butanone-d5	7.075	46		182163	60.462	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	120.920%		
24) Chloroform-d	7.648	84		636332	27.308	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	109.240%		
26) 1,2-Dichloroethane-d4	8.307	65		339846	28.034	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	112.120%		
32) Benzene-d6	8.270	84		1175735	58.935	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	235.760%#		
36) 1,2-Dichloropropane-d6	9.276	67		381463	61.325	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	245.320%#		
41) Toluene-d8	10.325	98		622612	35.728	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	142.920%#		
43) trans-1,3-Dichloroprop...	10.575	79		76707	32.892	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	131.560%		
47) 2-Hexanone-d5	10.922	63		82230	96.715	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	193.420%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		180005	42.874	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	171.480%#		
66) 1,2-Dichlorobenzene-d4	13.849	152		32488	29.476	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	117.920%		
Target Compounds							
13) Acetone	4.131	43		7037	2.760	ug/L	91
16) Methylene chloride	4.917	84		32447	2.460	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042523\
Data File : VW025673.D
Acq On : 25 Apr 2023 11:03
Operator : SY/MD
Sample : 02479-02
Misc : 4.63g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW943

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/26/2023
Supervised By :Mahesh Dadoda 04/26/2023

Quant Time: Apr 26 01:14:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 26 01:13:04 2023
Response via : Initial Calibration

