

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042523\
 Data File : VW025676.D
 Acq On : 25 Apr 2023 12:15
 Operator : SY/MD
 Sample : 02479-12
 Misc : 5.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW953

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/26/2023
 Supervised By :Mahesh Dadoda 04/26/2023

Quant Time: Apr 26 01:15:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 26 01:13:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	619980	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	338883	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	55607	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	160895	15.948	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	63.800%	
7) Chloroethane-d5	2.899	69	147695	20.562	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	82.240%	
11) 1,1-Dichloroethene-d2	4.027	63	266532	13.063	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	52.240%	
21) 2-Butanone-d5	7.075	46	161572	71.788	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	143.580%#	
24) Chloroform-d	7.648	84	406569	23.356	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	93.440%	
26) 1,2-Dichloroethane-d4	8.307	65	231045m	25.512	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	102.040%	
32) Benzene-d6	8.276	84	757868	34.538	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	138.160%#	
36) 1,2-Dichloropropane-d6	9.276	67	261600	38.235	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	152.920%#	
41) Toluene-d8	10.325	98	498794	26.022	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	104.080%	
43) trans-1,3-Dichloroprop...	10.575	79	65937	25.705	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	102.800%	
47) 2-Hexanone-d5	10.922	63	86342	92.325	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	184.660%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	174627	37.815	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	151.240%#	
66) 1,2-Dichlorobenzene-d4	13.848	152	53680	28.099	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	112.400%	
Target Compounds					Qvalue	
13) Acetone	4.118	43	17807	9.348	ug/L	95
16) Methylene chloride	4.923	84	54628	5.543	ug/L	93
46) Tetrachloroethene	10.861	164	12191	2.825	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042523\
Data File : VW025676.D
Acq On : 25 Apr 2023 12:15
Operator : SY/MD
Sample : 02479-12
Misc : 5.58g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW953

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/26/2023
Supervised By :Mahesh Dadoda 04/26/2023

Quant Time: Apr 26 01:15:12 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 26 01:13:04 2023
Response via : Initial Calibration

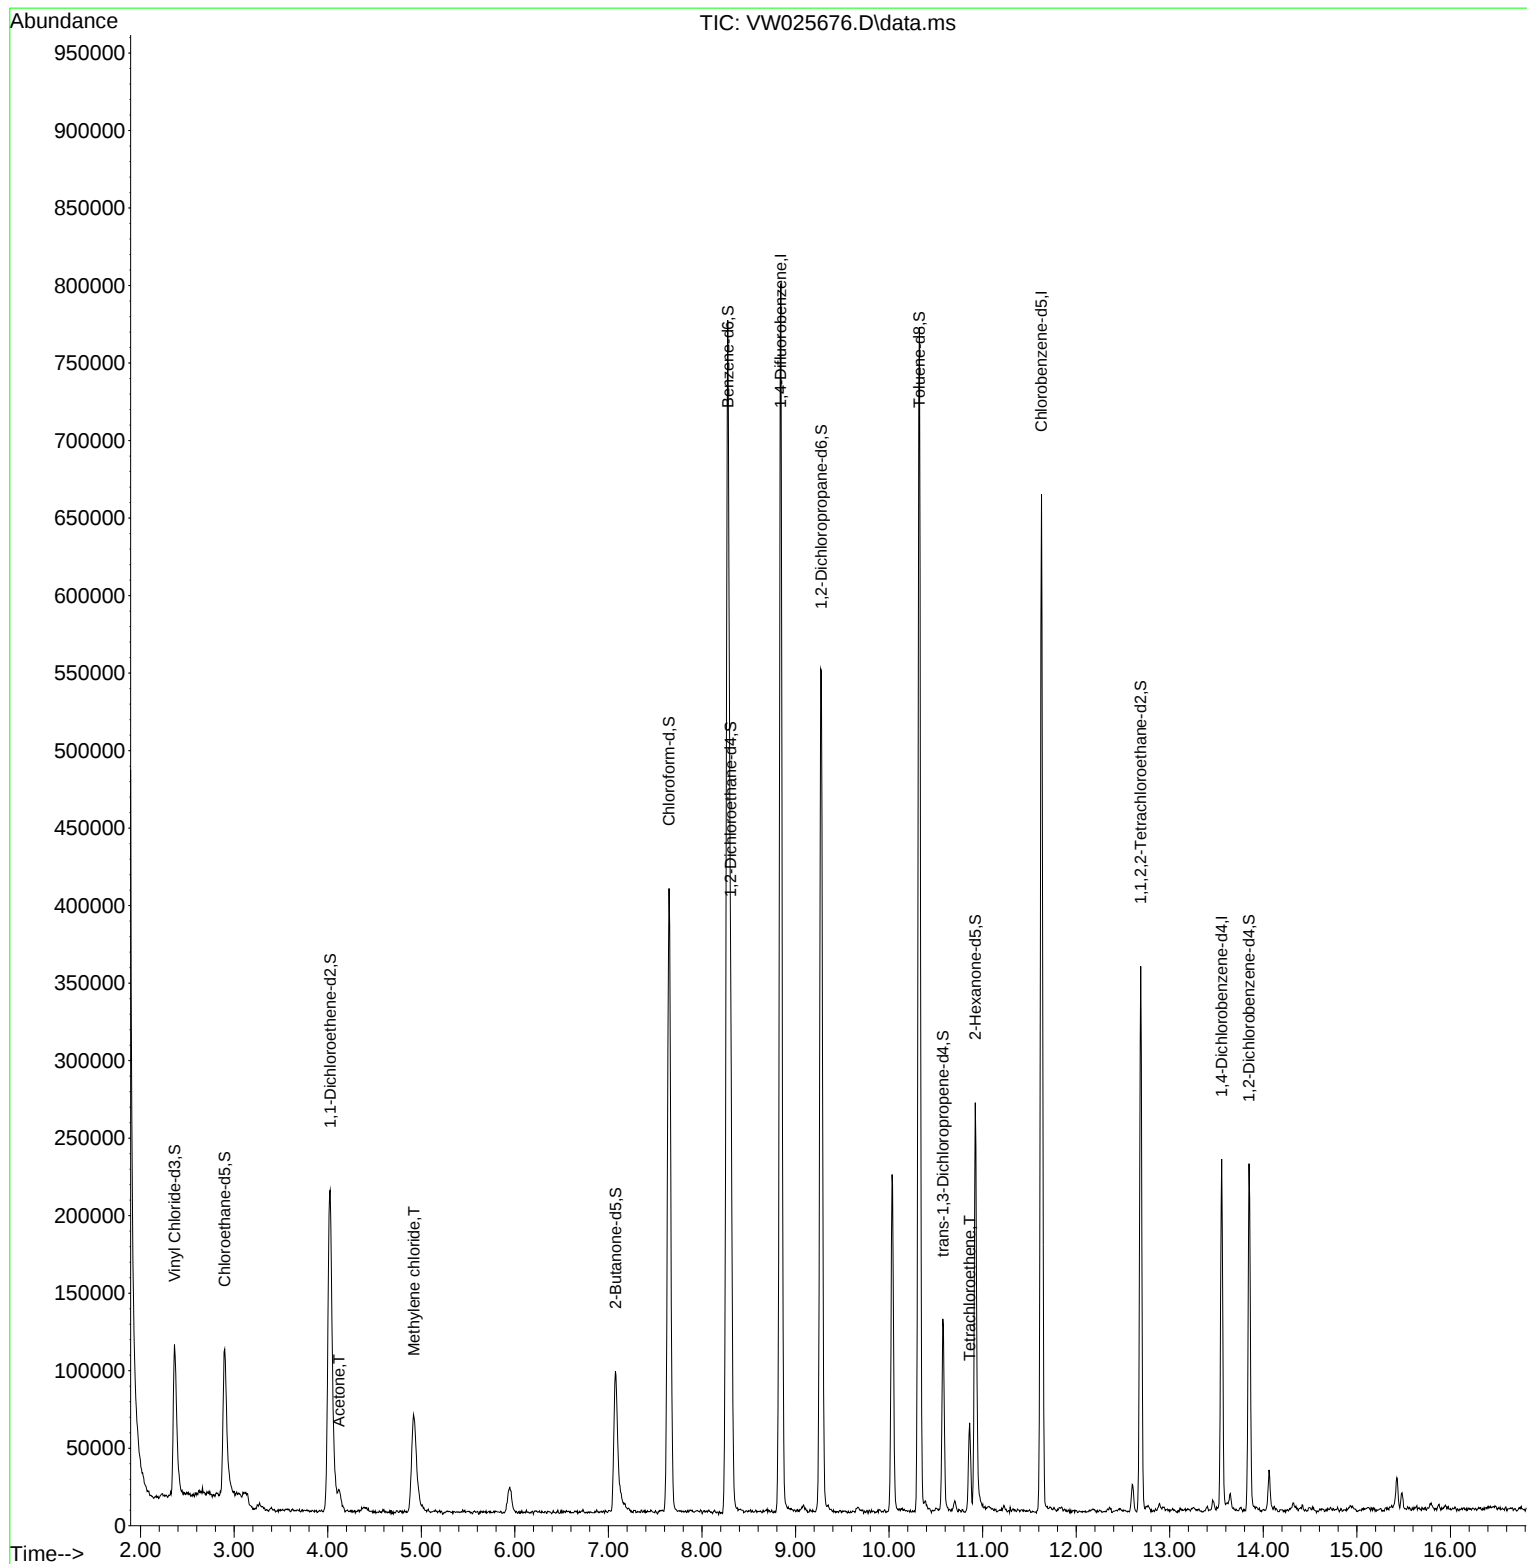

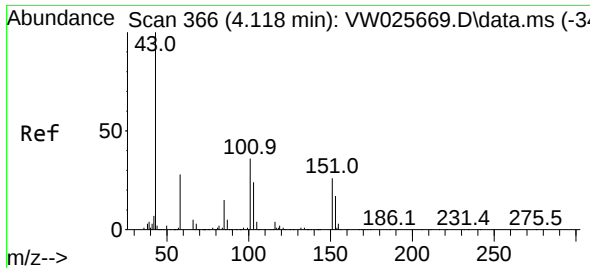

#13

Acetone

Concen: 9.348 ug/L

RT: 4.118 min Scan# 366

Delta R.T. -0.000 min

Lab File: VW025676.D

Acq: 25 Apr 2023 12:15

Instrument :

MSVOA_W

ClientSampleId :

EW953

Tgt Ion: 43 Resp: 1780

Ion Ratio Lower Upper

43 100





58 31.3 0.0 57.4

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 04/26/2023

Supervised By :Mahesh Dadoda 04/26/2023

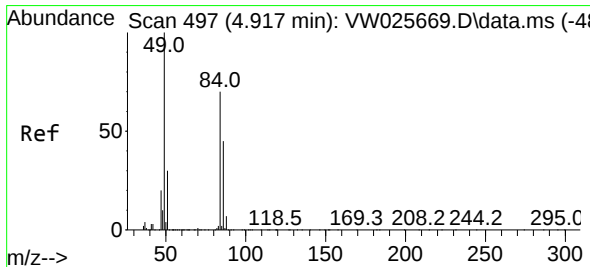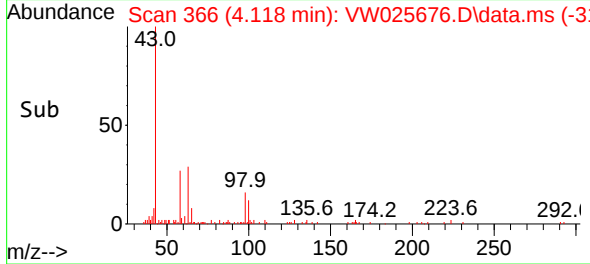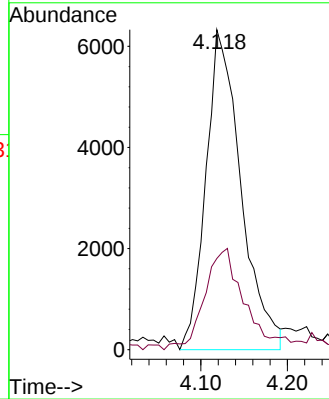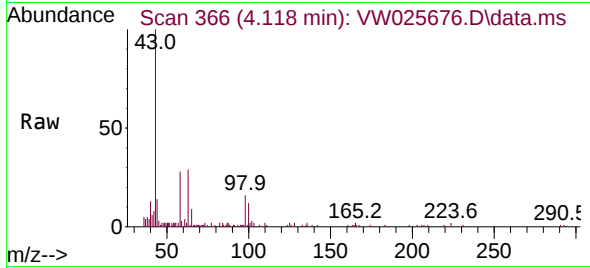

#16

Methylene chloride

Concen: 5.543 ug/L

RT: 4.923 min Scan# 498

Delta R.T. 0.006 min

Lab File: VW025676.D

Acq: 25 Apr 2023 12:15




Tgt Ion: 84 Resp: 54628


Ion Ratio Lower Upper

84 100

86 59.8 44.9 83.3


49 135.2 101.4 188.4

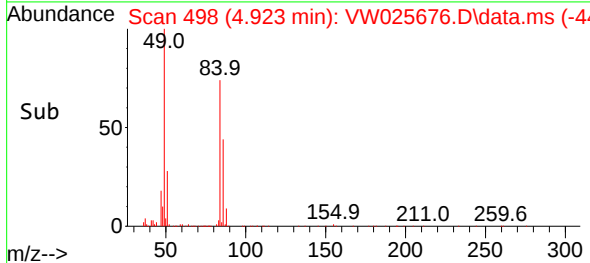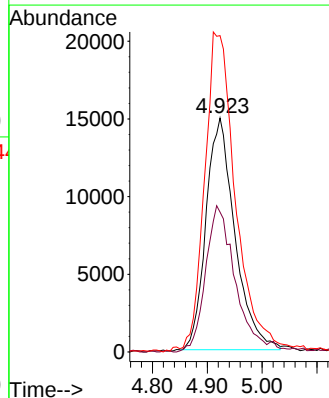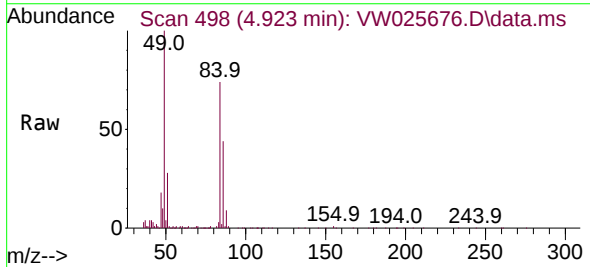

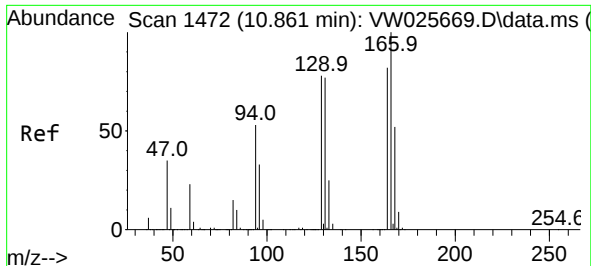

#46
Tetrachloroethene
Concen: 2.825 ug/L
RT: 10.861 min Scan# 1472
Delta R.T. -0.000 min
Lab File: VW025676.D
Acq: 25 Apr 2023 12:15

Instrument :
MSVOA_W
ClientSampleId :
EW953

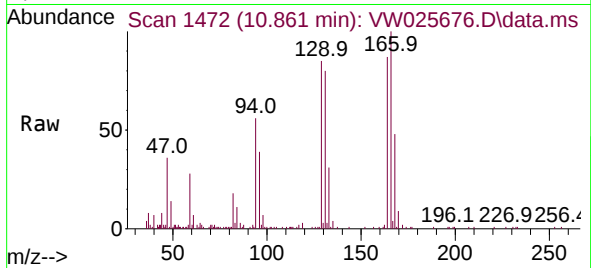

Tgt Ion	Ratio	Lower	Upper
164	100		
129	97.6	76.9	142.9
131	92.2	70.5	130.9
166	114.6	89.2	165.8

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/26/2023
Supervised By :Mahesh Dadoda 04/26/2023

