

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022618.D
 Acq On : 26 Apr 2022 11:40
 Operator : SY/VA
 Sample : N2470-04
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Apr 27 01:38:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	305670	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	290728	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	149738	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	134754	19.942	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.760%
7) Chloroethane-d5	2.885	69	91018	21.492	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.960%
11) 1,1-Dichloroethene-d2	4.013	63	142058	16.208	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.840%
21) 2-Butanone-d5	7.074	46	52251	44.290	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.580%
24) Chloroform-d	7.647	84	217506	22.765	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.080%
26) 1,2-Dichloroethane-d4	8.305	65	122919	22.517	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.080%
32) Benzene-d6	8.275	84	431480	24.292	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.160%
36) 1,2-Dichloropropane-d6	9.274	67	122462	23.824	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.280%
41) Toluene-d8	10.323	98	405392	23.303	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.200%
43) trans-1,3-Dichloroprop...	10.579	79	48509	19.996	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.000%
47) 2-Hexanone-d5	10.921	63	44767	46.810	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.620%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	103071	23.583	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.320%
66) 1,2-Dichlorobenzene-d4	13.853	152	135029	25.459	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.840%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	4930	0.657	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022618.D
Acq On : 26 Apr 2022 11:40
Operator : SY/VA
Sample : N2470-04
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Quant Time: Apr 27 01:38:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

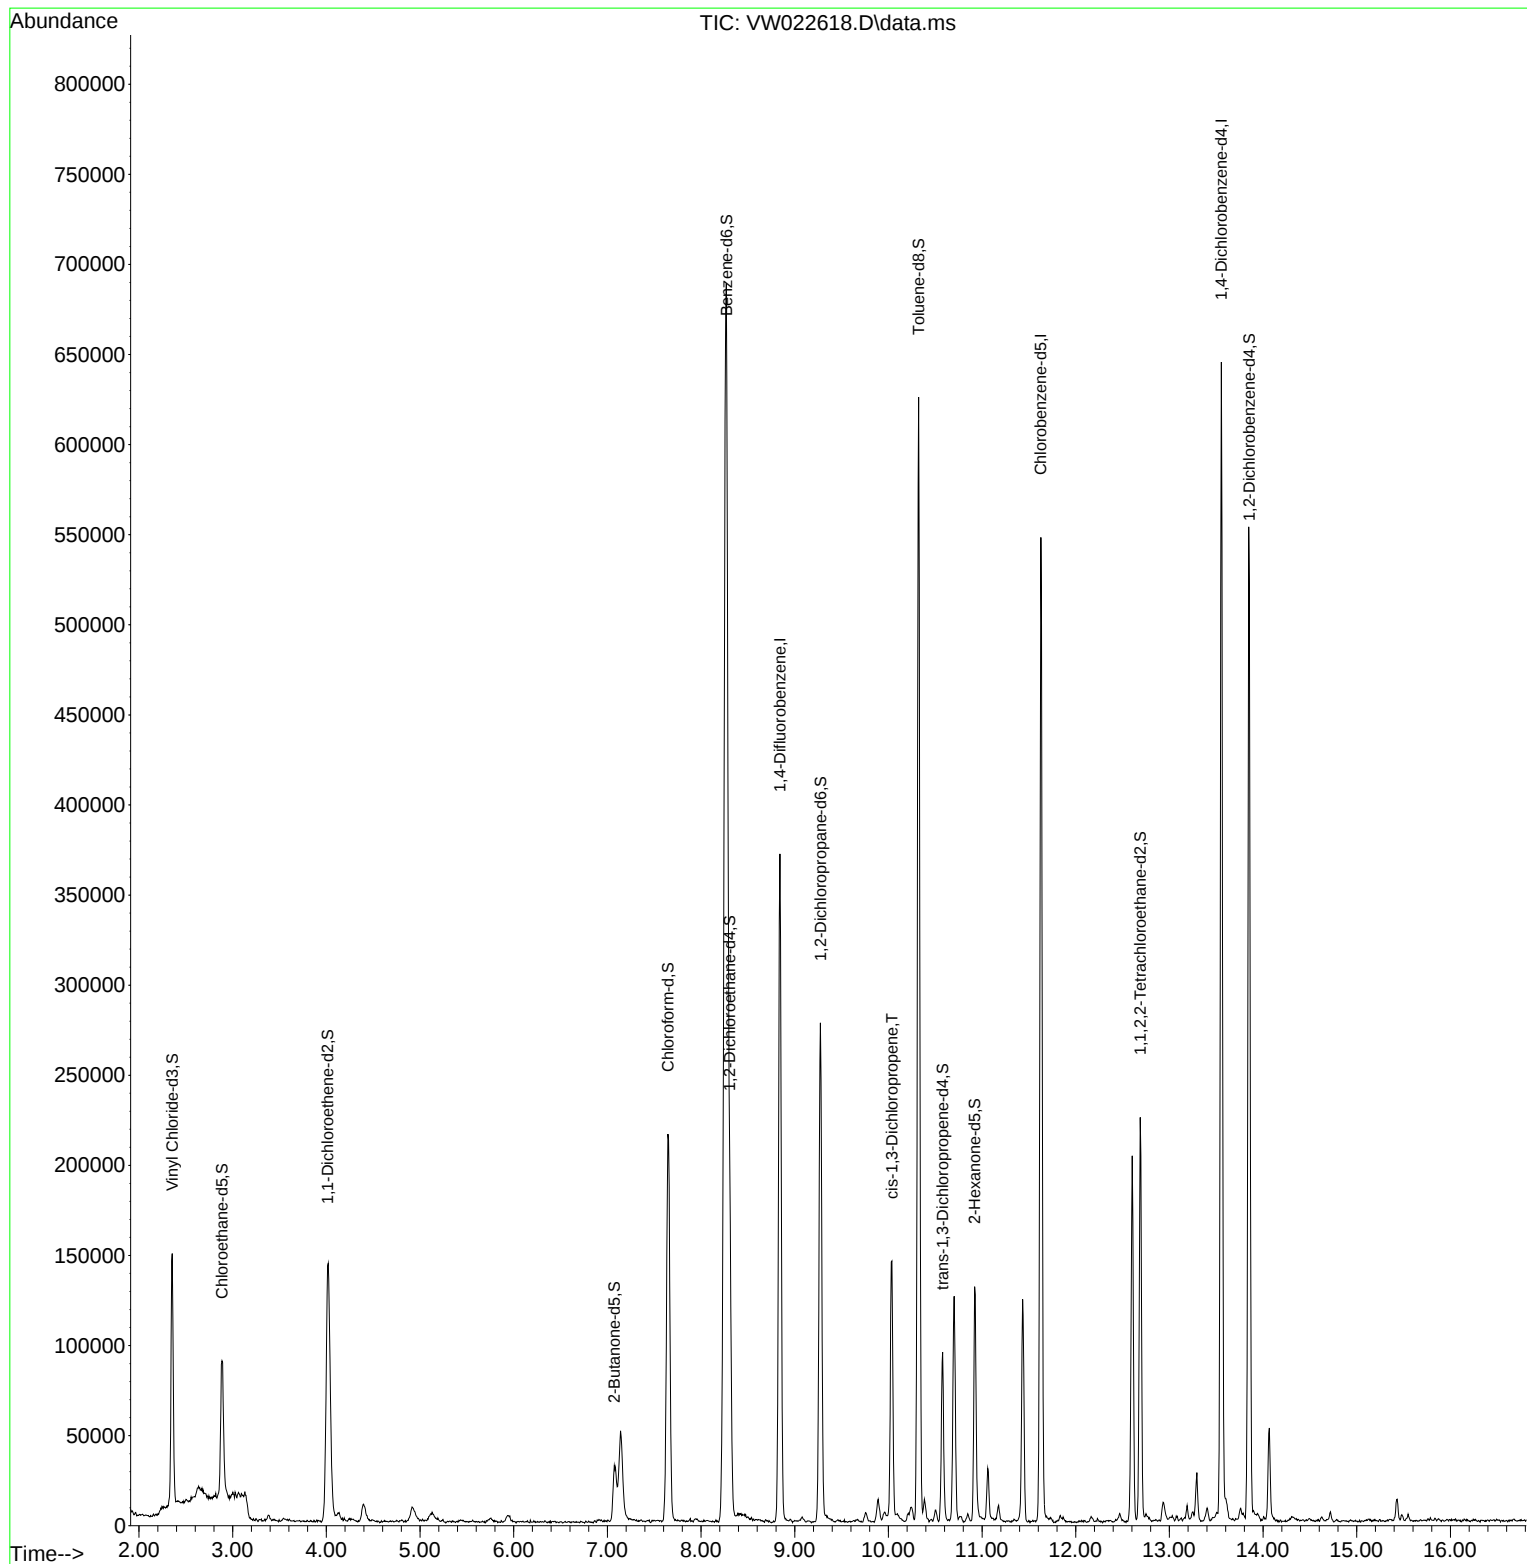

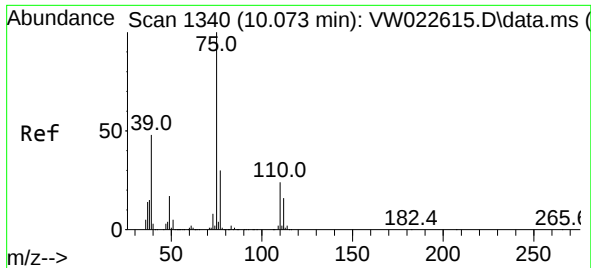

#39

cis-1,3-Dichloropropene

Concen: 0.657 ug/L

RT: 10.037 min Scan# 11

Delta R.T. -0.037 min

Lab File: VW022618.D


Acq: 26 Apr 2022 11:40

Instrument :

MSVOA_W

ClientSampleId :

VHBLK001

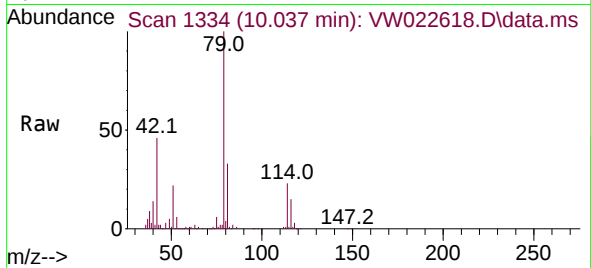

Tgt Ion: 75 Resp: 4930

Ion Ratio Lower Upper

75 100

77 36.8 22.6 42.0

