

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022626.D
 Acq On : 26 Apr 2022 15:50
 Operator : SY/VA
 Sample : N2562-06
 Misc : 8.07g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW467

Quant Time: Apr 27 01:40:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	282225	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	243691	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	94312	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	77038	12.348	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	49.400%
7) Chloroethane-d5	2.891	69	61467	15.720	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.880%
11) 1,1-Dichloroethene-d2	4.123	63	400	0.049	ug/L	0.10
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.200%#
21) 2-Butanone-d5	7.080	46	72368	66.437	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	132.880%
24) Chloroform-d	7.653	84	176568	20.016	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.080%
26) 1,2-Dichloroethane-d4	8.305	65	110698	21.963	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.840%
32) Benzene-d6	8.275	84	299869	20.141	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	80.560%
36) 1,2-Dichloropropane-d6	9.274	67	99269	23.040	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.160%
41) Toluene-d8	10.323	98	253321	17.372	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	69.480%
43) trans-1,3-Dichloroprop...	10.579	79	39295	19.325	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.280%
47) 2-Hexanone-d5	10.927	63	57725	72.010	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	144.020%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	111652	30.477	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	121.920%#
66) 1,2-Dichlorobenzene-d4	13.853	152	76795	22.989	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.960%
Target Compounds						
13) Acetone	4.135	43	2658	3.584	ug/L	Qvalue 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022626.D
Acq On : 26 Apr 2022 15:50
Operator : SY/VA
Sample : N2562-06
Misc : 8.07g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW467

Quant Time: Apr 27 01:40:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

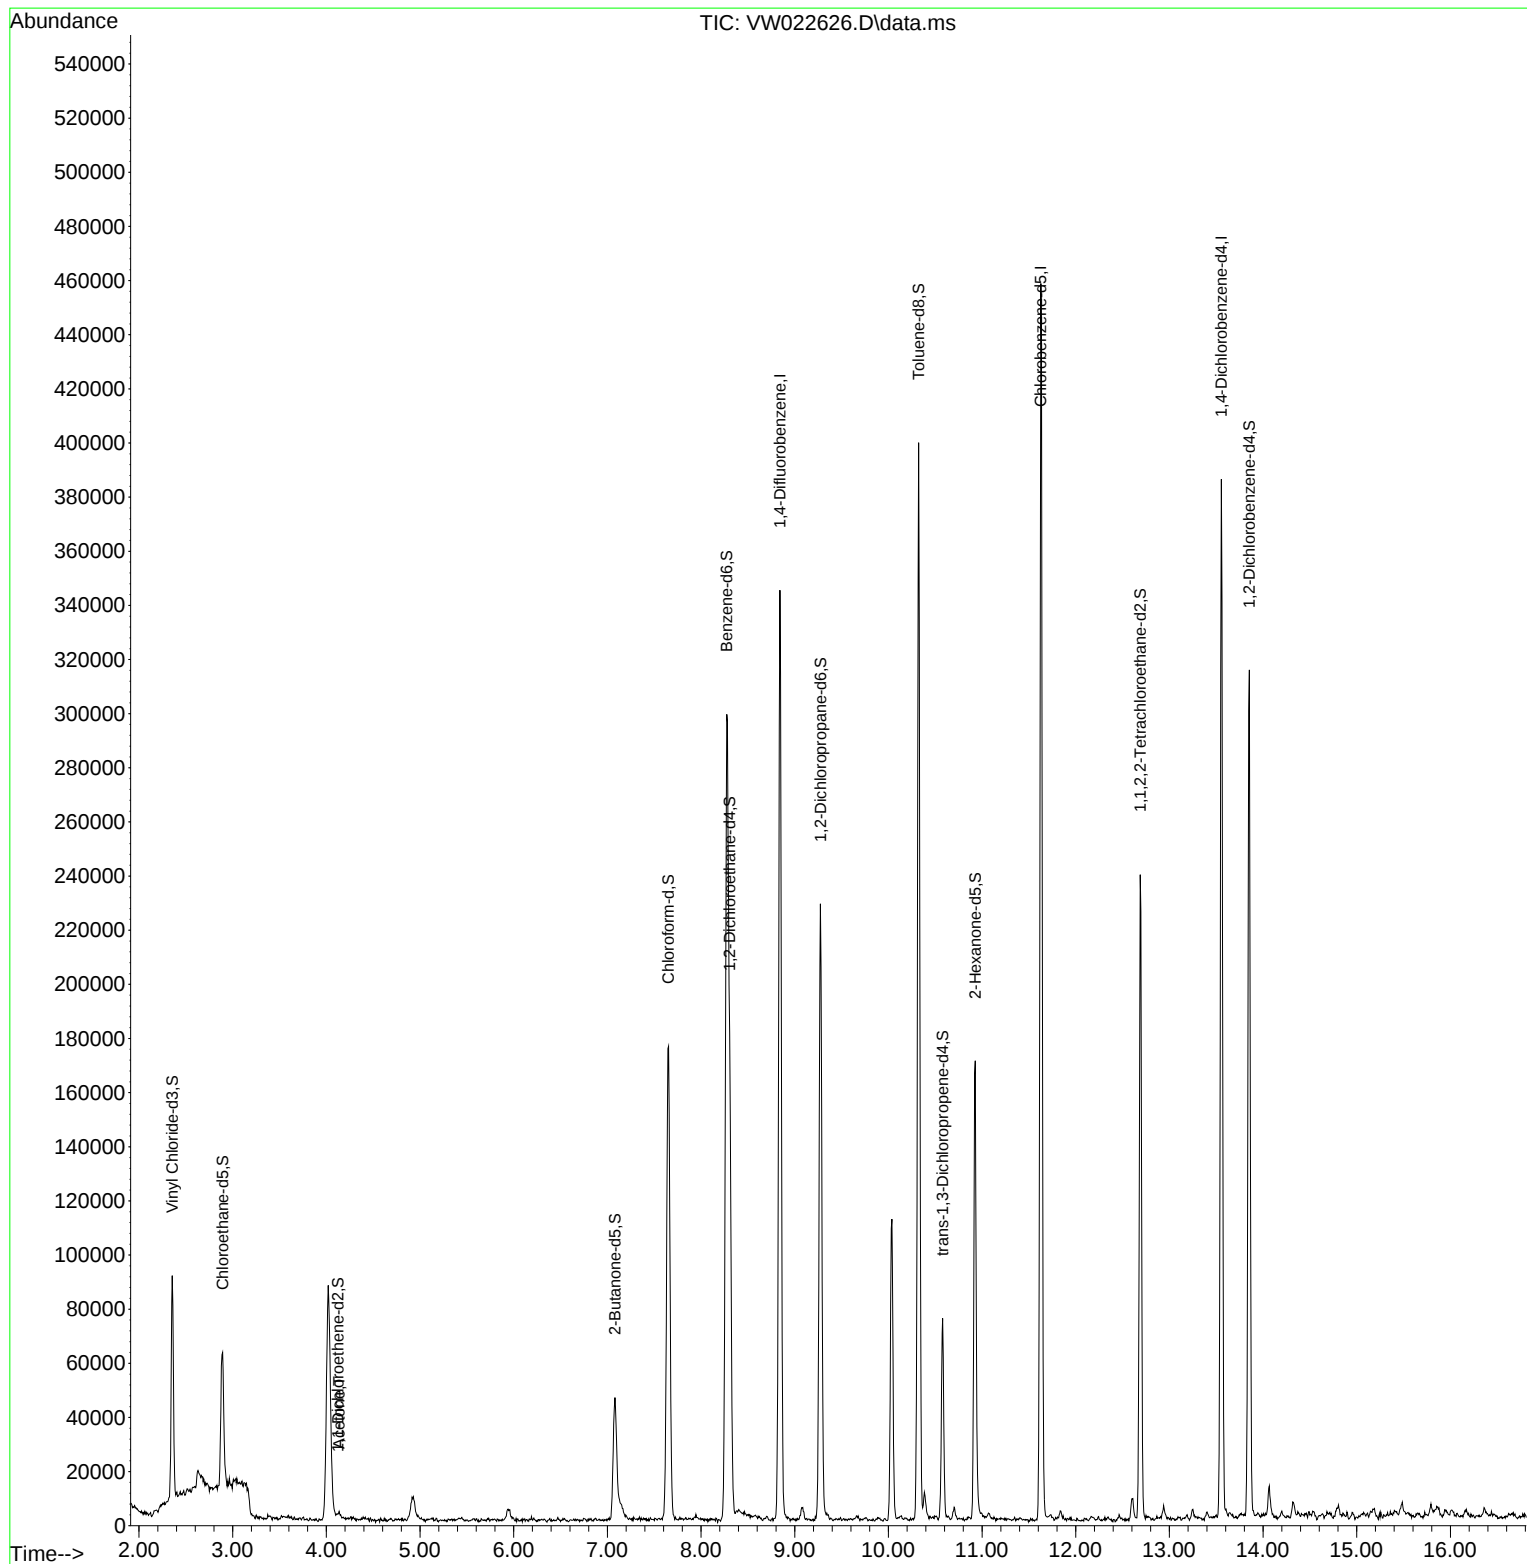

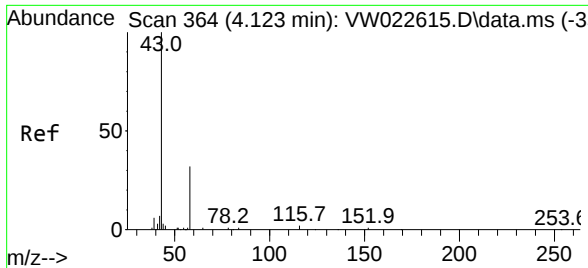

#13
 Acetone
 Concen: 3.584 ug/L
 RT: 4.135 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW022626.D
 Acq: 26 Apr 2022 15:50

Instrument :
 MSVOA_W
 ClientSampleId :
 EW467

Tgt Ion: 43 Resp: 2658
 Ion Ratio Lower Upper
 43 100
 58 19.1 0.0 57.0

