

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022627.D
 Acq On : 26 Apr 2022 16:14
 Operator : SY/VA
 Sample : N2562-07
 Misc : 8.29g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW468

Quant Time: Apr 27 01:40:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	263609	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	216850	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	72114	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	74350	12.758	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	51.040%
7) Chloroethane-d5	2.885	69	58102	15.908	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	63.640%
11) 1,1-Dichloroethene-d2	4.019	63	75075	9.932	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	39.720%#
21) 2-Butanone-d5	7.080	46	76326	75.019	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	150.040%#
24) Chloroform-d	7.647	84	167339	20.309	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.240%
26) 1,2-Dichloroethane-d4	8.403	65	144	0.031	ug/L	0.10
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.120%#
32) Benzene-d6	8.275	84	285125	21.521	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.080%
36) 1,2-Dichloropropane-d6	9.274	67	95693	24.959	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.840%
41) Toluene-d8	10.323	98	229111	17.657	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	70.640%
43) trans-1,3-Dichloroprop...	10.579	79	35244	19.478	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.920%
47) 2-Hexanone-d5	10.920	63	61595	86.349	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	172.700%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	106637	32.711	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	130.840%#
66) 1,2-Dichlorobenzene-d4	13.853	152	57609	22.554	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.200%
Target Compounds					Qvalue	
13) Acetone	4.129	43	3519	5.080	ug/L	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022627.D
Acq On : 26 Apr 2022 16:14
Operator : SY/VA
Sample : N2562-07
Misc : 8.29g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW468

Quant Time: Apr 27 01:40:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

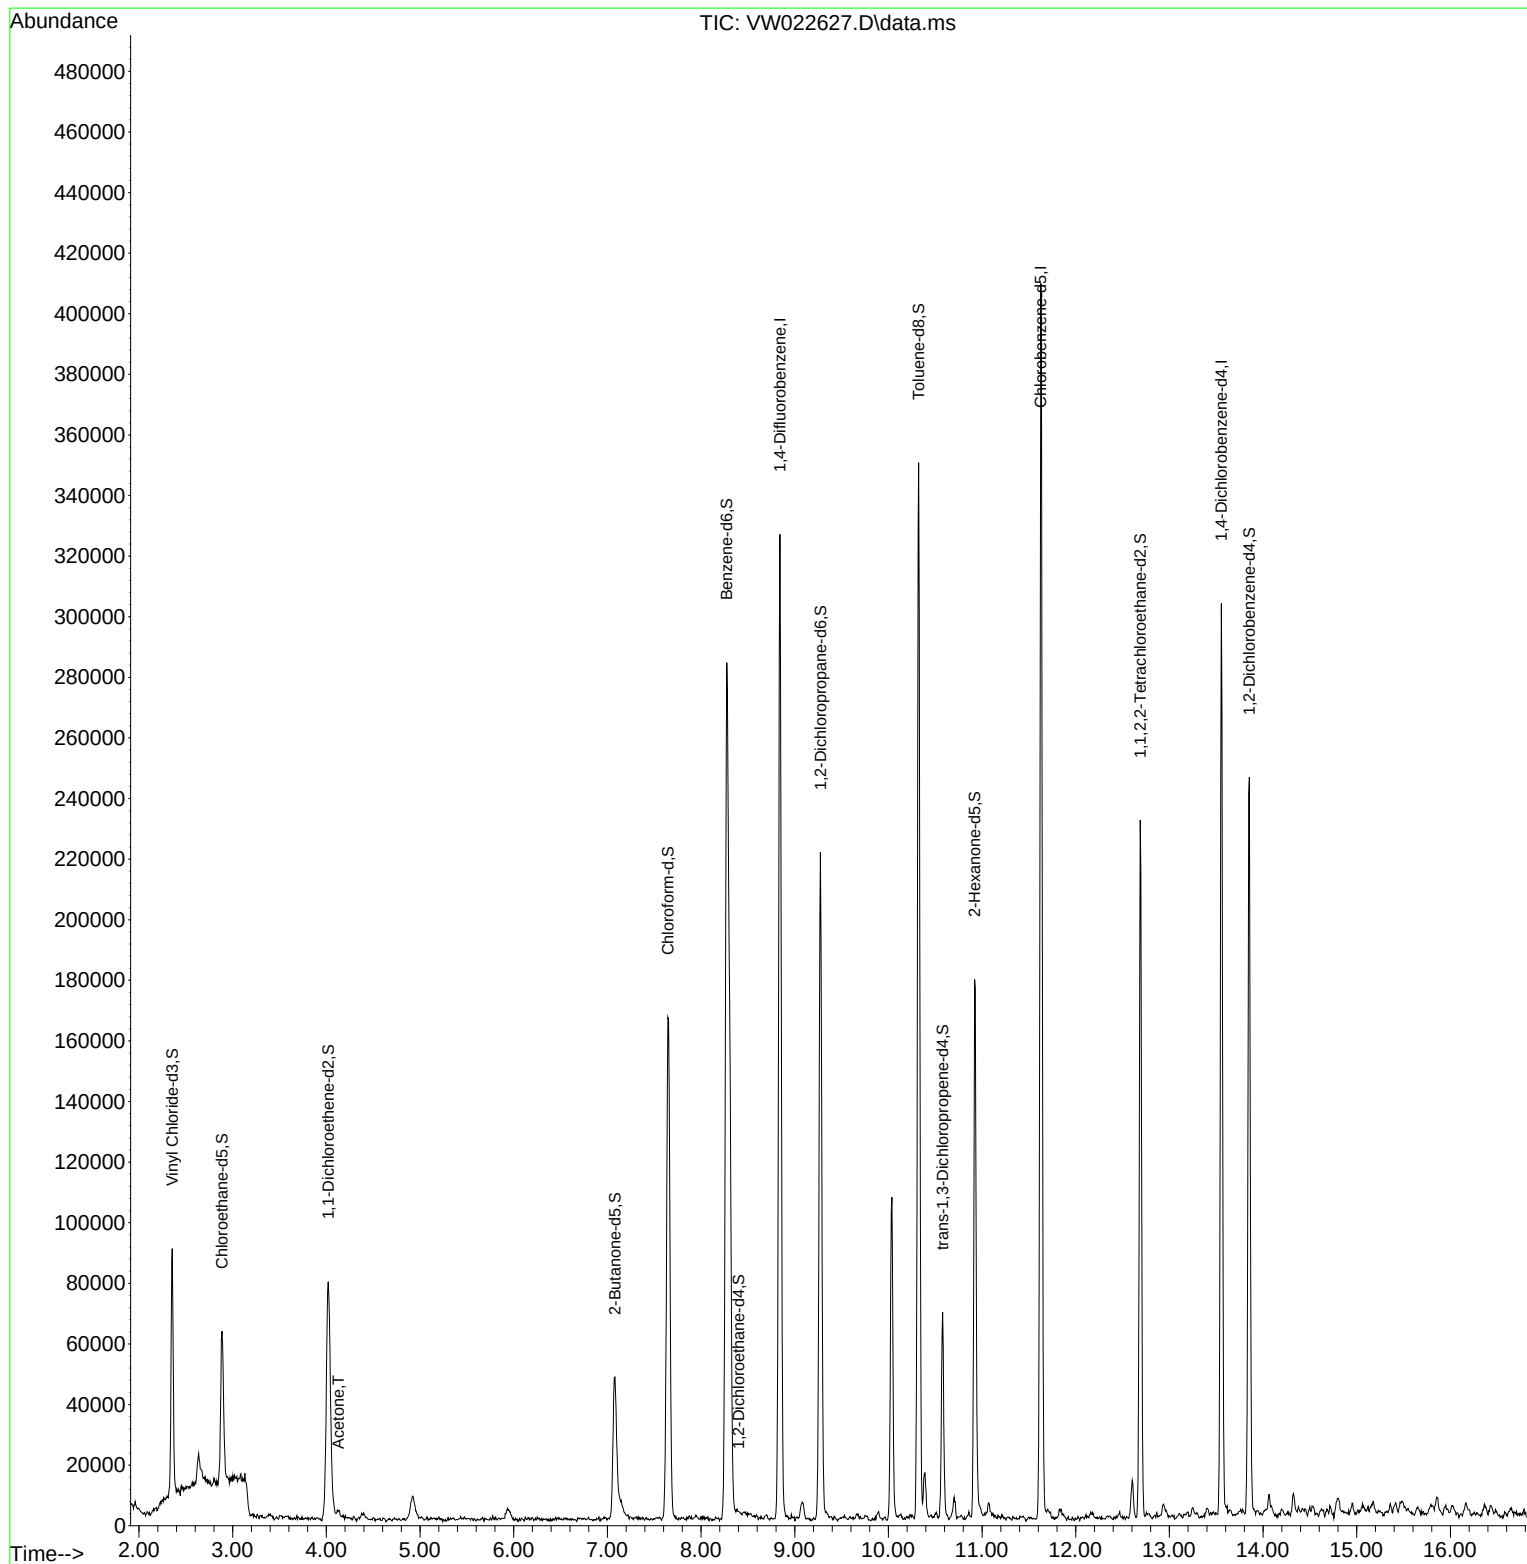

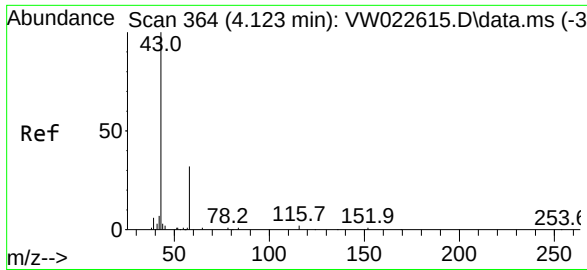

#13

Acetone

Concen: 5.080 ug/L

RT: 4.129 min Scan# 30

Delta R.T. 0.006 min

Lab File: VW022627.D

Acq: 26 Apr 2022 16:14

Instrument :

MSVOA_W

ClientSampleId :

EW468

Tgt Ion: 43 Resp: 3519

Ion Ratio Lower Upper

43 100

58 43.1 0.0 57.0

