




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022616.D
 Acq On : 26 Apr 2022 10:52
 Operator : SY/VA
 Sample : VW0426SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK486

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:38:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

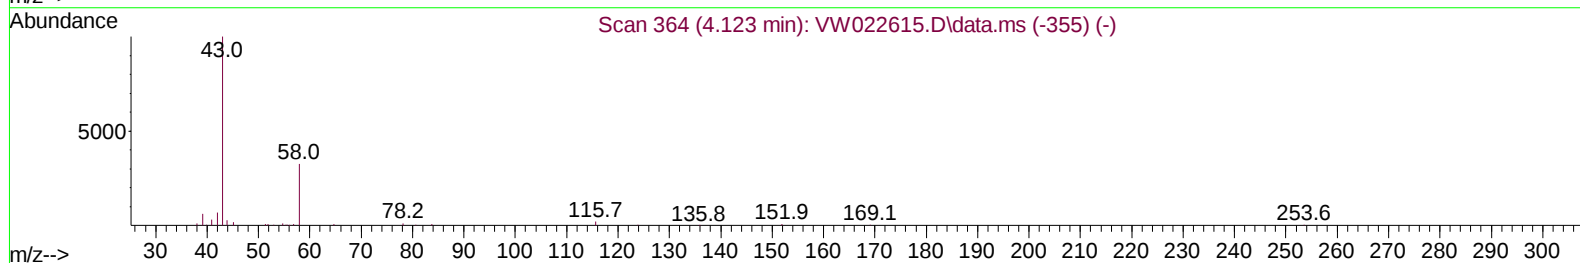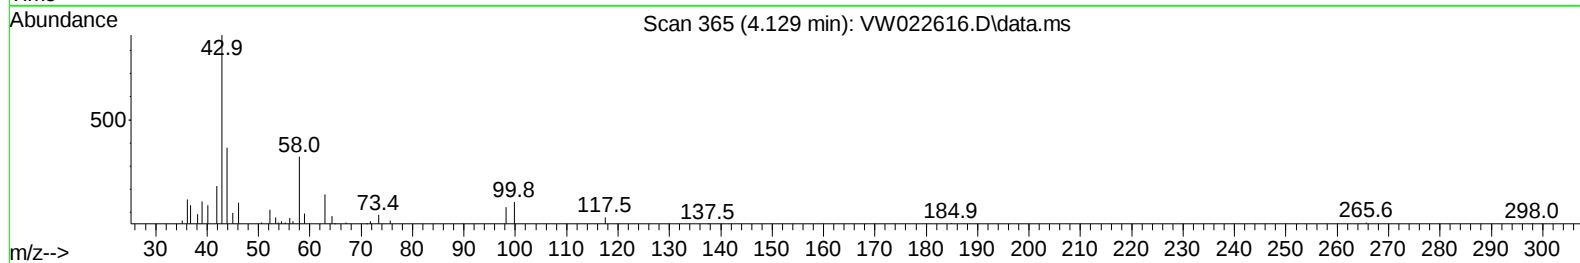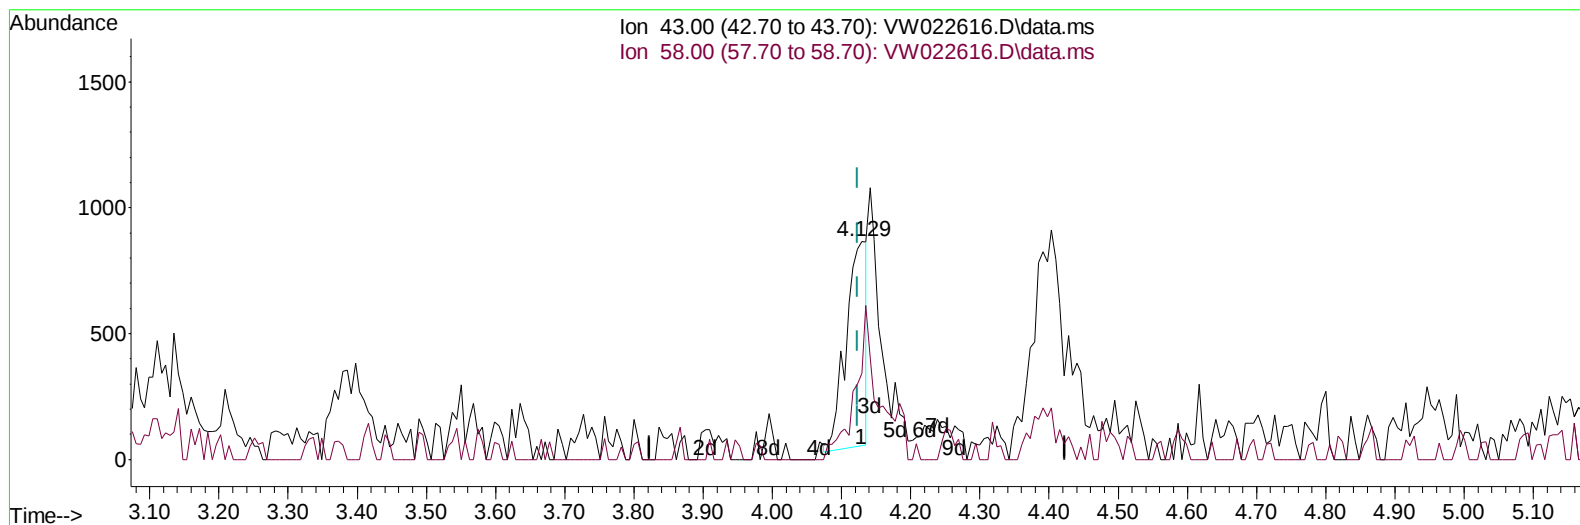

TIC: VW022616.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 2.24 ug/L

response 1687

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	11.38
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022616.D
 Acq On : 26 Apr 2022 10:52
 Operator : SY/VA
 Sample : VW0426SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK486

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:38:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

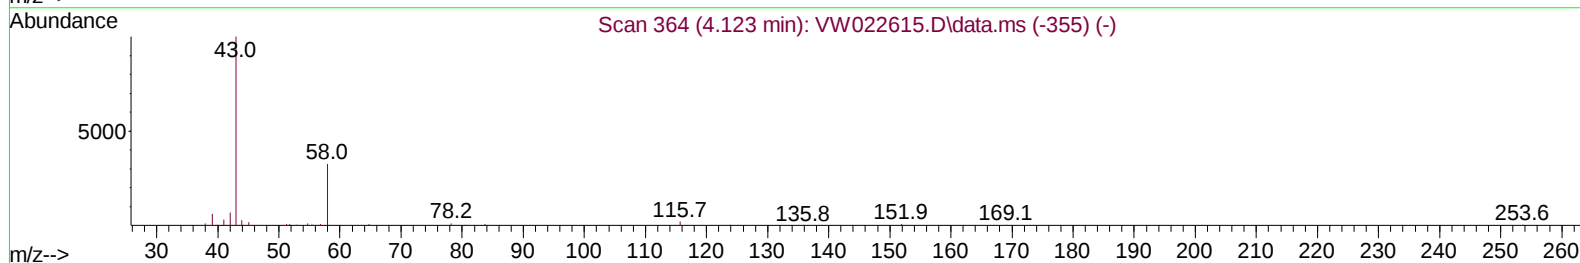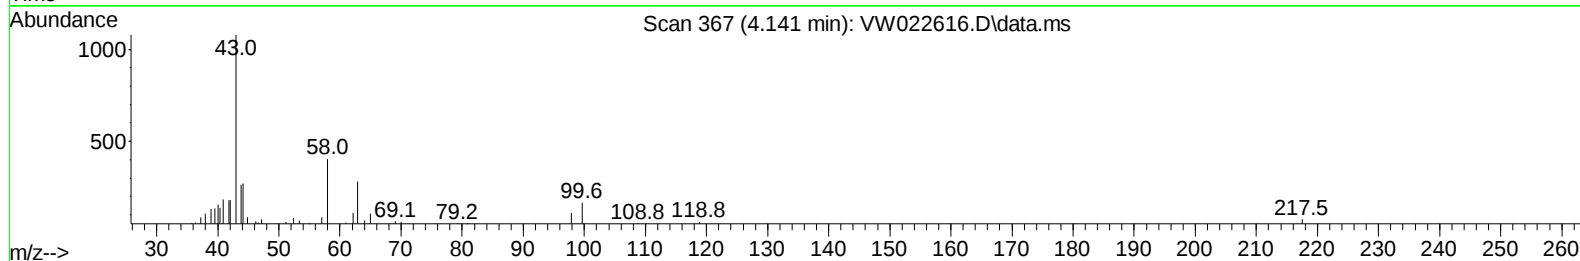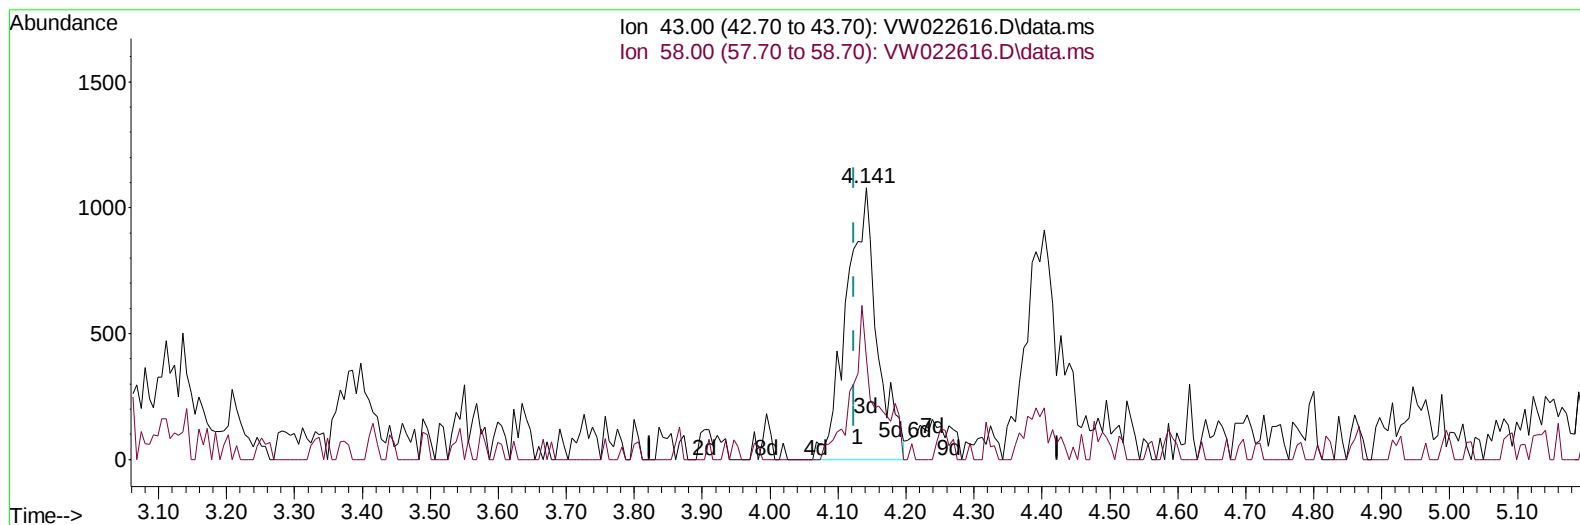

TIC: VW022616.D\data.ms

(13) Acetone (T)

4.141min (+ 0.018) 4.49 ug/L m

response 3383

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	5.68
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022616.D
 Acq On : 26 Apr 2022 10:52
 Operator : SY/VA
 Sample : VW0426SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK486

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:38:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

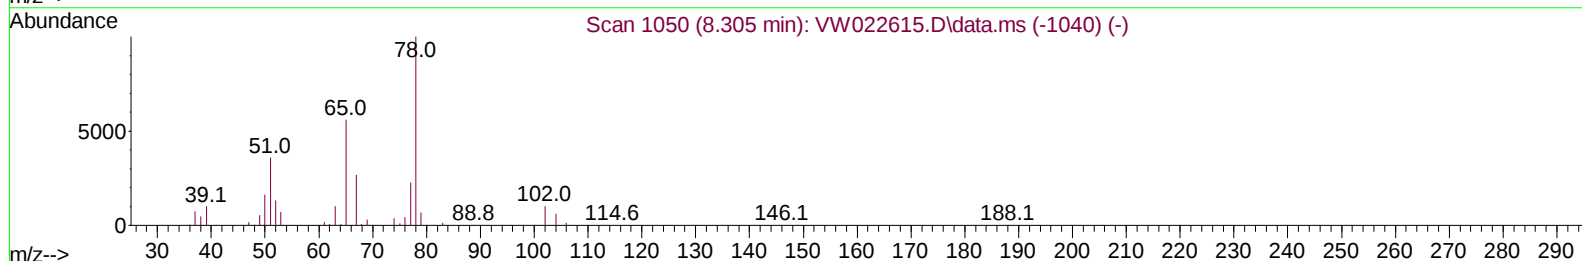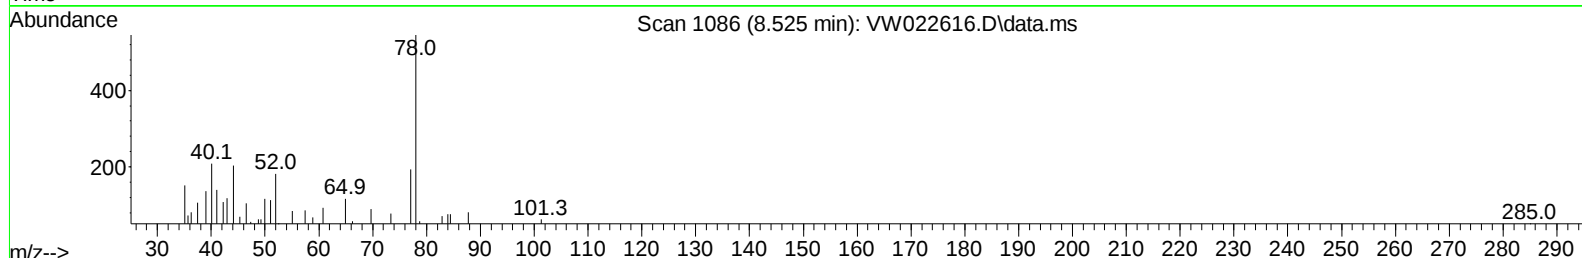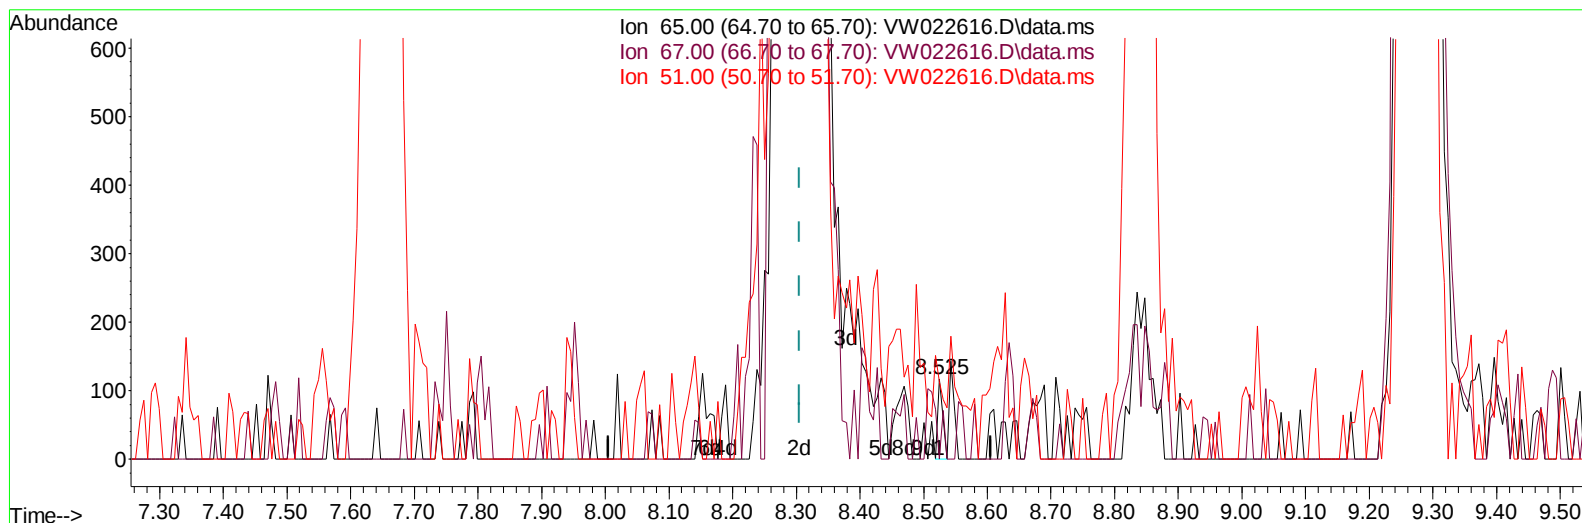

TIC: VW022616.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.525min (+ 0.220) 0.01 ug/L

response 64

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	40.63
51.00	99.30	101.56
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022616.D
Acq On : 26 Apr 2022 10:52
Operator : SY/VA
Sample : VW0426SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK486

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:38:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

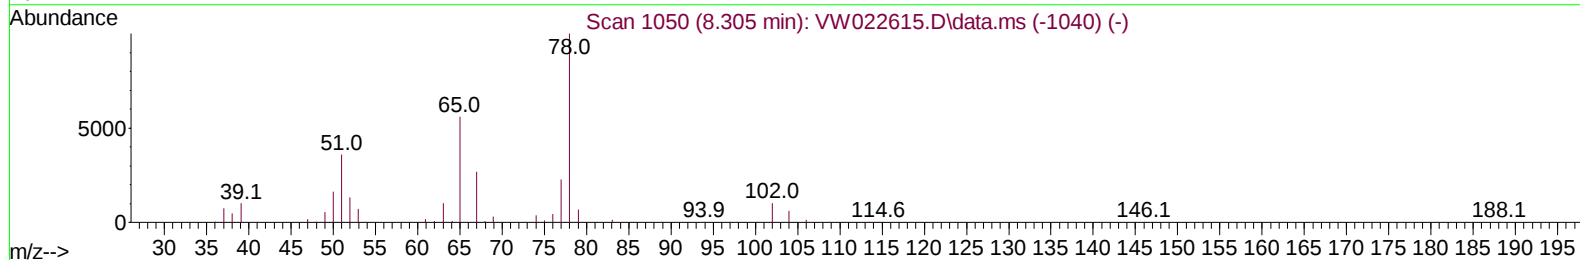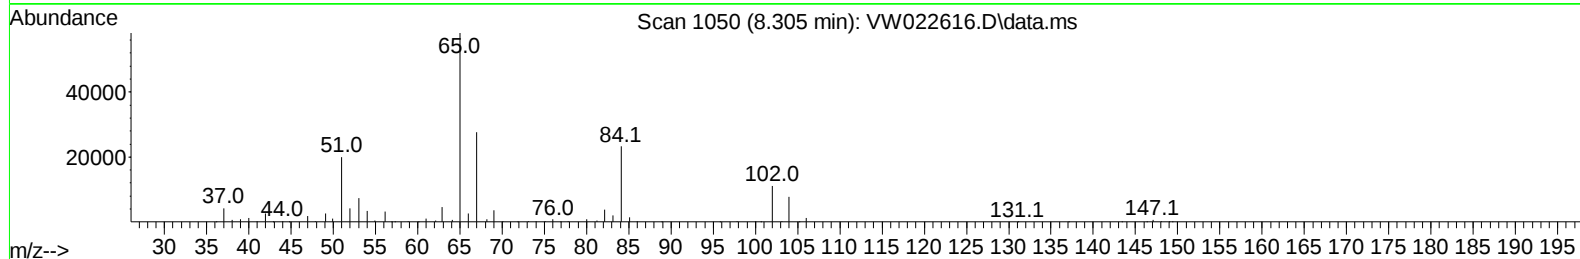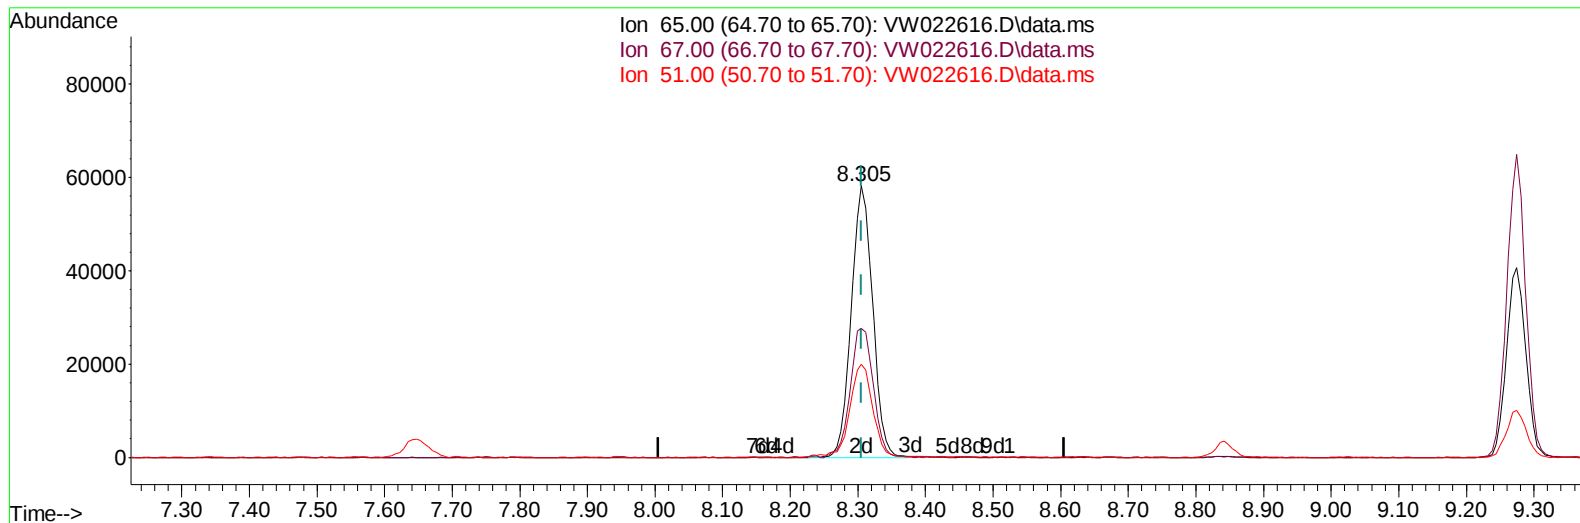

TIC: VW022616.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 24.83 ug/L m

response 127184

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.02#
51.00	99.30	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022616.D
 Acq On : 26 Apr 2022 10:52
 Operator : SY/VA
 Sample : VW0426SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK486

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:38:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		286777	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		280743	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		149596	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		137318	21.660	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	86.640%		
7) Chloroethane-d5	2.885	69		92712	23.334	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	93.320%		
11) 1,1-Dichloroethene-d2	4.013	63		151128	18.379	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110		Recovery =	73.520%		
21) 2-Butanone-d5	7.080	46		55972	50.569	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	101.140%		
24) Chloroform-d	7.653	84		225713	25.181	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	100.720%		
26) 1,2-Dichloroethane-d4	8.305	65		127184m	24.833	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	99.320%		
32) Benzene-d6	8.275	84		442595	25.804	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	103.200%		
36) 1,2-Dichloropropane-d6	9.274	67		125774	25.339	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	101.360%		
41) Toluene-d8	10.323	98		423974	25.238	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	100.960%		
43) trans-1,3-Dichloroprop...	10.579	79		52073	22.229	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	88.920%		
47) 2-Hexanone-d5	10.921	63		44970	48.695	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	97.380%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84		106050	25.127	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	100.520%		
66) 1,2-Dichlorobenzene-d4	13.853	152		140640	26.542	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	106.160%		
Target Compounds							
13) Acetone	4.141	43		3383m	4.489	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022616.D
Acq On : 26 Apr 2022 10:52
Operator : SY/VA
Sample : VW0426SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK486

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:38:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

