




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022617.D
 Acq On : 26 Apr 2022 11:16
 Operator : SY/VA
 Sample : N2469-03
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:38:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

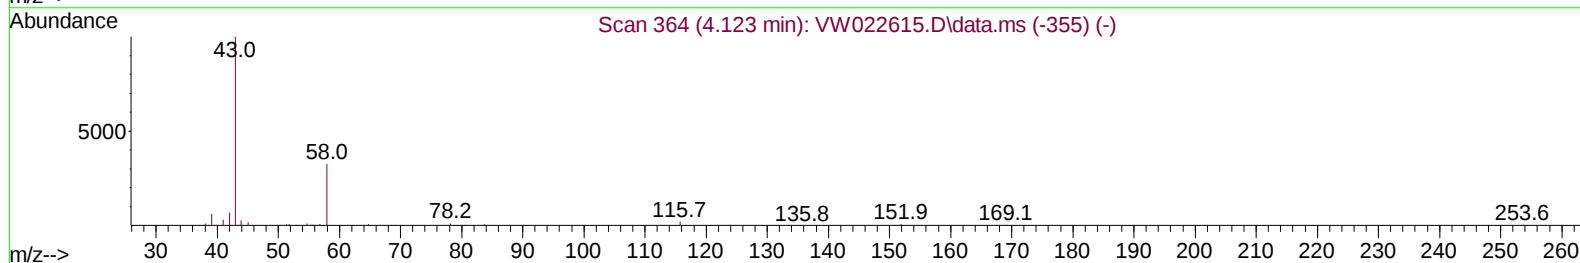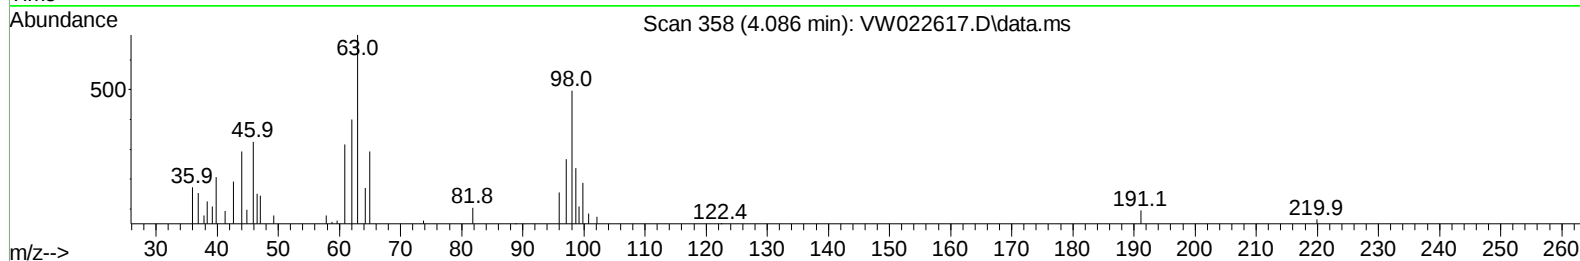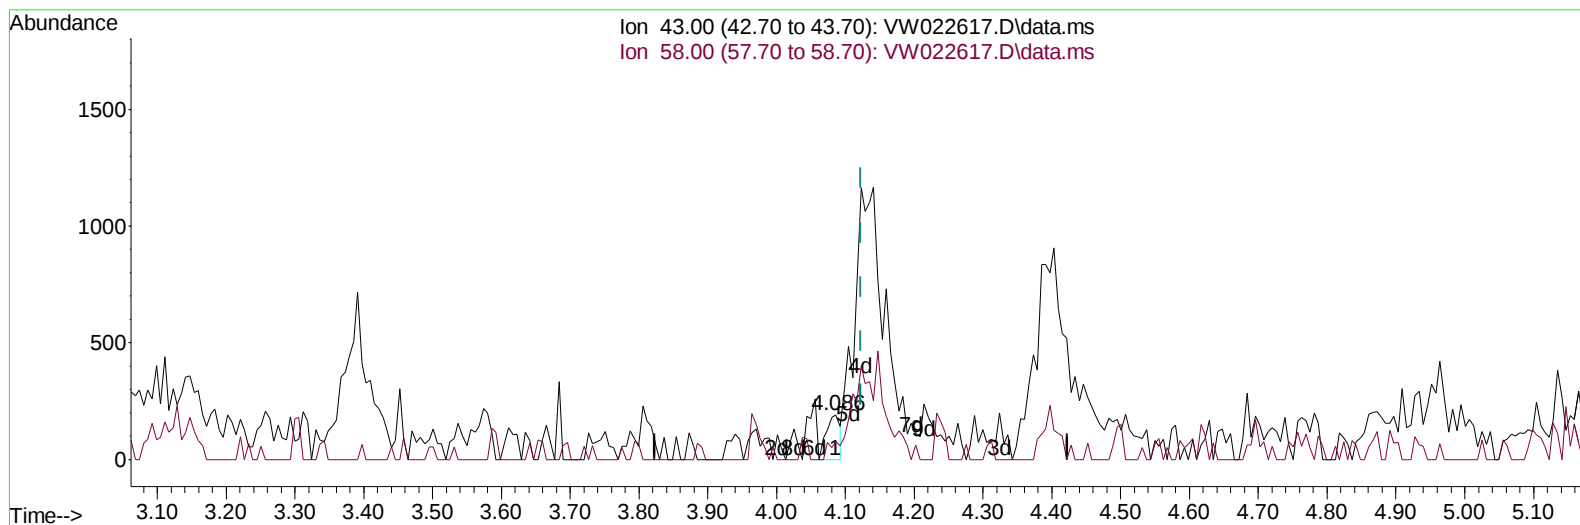

TIC: VW022617.D\data.ms

(13) Acetone (T)

4.086min (-0.037) 0.34 ug/L

response 268

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	16.79
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022617.D
 Acq On : 26 Apr 2022 11:16
 Operator : SY/VA
 Sample : N2469-03
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:38:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

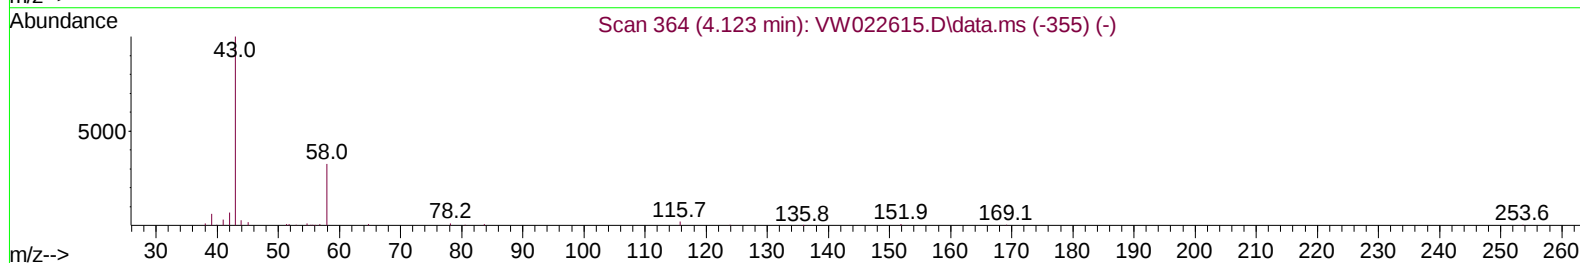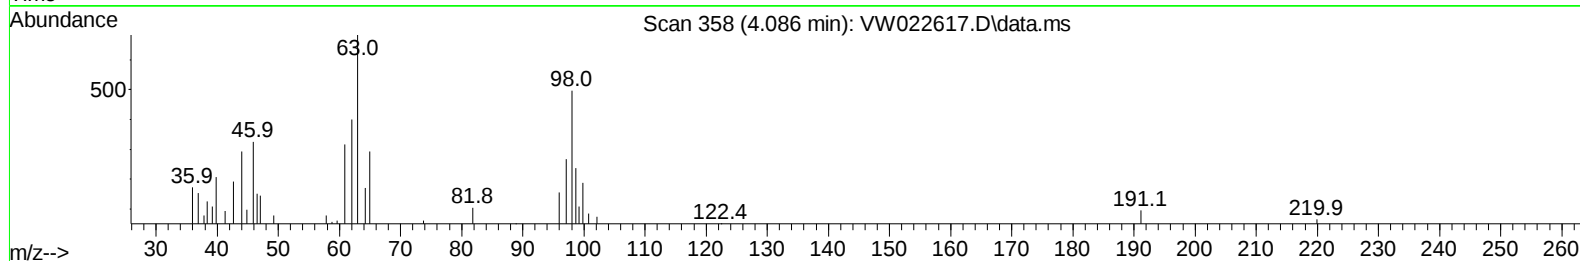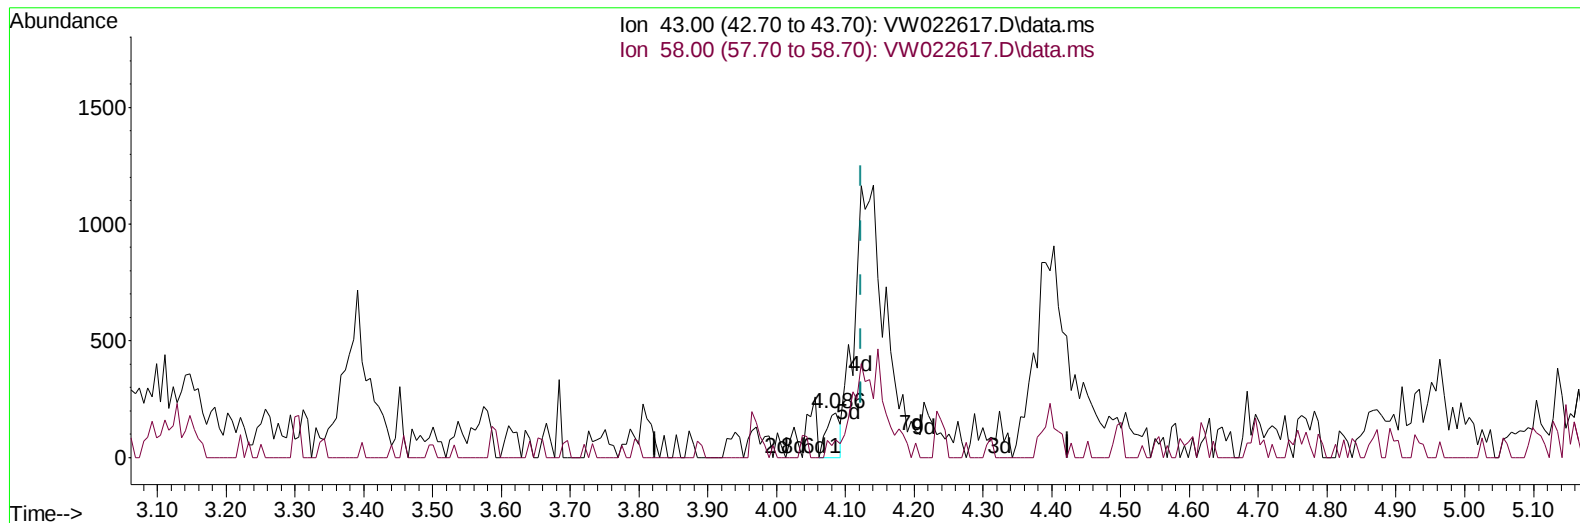

TIC: VW022617.D\data.ms

(13) Acetone (T)

4.086min (-0.037) 0.34 ug/L

response 268

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	16.79
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022617.D
 Acq On : 26 Apr 2022 11:16
 Operator : SY/VA
 Sample : N2469-03
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:38:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

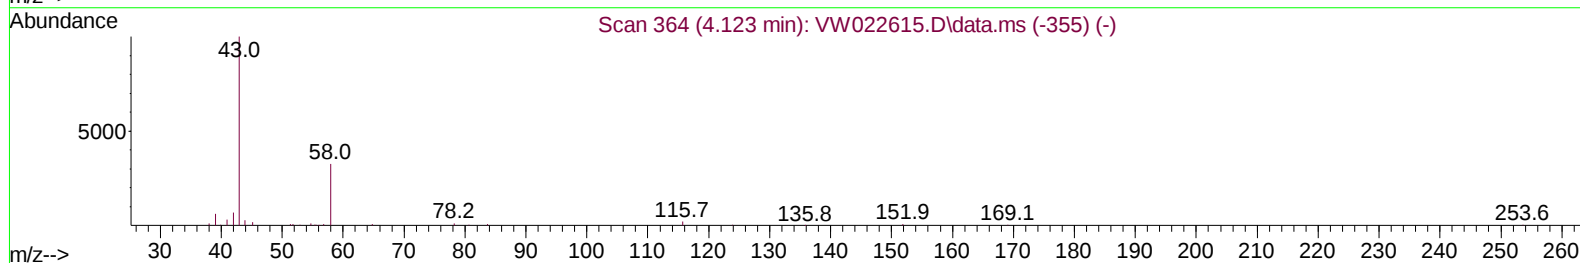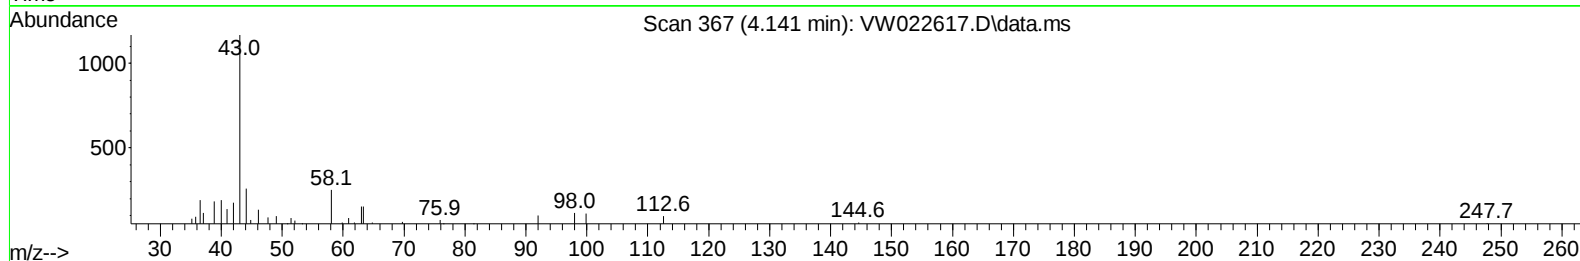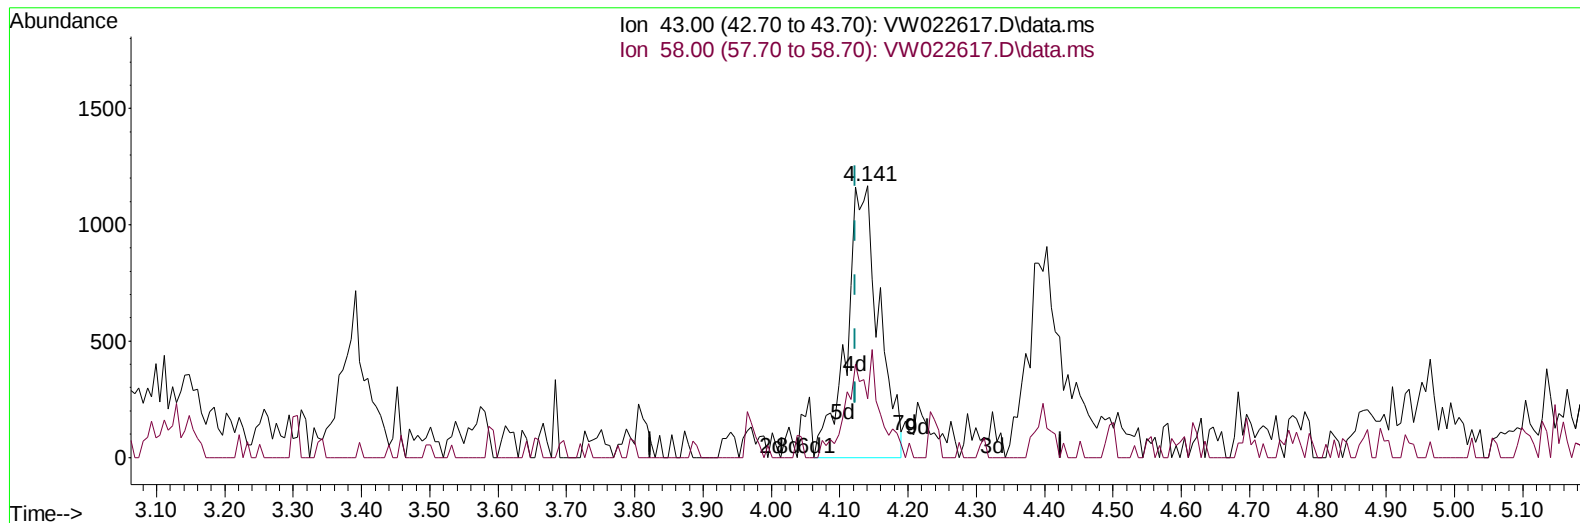

TIC: VW022617.D\data.ms

(13) Acetone (T)

4.141min (+ 0.018) 4.94 ug/L m

response 3842

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	1.17
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022617.D
 Acq On : 26 Apr 2022 11:16
 Operator : SY/VA
 Sample : N2469-03
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:38:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		296012	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		288673	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		148283	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		127594	19.498	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	78.000%	
7) Chloroethane-d5	2.885	69		85473	20.841	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	83.360%	
11) 1,1-Dichloroethene-d2	4.013	63		139743	16.464	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110		Recovery	=	65.840%	
21) 2-Butanone-d5	7.073	46		56673	49.605	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	99.220%	
24) Chloroform-d	7.647	84		215989	23.344	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	93.360%	
26) 1,2-Dichloroethane-d4	8.305	65		123855	23.429	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	93.720%	
32) Benzene-d6	8.274	84		418900	23.752	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	95.000%	
36) 1,2-Dichloropropane-d6	9.274	67		120913	23.690	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	94.760%	
41) Toluene-d8	10.323	98		395354	22.888	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	91.560%	
43) trans-1,3-Dichloroprop...	10.579	79		49208	20.429	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	81.720%	
47) 2-Hexanone-d5	10.926	63		46448	48.914	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	97.820%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		104059	23.978	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	95.920%	
66) 1,2-Dichlorobenzene-d4	13.847	152		125749	23.942	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	95.760%	
Target Compounds							Qvalue
13) Acetone	4.141	43		3842m	4.939	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022617.D
Acq On : 26 Apr 2022 11:16
Operator : SY/VA
Sample : N2469-03
Misc : 5.01g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:38:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

