




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022618.D
 Acq On : 26 Apr 2022 11:40
 Operator : SY/VA
 Sample : N2470-04
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:38:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

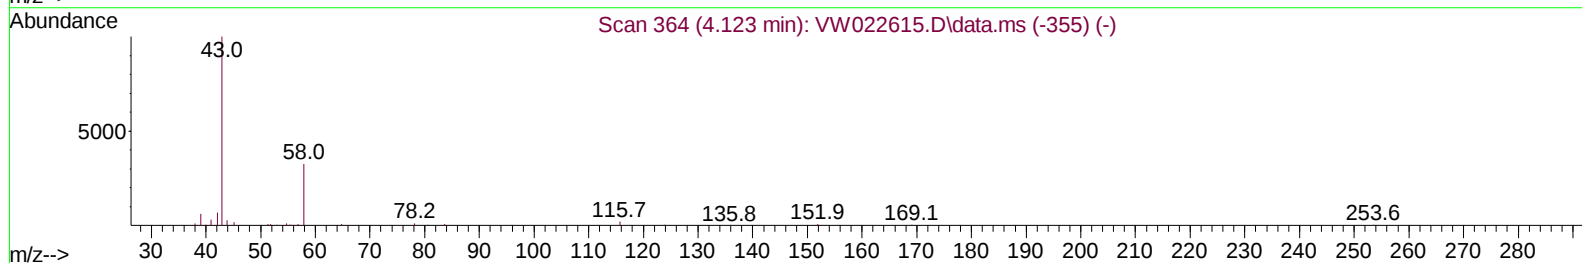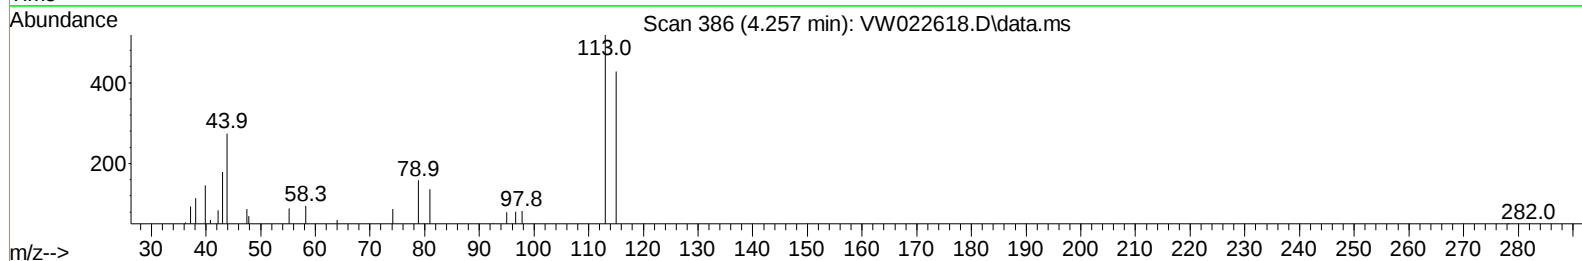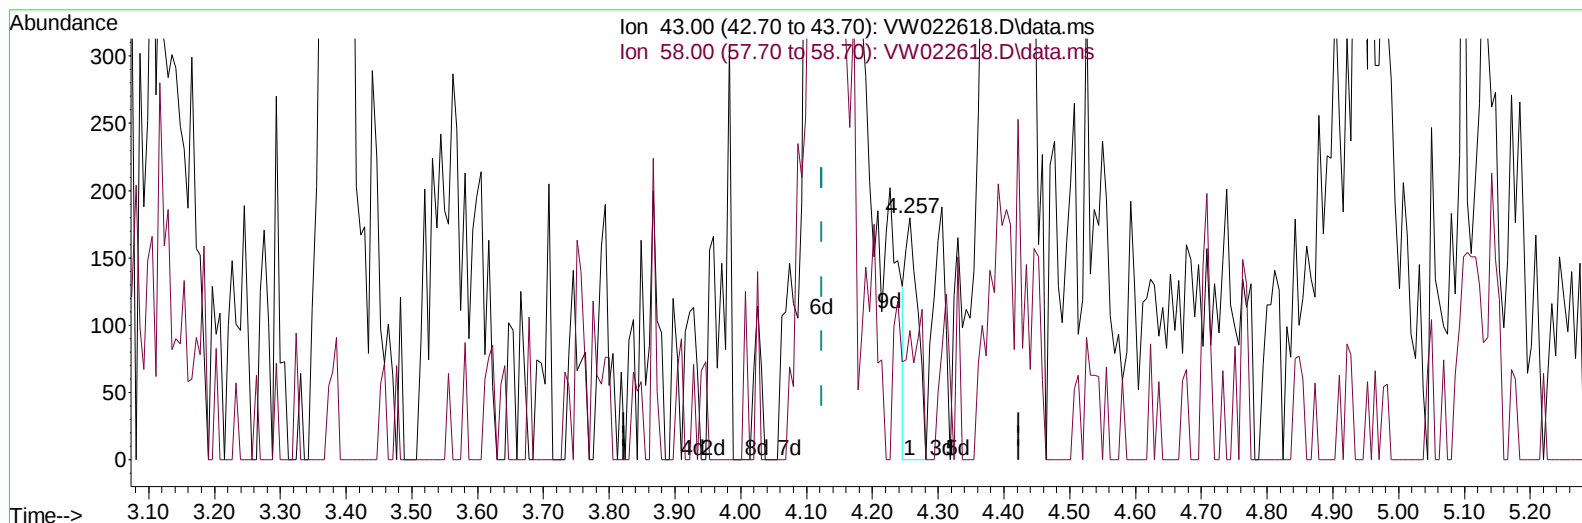

TIC: VW022618.D\data.ms

(13) Acetone (T)

4.257min (+ 0.134) 0.30 ug/L

response 240

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	4.17
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022618.D
 Acq On : 26 Apr 2022 11:40
 Operator : SY/VA
 Sample : N2470-04
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:38:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

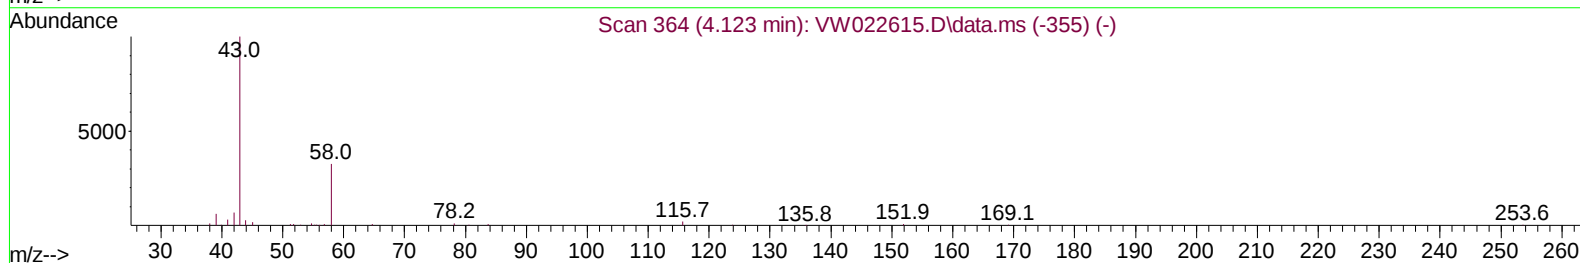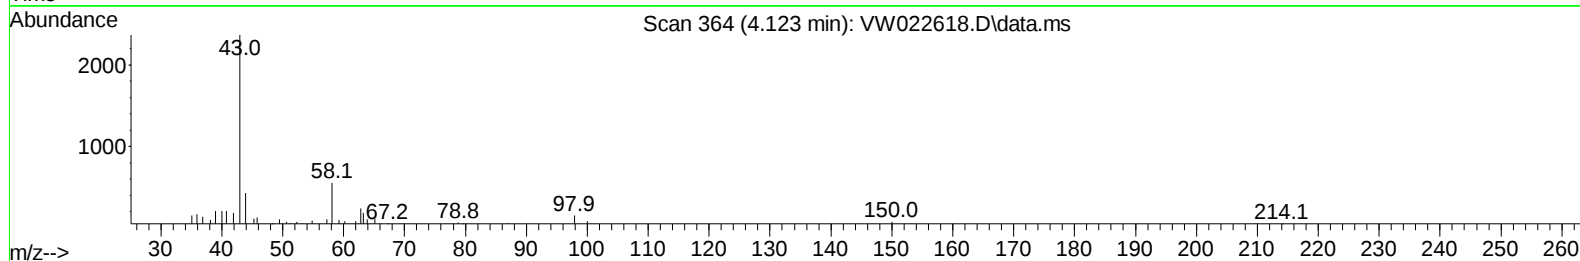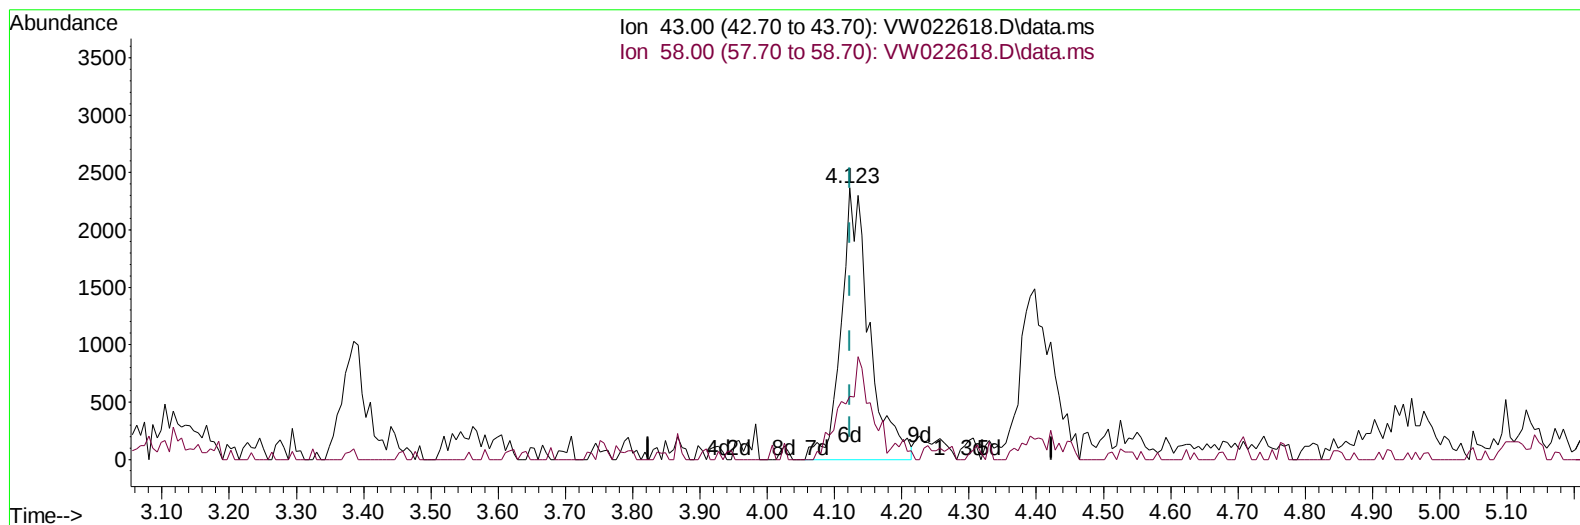

TIC: VW022618.D\data.ms

(13) Acetone (T)

4.123min (0.000) 8.58 ug/L m

response 6891

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	0.15
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022618.D
 Acq On : 26 Apr 2022 11:40
 Operator : SY/VA
 Sample : N2470-04
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:38:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	305670	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	290728	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	149738	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	134754	19.942	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	79.760%	
7) Chloroethane-d5	2.885	69	91018	21.492	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	85.960%	
11) 1,1-Dichloroethene-d2	4.013	63	142058	16.208	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	64.840%	
21) 2-Butanone-d5	7.074	46	52251	44.290	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	88.580%	
24) Chloroform-d	7.647	84	217506	22.765	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	91.080%	
26) 1,2-Dichloroethane-d4	8.305	65	122919	22.517	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	90.080%	
32) Benzene-d6	8.275	84	431480	24.292	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	97.160%	
36) 1,2-Dichloropropane-d6	9.274	67	122462	23.824	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	95.280%	
41) Toluene-d8	10.323	98	405392	23.303	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	93.200%	
43) trans-1,3-Dichloroprop...	10.579	79	48509	19.996	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	80.000%	
47) 2-Hexanone-d5	10.921	63	44767	46.810	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	93.620%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	103071	23.583	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	94.320%	
66) 1,2-Dichlorobenzene-d4	13.853	152	135029	25.459	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	101.840%	
Target Compounds						
13) Acetone	4.123	43	6891m	8.579	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022618.D
Acq On : 26 Apr 2022 11:40
Operator : SY/VA
Sample : N2470-04
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:38:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

