




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022620.D
 Acq On : 26 Apr 2022 13:07
 Operator : SY/VA
 Sample : N2562-02
 Misc : 6.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW462

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:39:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

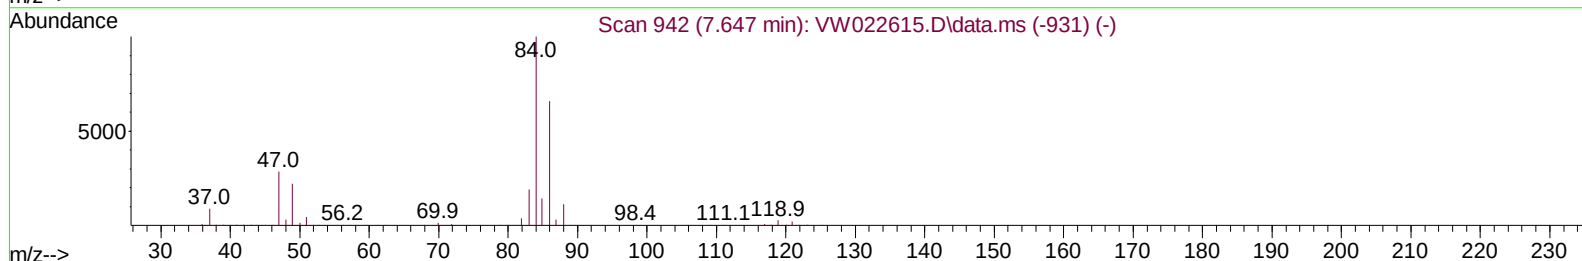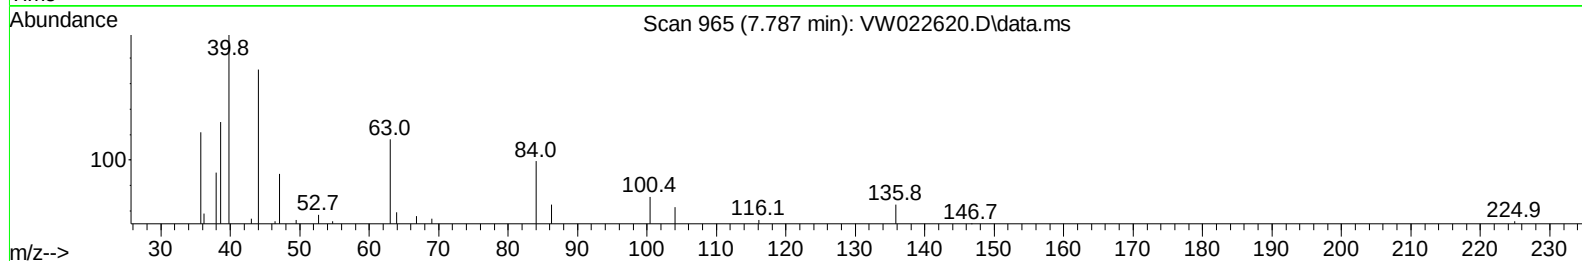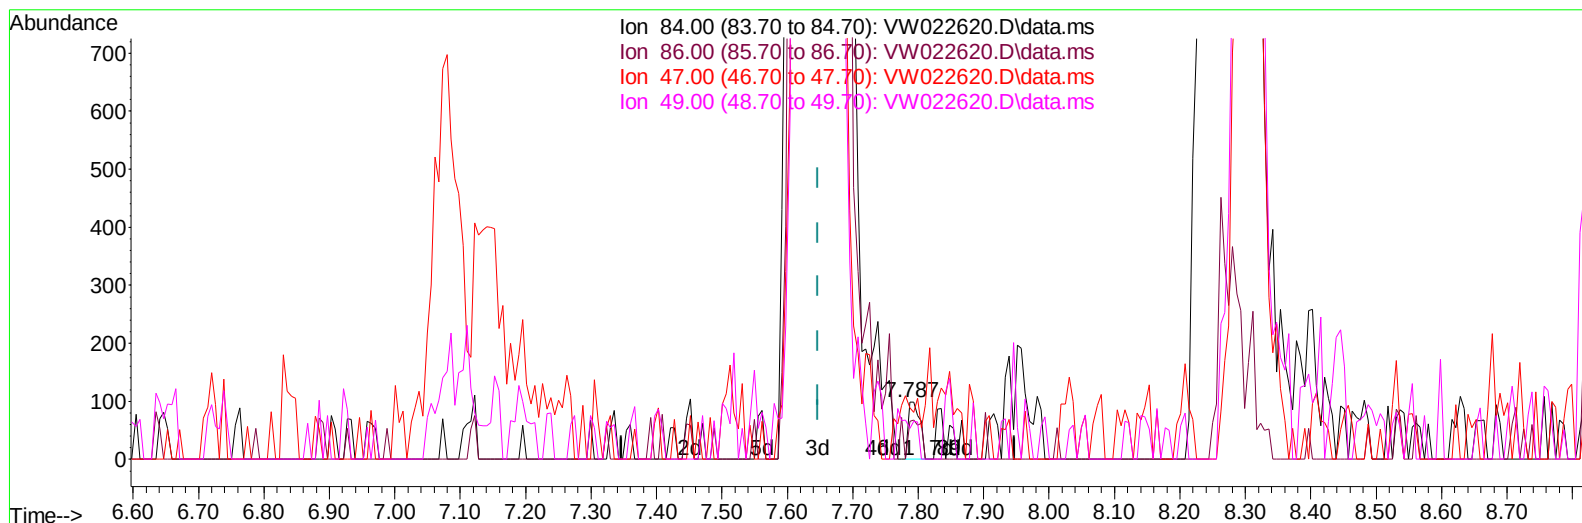

TIC: VW022620.D\data.ms

(24) Chloroform-d (S)

7.787min (+ 0.140) 0.01 ug/L

response 124

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.80	56.45
47.00	51.50	46.77
49.00	31.80	38.71




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022620.D
 Acq On : 26 Apr 2022 13:07
 Operator : SY/VA
 Sample : N2562-02
 Misc : 6.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW462

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:39:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

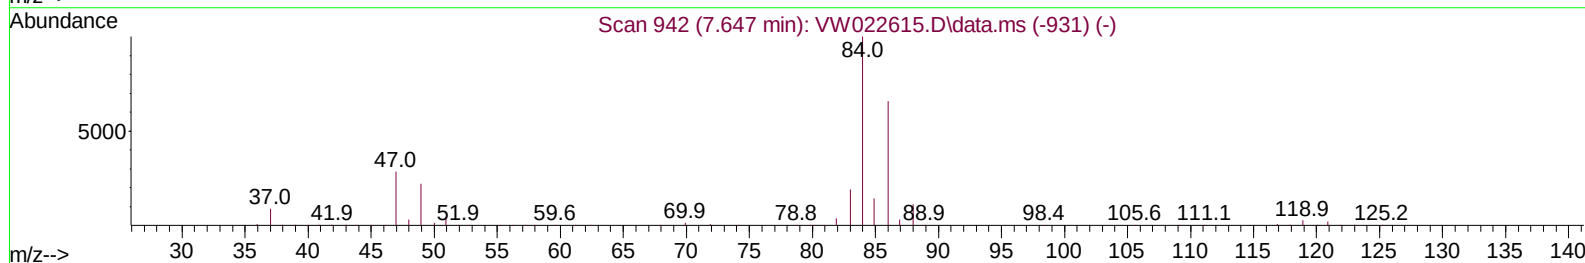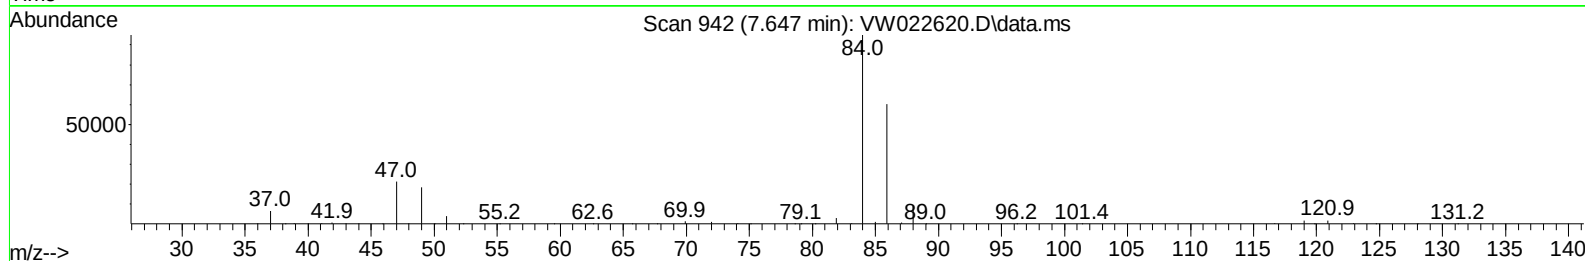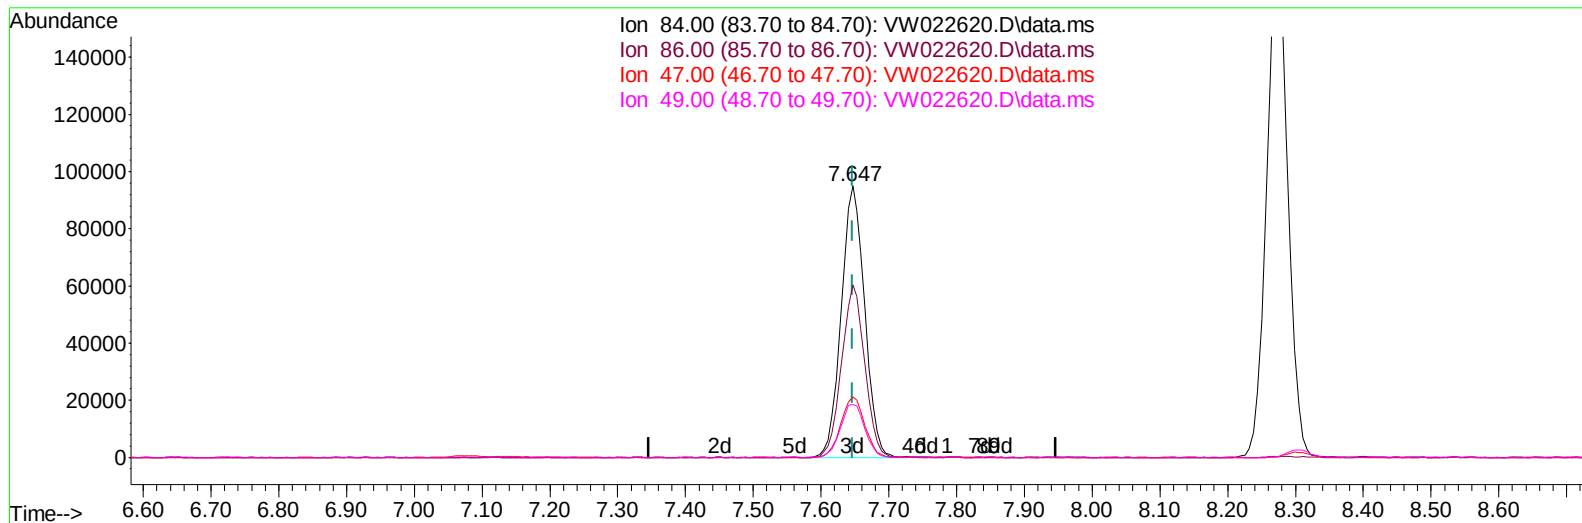

TIC: VW022620.D\data.ms

(24) Chloroform-d (S)

7.647min (-0.000) 20.51 ug/L m

response 227840

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.80	0.03#
47.00	51.50	0.03#
49.00	31.80	0.02#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022620.D
Acq On : 26 Apr 2022 13:07
Operator : SY/VA
Sample : N2562-02
Misc : 6.90g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW462

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:39:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

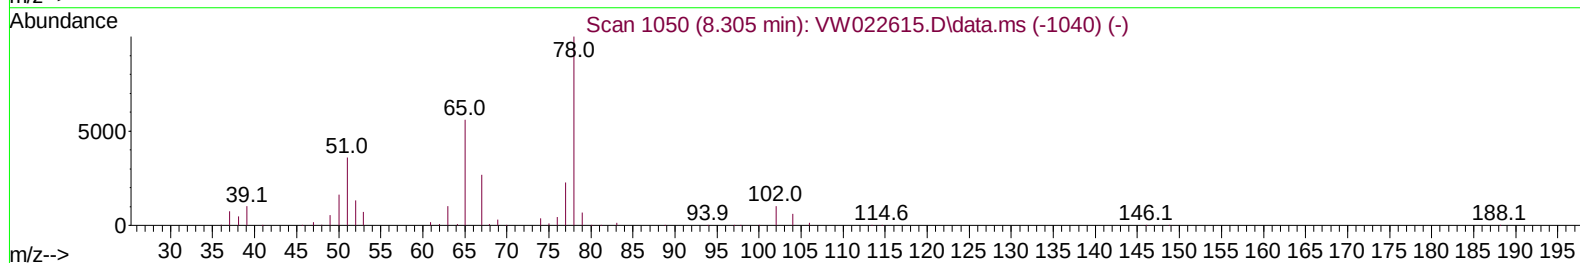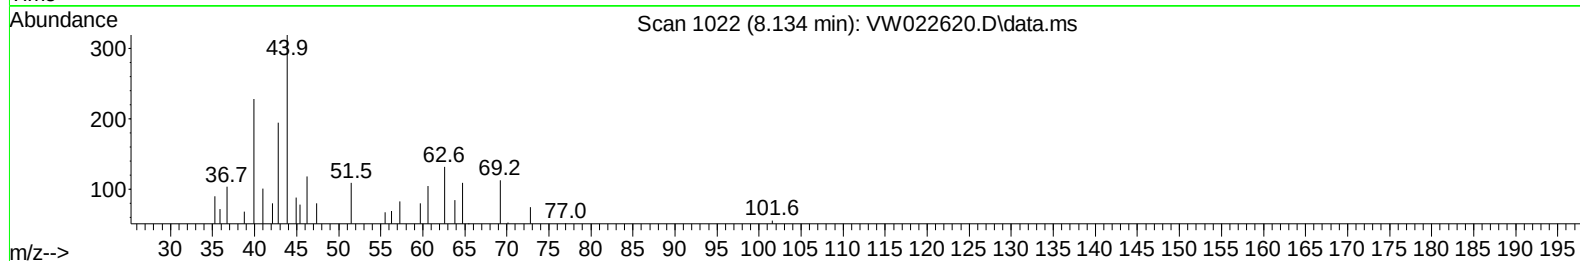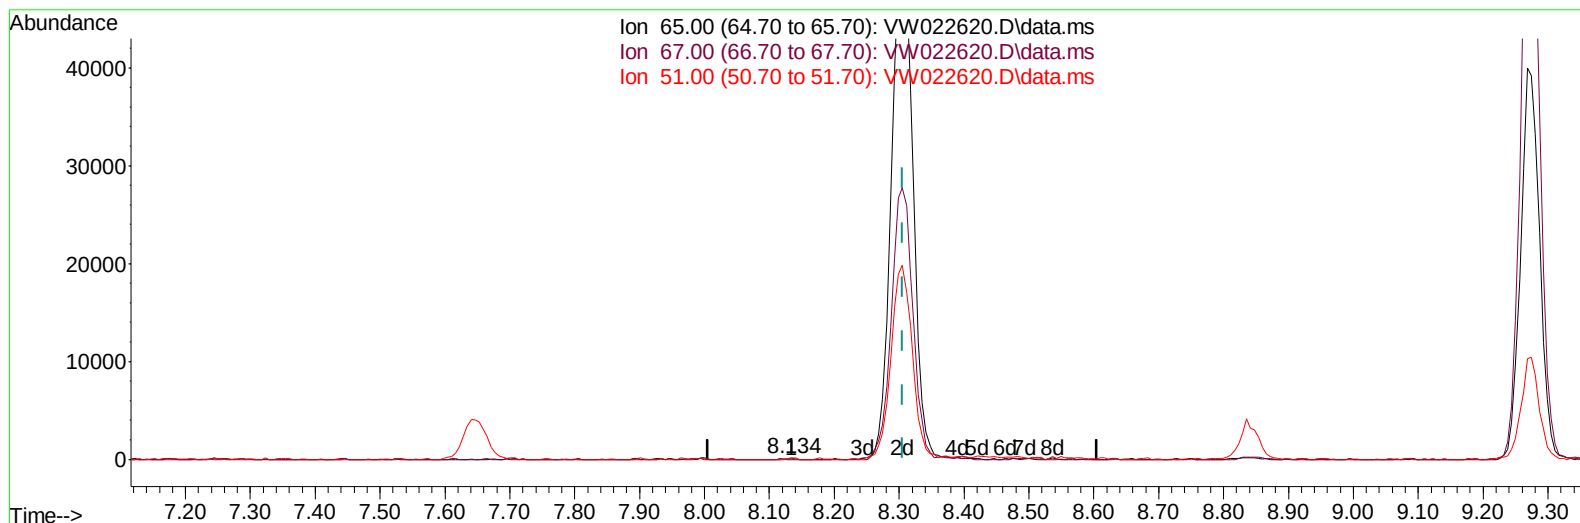

TIC: VW022620.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.134min (-0.171) 0.02 ug/L

response 118

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	53.39
51.00	99.30	101.69
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022620.D
Acq On : 26 Apr 2022 13:07
Operator : SY/VA
Sample : N2562-02
Misc : 6.90g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW462

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:39:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

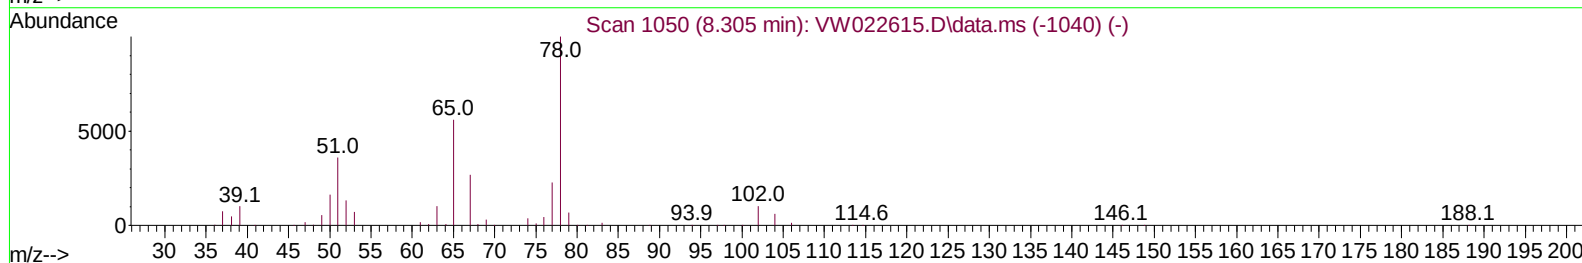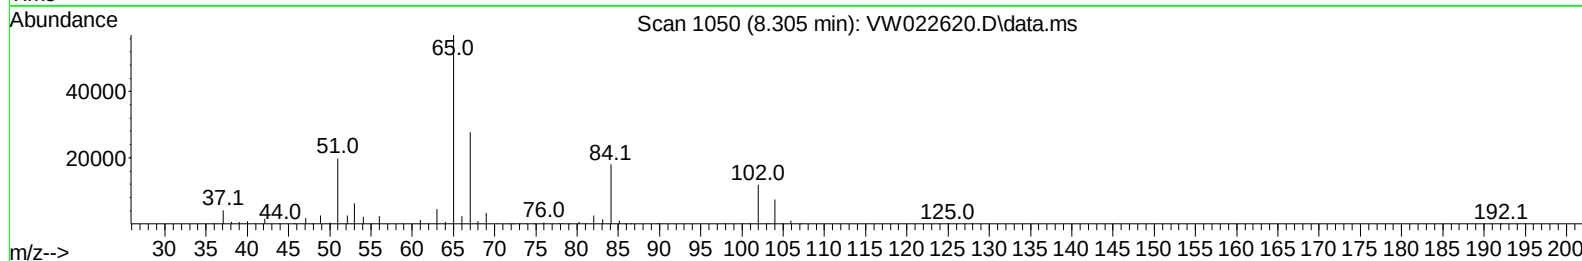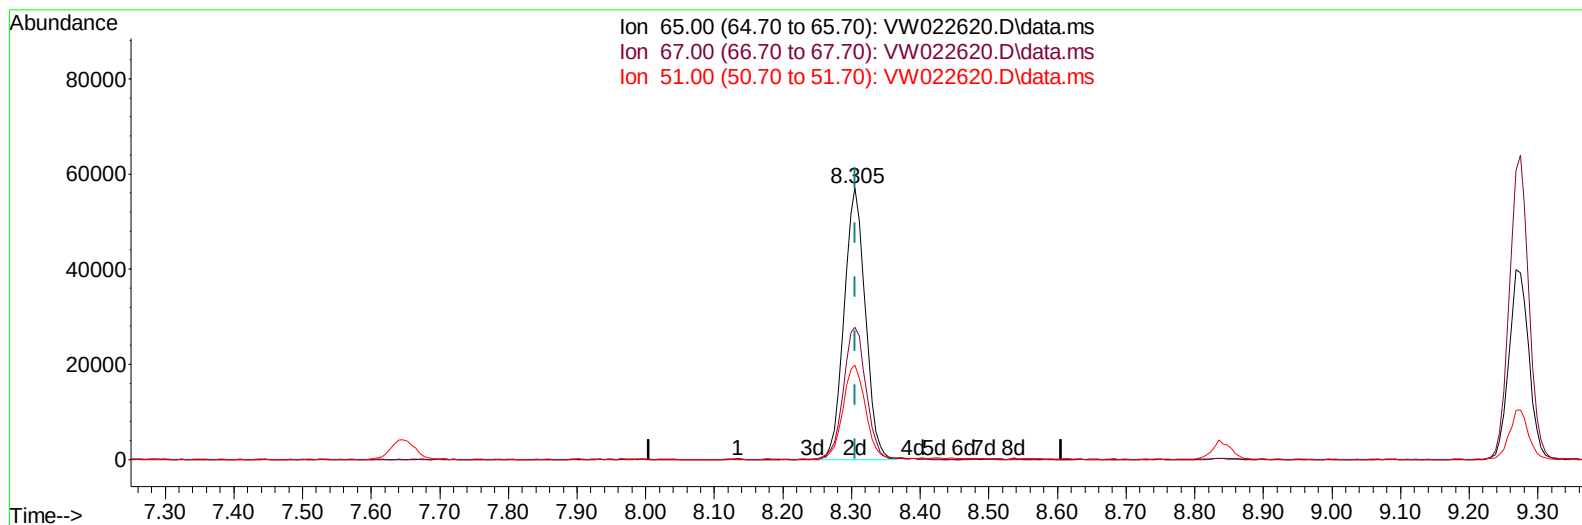

TIC: VW022620.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 19.31 ug/L m

response 122605

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.05#
51.00	99.30	0.10#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022620.D
 Acq On : 26 Apr 2022 13:07
 Operator : SY/VA
 Sample : N2562-02
 Misc : 6.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW462

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:39:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		355444	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		264806	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		73681	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		103329	13.150	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	52.600%		
7) Chloroethane-d5	2.885	69		78646	15.970	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	63.880%		
11) 1,1-Dichloroethene-d2	4.013	63		109127	10.707	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110		Recovery =	42.840%#		
21) 2-Butanone-d5	7.074	46		68239	49.742	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	99.480%		
24) Chloroform-d	7.647	84		227840m	20.508	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	82.040%		
26) 1,2-Dichloroethane-d4	8.305	65		122605m	19.314	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	77.240%		
32) Benzene-d6	8.275	84		382258	23.627	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	94.520%		
36) 1,2-Dichloropropane-d6	9.274	67		126480	27.015	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	108.040%		
41) Toluene-d8	10.323	98		303442	19.150	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	76.600%		
43) trans-1,3-Dichloroprop...	10.573	79		39130	17.709	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	70.840%		
47) 2-Hexanone-d5	10.920	63		49964	57.359	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	114.720%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		114609	28.789	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	115.160%		
66) 1,2-Dichlorobenzene-d4	13.853	152		68340	26.186	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	104.760%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022620.D
Acq On : 26 Apr 2022 13:07
Operator : SY/VA
Sample : N2562-02
Misc : 6.90g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW462

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:39:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

