




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022622.D
 Acq On : 26 Apr 2022 14:14
 Operator : SY/VA
 Sample : N2562-01
 Misc : 6.94g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW461

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:39:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

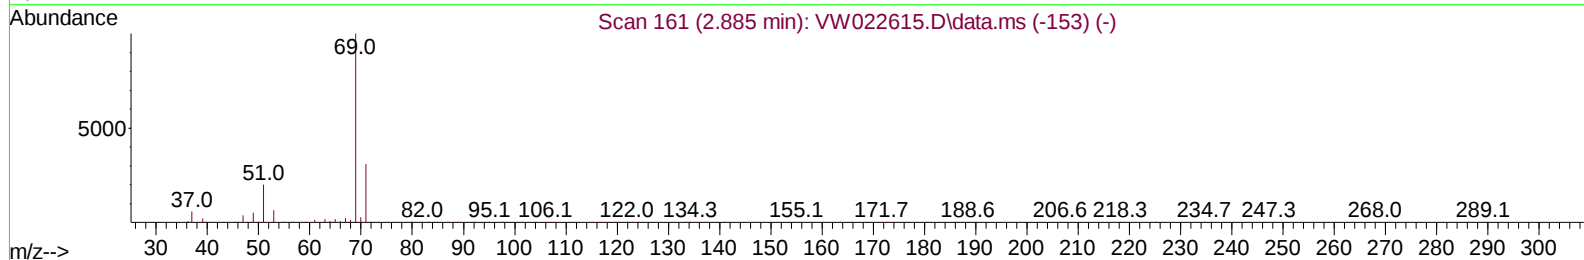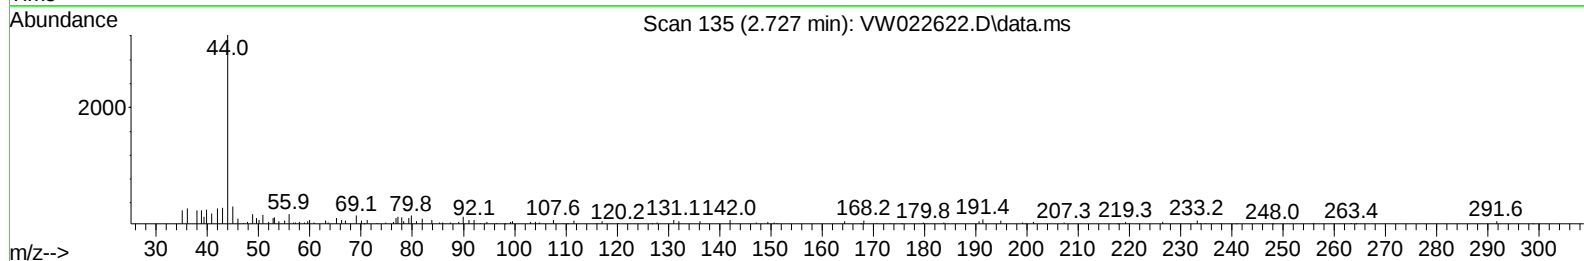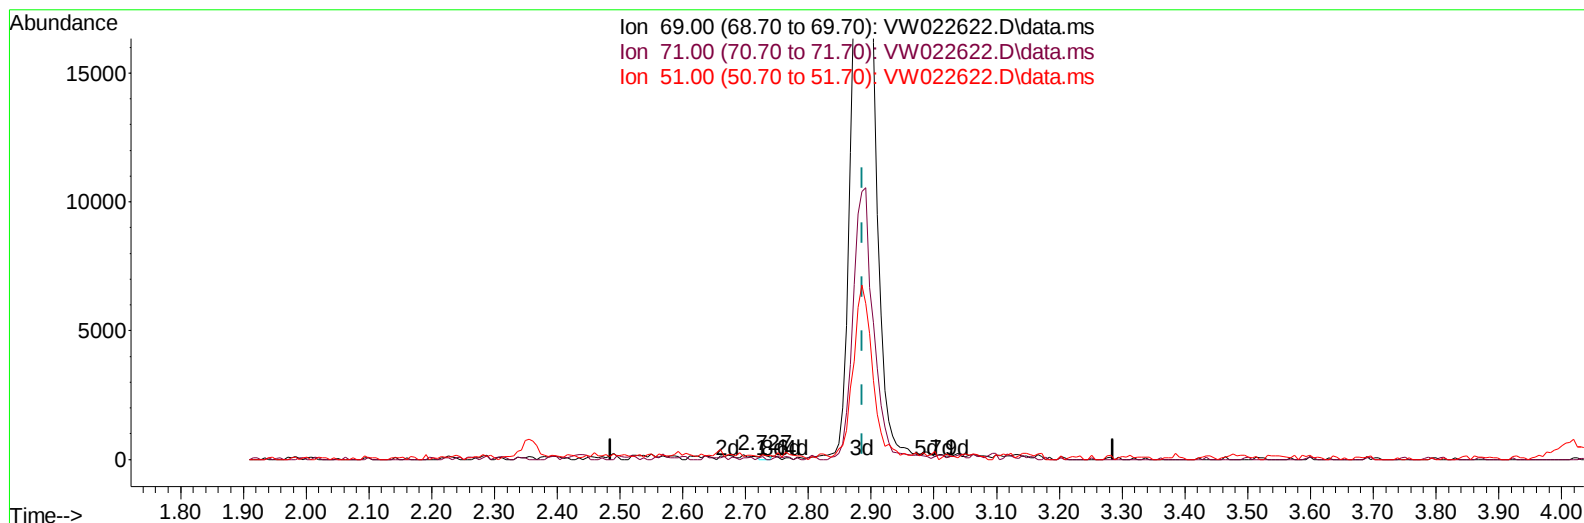

TIC: VW022622.D\data.ms

(7) Chloroethane-d5 (S)

2.727min (-0.158) 0.03 ug/L

response 150

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.80	42.00
51.00	28.60	31.33
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022622.D
 Acq On : 26 Apr 2022 14:14
 Operator : SY/VA
 Sample : N2562-01
 Misc : 6.94g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW461

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:39:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

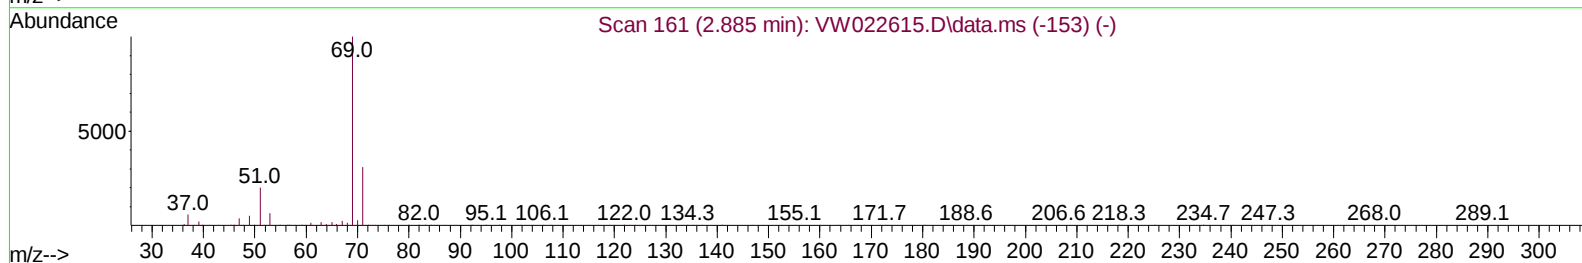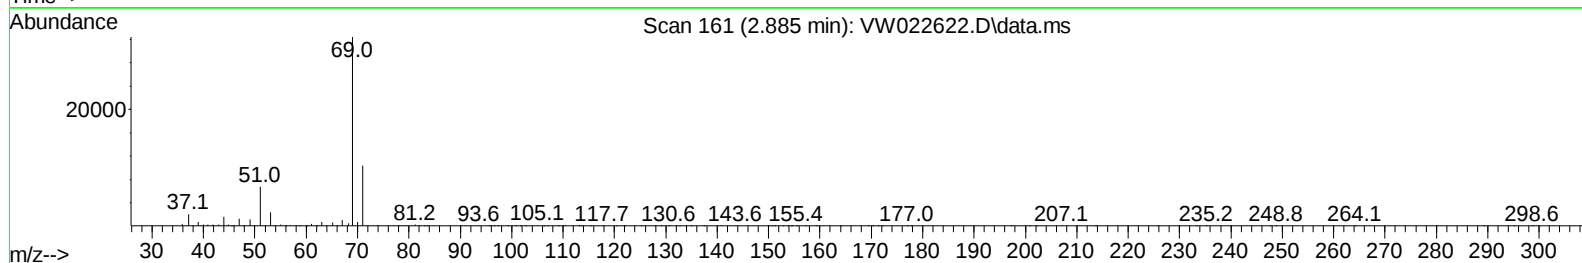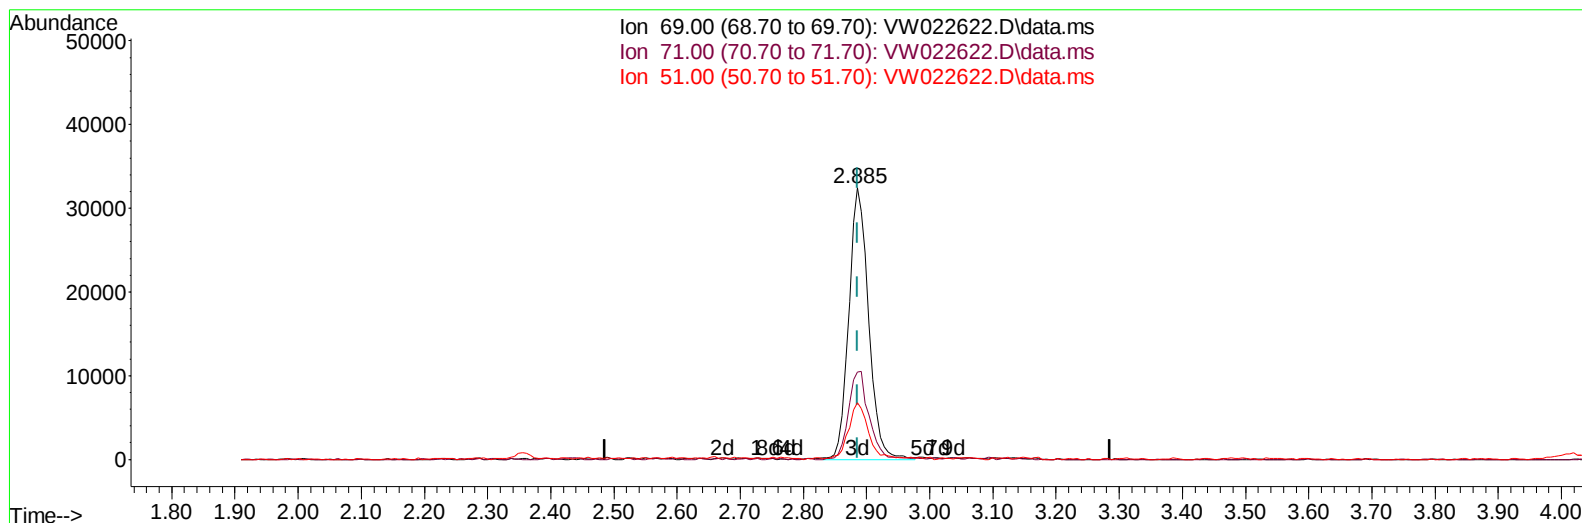

TIC: VW022622.D\data.ms

(7) Chloroethane-d5 (S)

2.885min (+ 0.000) 15.77 ug/L m

response 70548

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.80	0.09#
51.00	28.60	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022622.D
 Acq On : 26 Apr 2022 14:14
 Operator : SY/VA
 Sample : N2562-01
 Misc : 6.94g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW461

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:39:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	322982	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	310056	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	141596	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	91886	12.869	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	51.480%	
7) Chloroethane-d5	2.885	69	70548m	15.765	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	63.080%	
11) 1,1-Dichloroethene-d2	4.013	63	101691	10.981	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	43.920%#	
21) 2-Butanone-d5	7.074	46	70539	56.586	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	113.180%	
24) Chloroform-d	7.647	84	208133	20.617	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	82.480%	
26) 1,2-Dichloroethane-d4	8.305	65	120200	20.839	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	83.360%	
32) Benzene-d6	8.275	84	360925	19.053	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	76.200%	
36) 1,2-Dichloropropane-d6	9.275	67	117332	21.403	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	85.600%	
41) Toluene-d8	10.323	98	318738	17.180	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	68.720%	
43) trans-1,3-Dichloroprop...	10.573	79	45890	17.738	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	70.960%	
47) 2-Hexanone-d5	10.921	63	56568	55.463	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	110.920%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	119754	25.692	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	102.760%	
66) 1,2-Dichlorobenzene-d4	13.853	152	112988	22.528	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	90.120%	
Target Compounds						
13) Acetone	4.123	43	10140	11.947	ug/L	Qvalue 88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022622.D
Acq On : 26 Apr 2022 14:14
Operator : SY/VA
Sample : N2562-01
Misc : 6.94g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW461

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:39:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

