




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022623.D
 Acq On : 26 Apr 2022 14:38
 Operator : SY/VA
 Sample : N2562-03
 Misc : 9.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW463

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:39:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

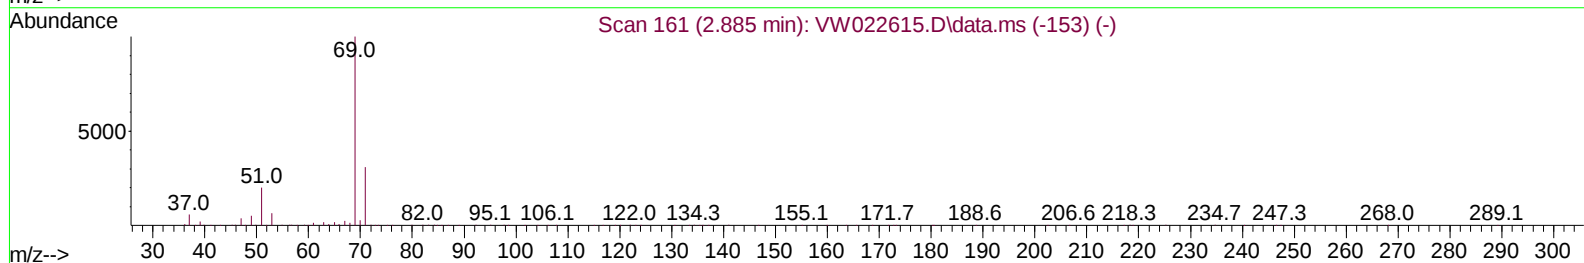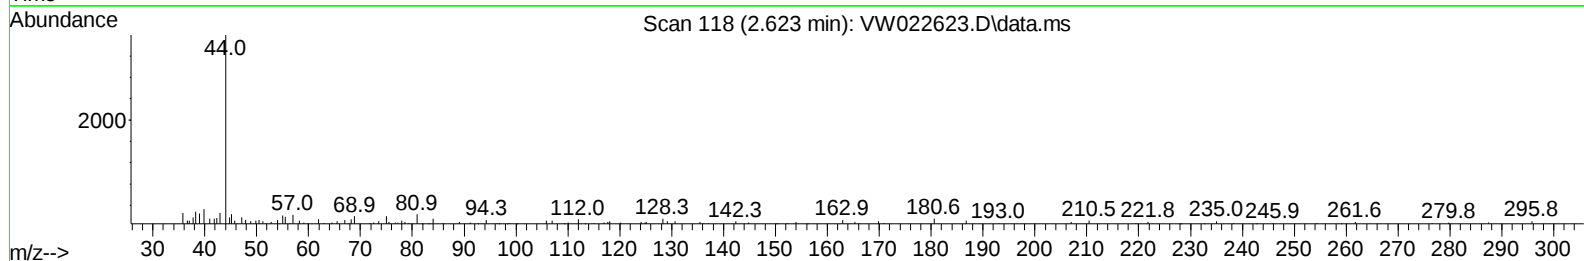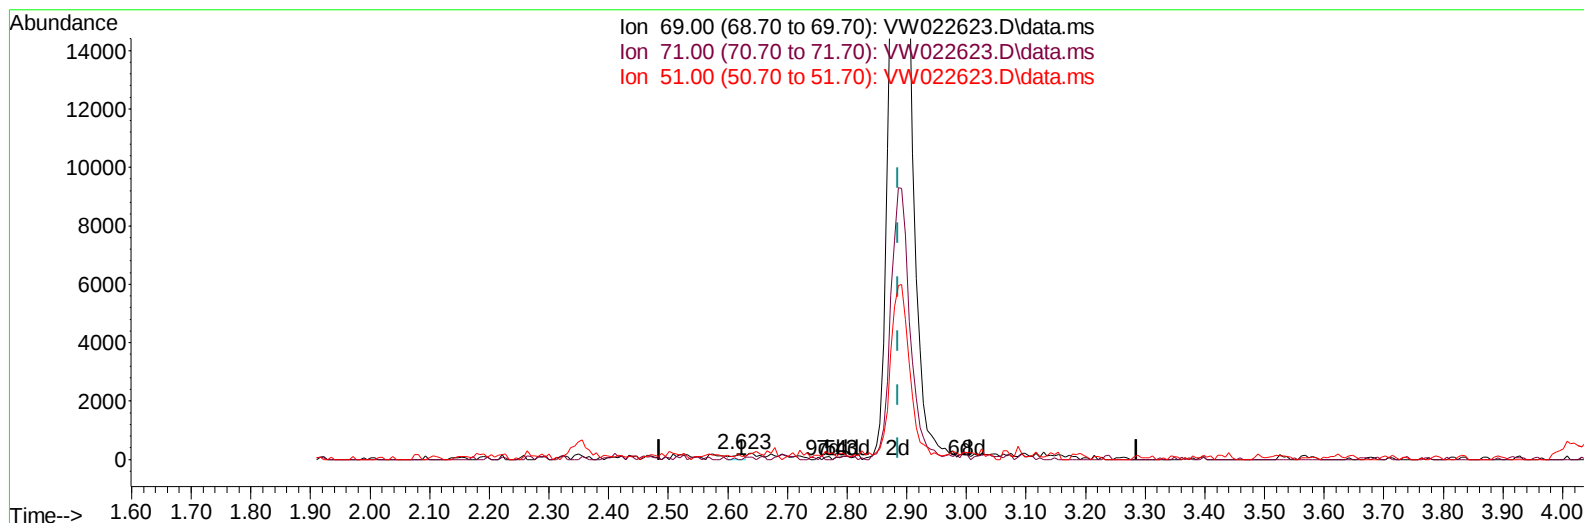

TIC: VW022623.D\data.ms

(7) Chloroethane-d5 (S)

2.623min (-0.262) 0.06 ug/L

response 236

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.80	36.44
51.00	28.60	23.73
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022623.D
 Acq On : 26 Apr 2022 14:38
 Operator : SY/VA
 Sample : N2562-03
 Misc : 9.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW463

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:39:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

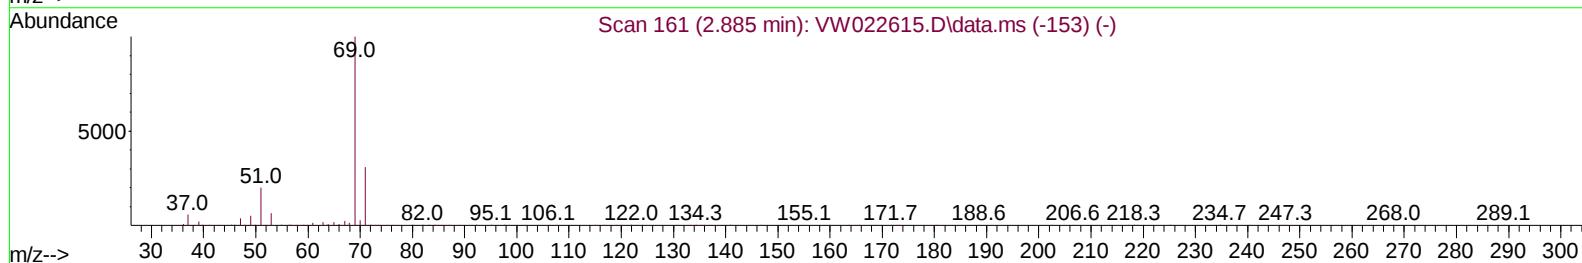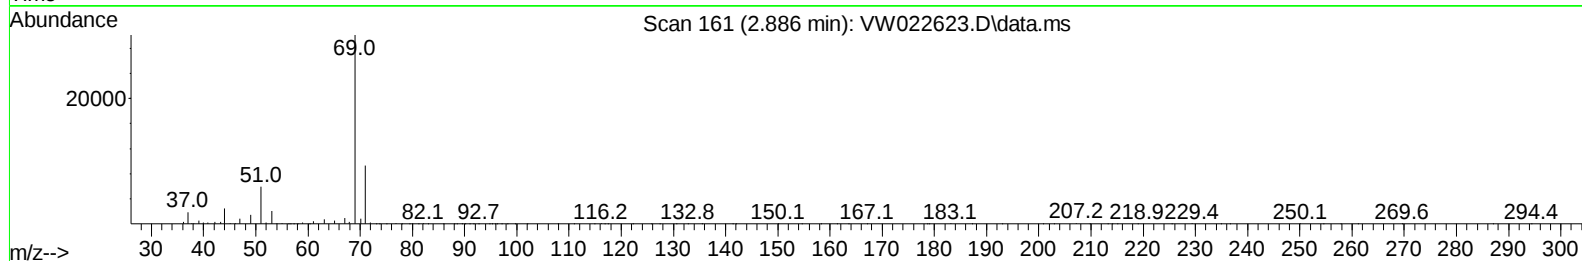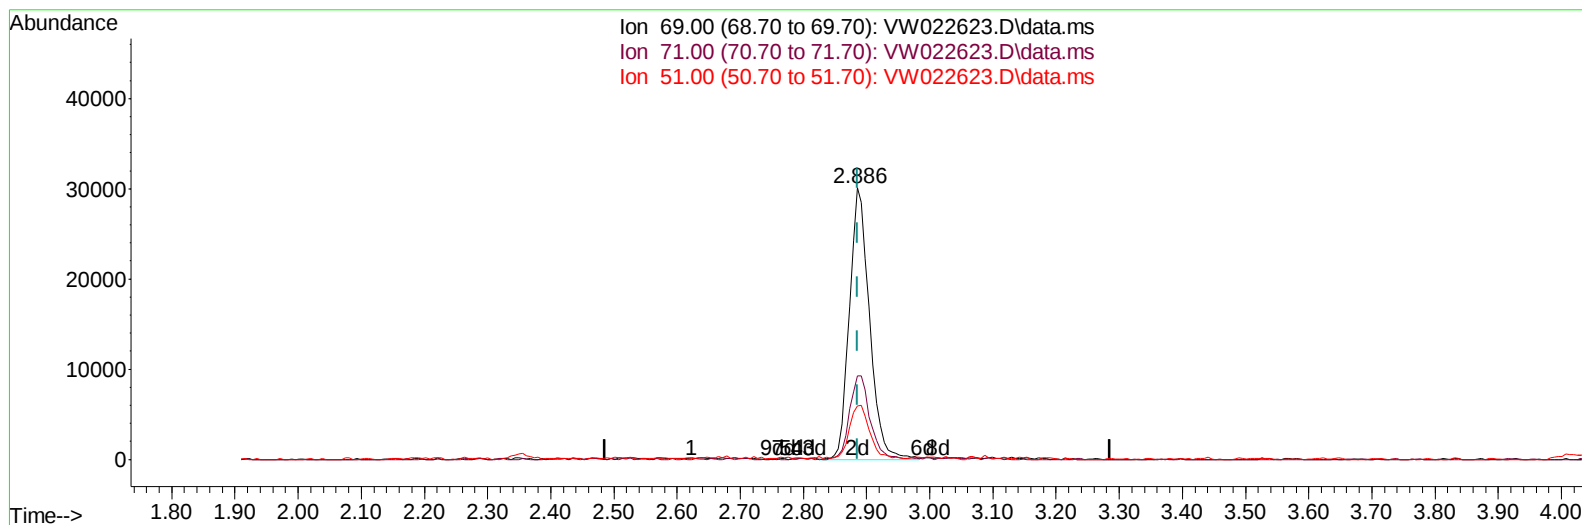

TIC: VW022623.D\data.ms

(7) Chloroethane-d5 (S)

2.886min (+ 0.000) 17.21 ug/L m

response 66703

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.80	0.13#
51.00	28.60	0.08#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022623.D
 Acq On : 26 Apr 2022 14:38
 Operator : SY/VA
 Sample : N2562-03
 Misc : 9.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW463

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:39:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		279681	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		246004	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152		97712	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		82114	13.281	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	53.120%		
7) Chloroethane-d5	2.886	69		66703m	17.214	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	68.840%		
11) 1,1-Dichloroethene-d2	4.019	63		85281	10.634	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	42.520%#		
21) 2-Butanone-d5	7.080	46		74300	68.831	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	137.660%#		
24) Chloroform-d	7.647	84		181353	20.745	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	83.000%		
26) 1,2-Dichloroethane-d4	8.311	65		113333	22.690	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	90.760%		
32) Benzene-d6	8.275	84		306139	20.369	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	81.480%		
36) 1,2-Dichloropropane-d6	9.275	67		102036	23.459	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	93.840%		
41) Toluene-d8	10.323	98		256417	17.419	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	69.680%		
43) trans-1,3-Dichloroprop...	10.579	79		39513	19.249	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	77.000%		
47) 2-Hexanone-d5	10.927	63		56147	69.383	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	138.760%#		
56) 1,1,2,2-Tetrachloroeth...	12.689	84		109611	29.638	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	118.560%		
66) 1,2-Dichlorobenzene-d4	13.853	152		76225	22.024	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	88.080%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022623.D
Acq On : 26 Apr 2022 14:38
Operator : SY/VA
Sample : N2562-03
Misc : 9.08g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW463

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:39:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

