




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022626.D
Acq On : 26 Apr 2022 15:50
Operator : SY/VA
Sample : N2562-06
Misc : 8.07g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW467

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:40:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

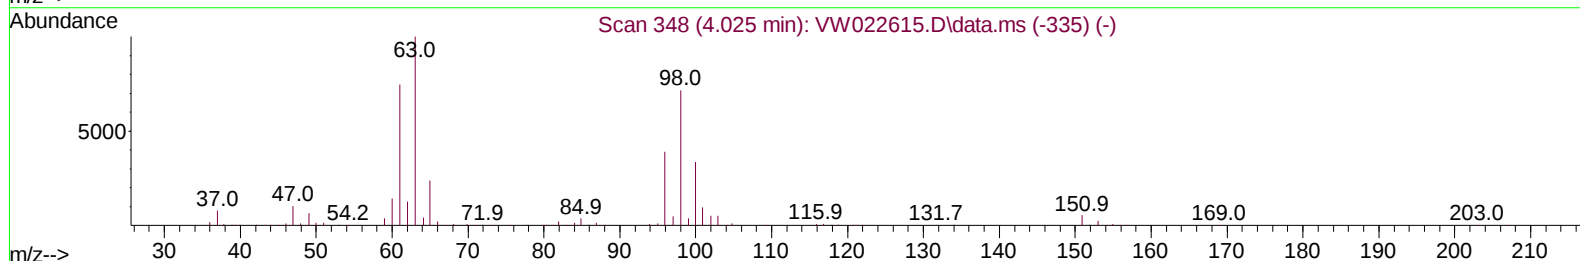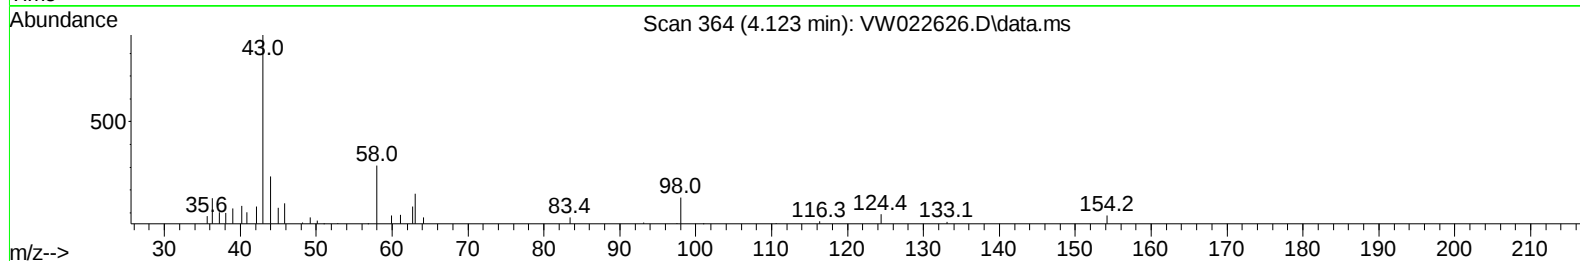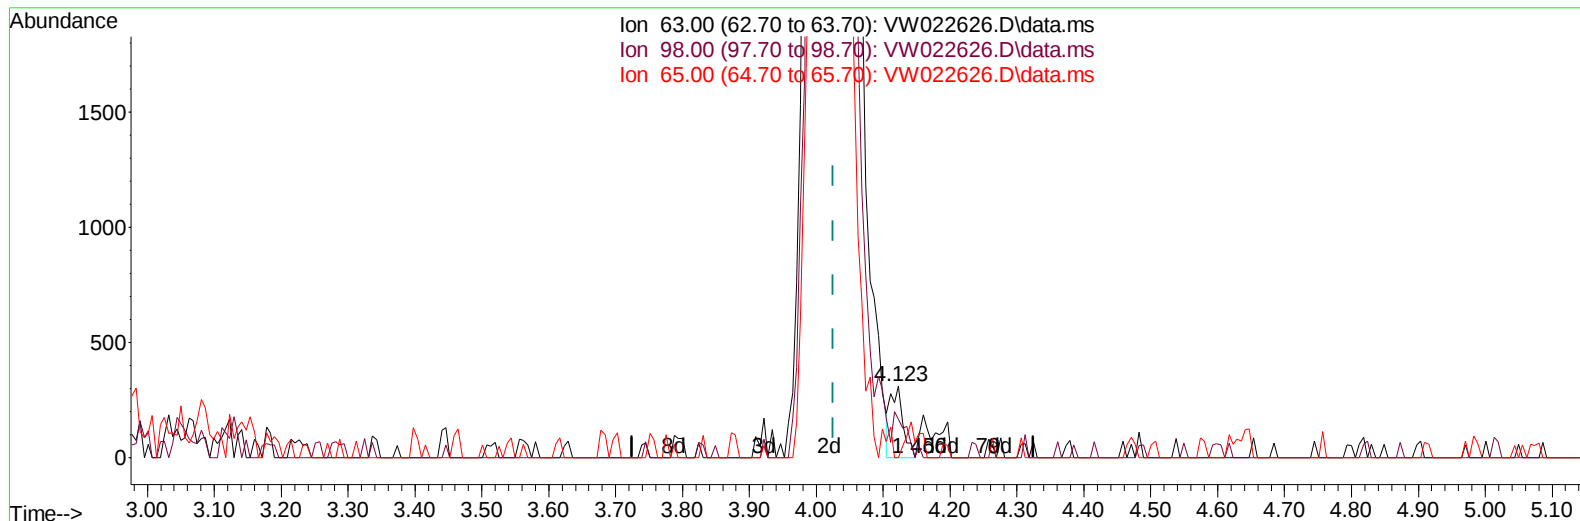

TIC: VW022626.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.123min (+ 0.098) 0.05 ug/L

response 400

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	68.50	62.75
65.00	22.80	29.50
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022626.D
 Acq On : 26 Apr 2022 15:50
 Operator : SY/VA
 Sample : N2562-06
 Misc : 8.07g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW467

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:40:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

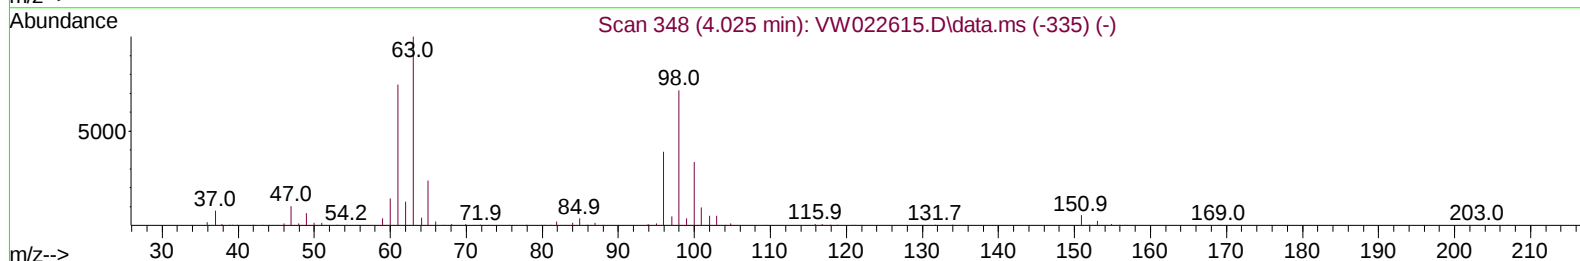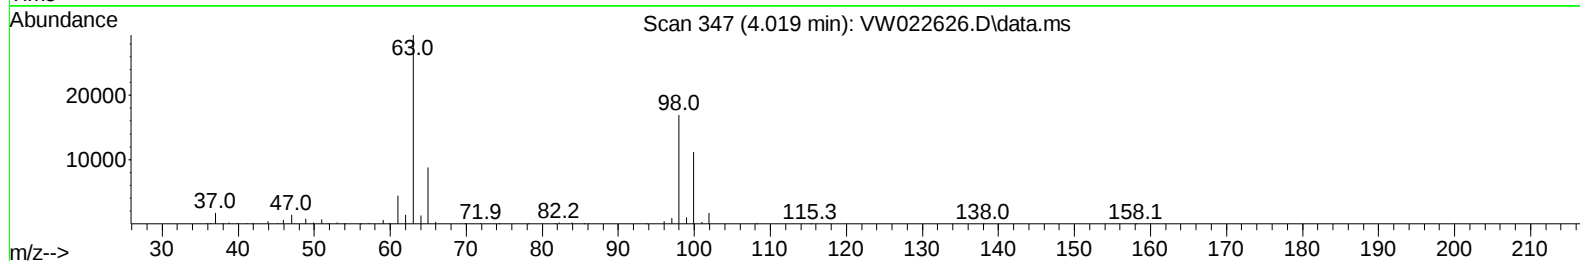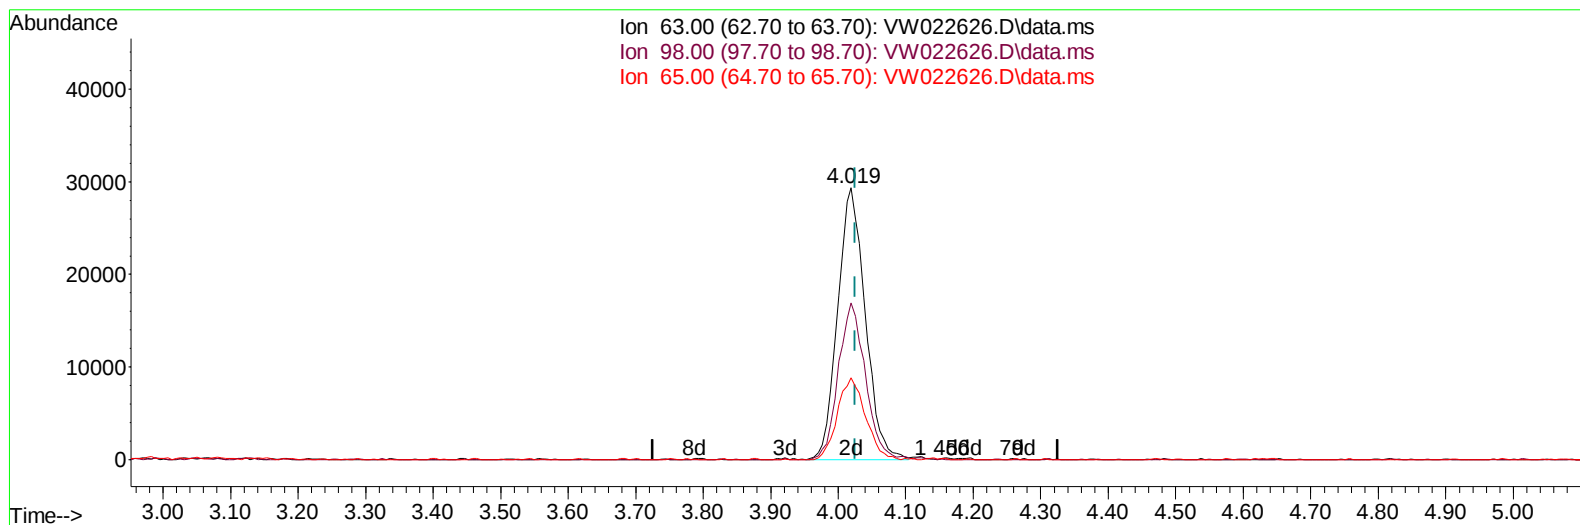

TIC: VW022626.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.019min (-0.006) 10.25 ug/L m

response 82974

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	68.50	0.30#
65.00	22.80	0.14#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022626.D
Acq On : 26 Apr 2022 15:50
Operator : SY/VA
Sample : N2562-06
Misc : 8.07g/10mL/MSVOA_W/soil
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW467

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:40:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

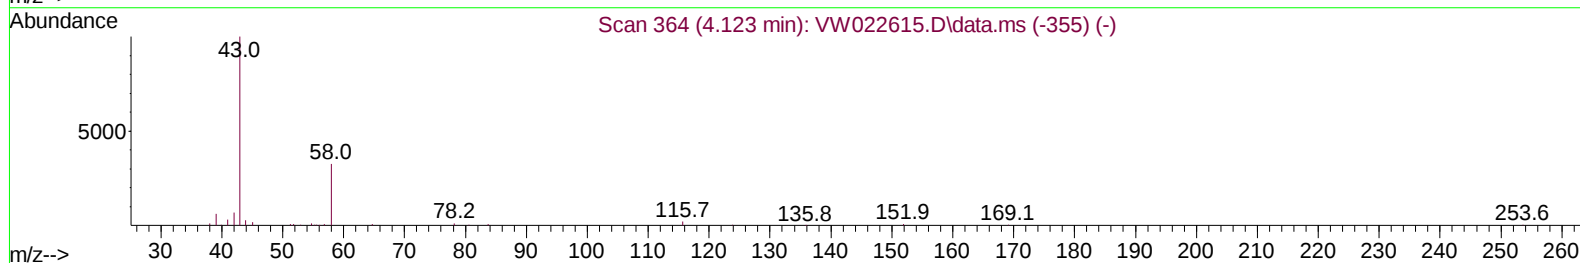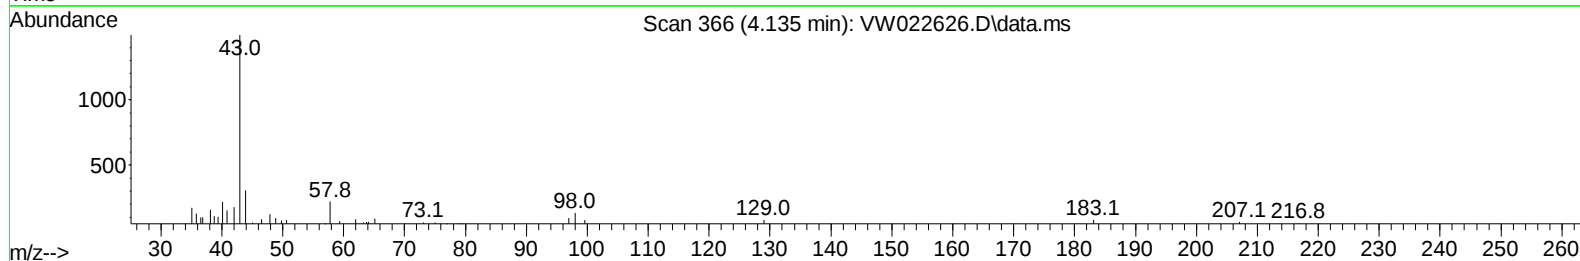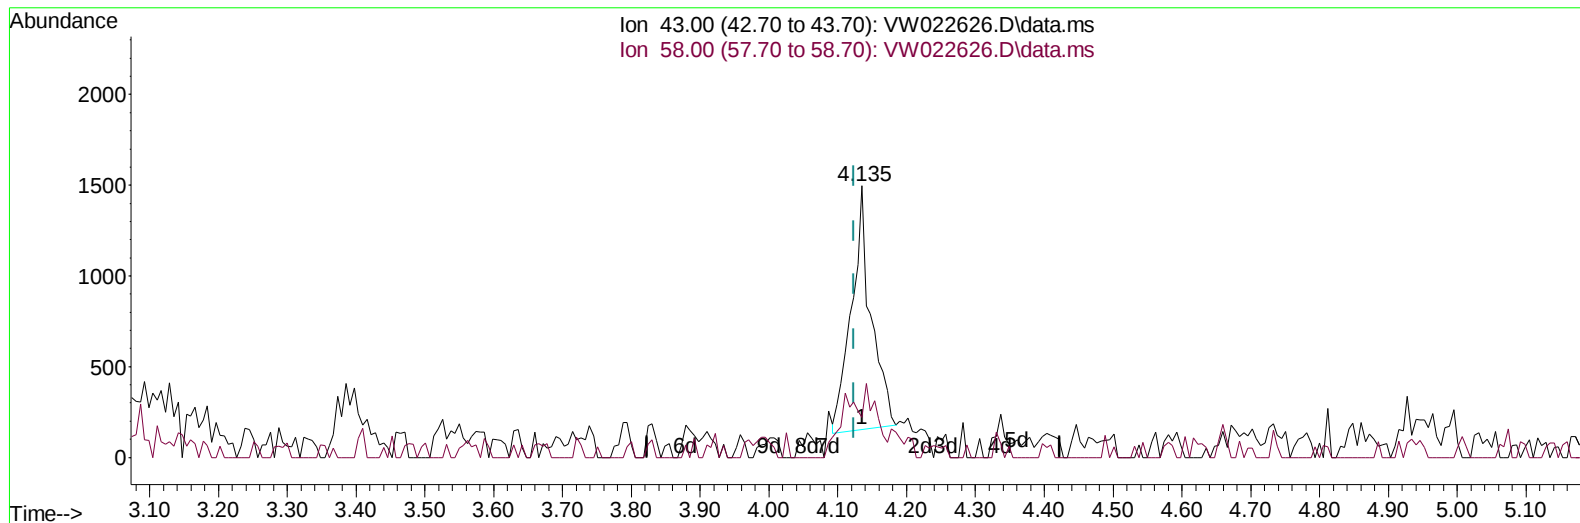

TIC: VW022626.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 3.58 ug/L

response 2658

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	19.11
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022626.D
Acq On : 26 Apr 2022 15:50
Operator : SY/VA
Sample : N2562-06
Misc : 8.07g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW467

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:40:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

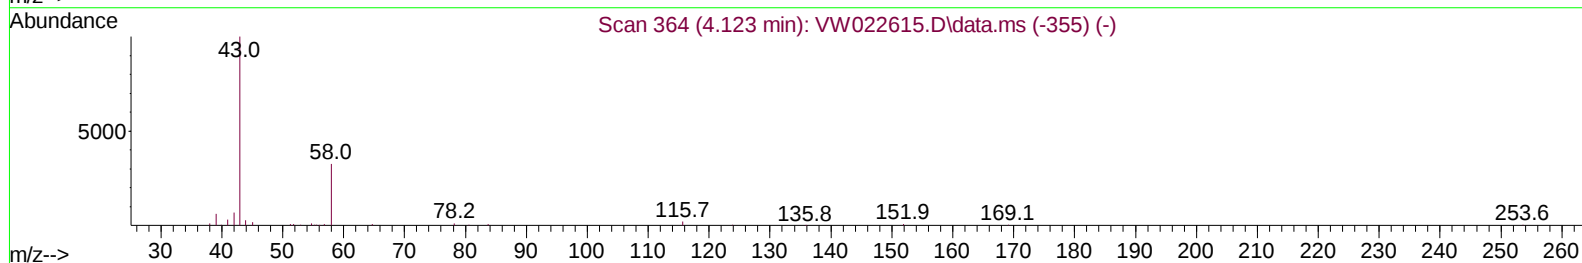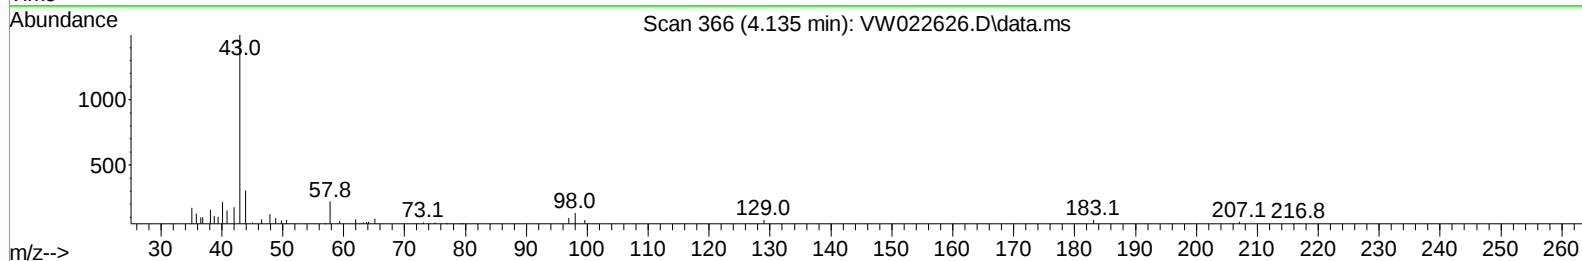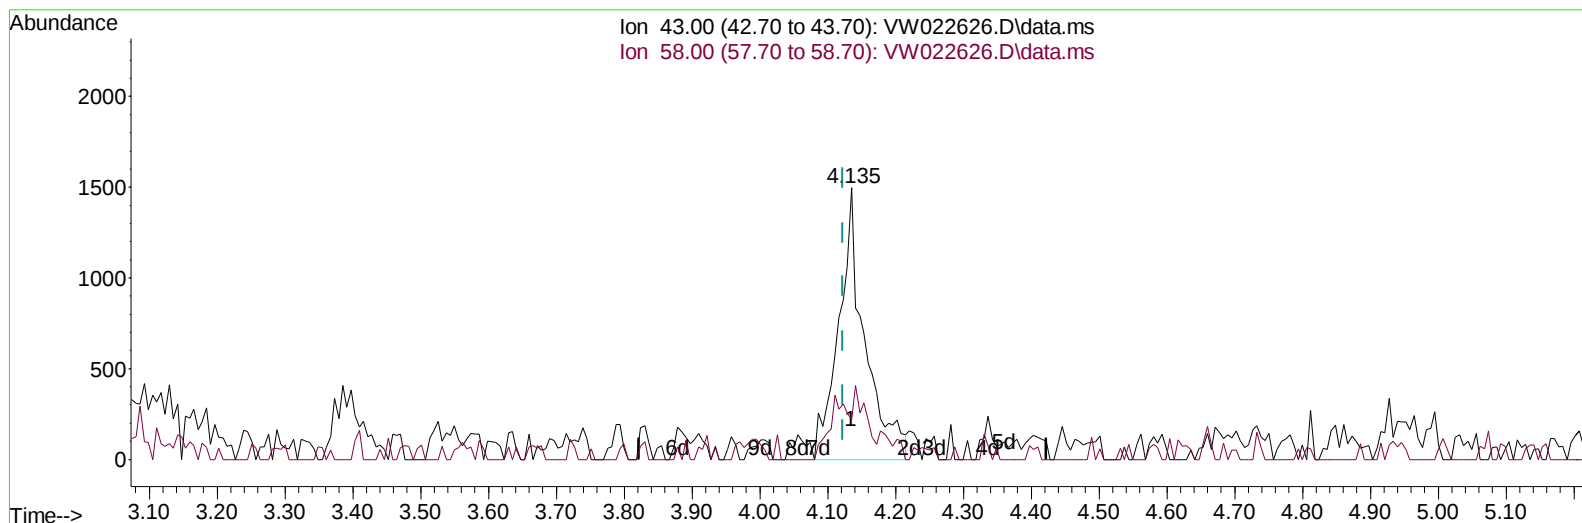

TIC: VW022626.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 5.38 ug/L m

response 3991

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	12.73
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022626.D
 Acq On : 26 Apr 2022 15:50
 Operator : SY/VA
 Sample : N2562-06
 Misc : 8.07g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW467

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:40:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	282225	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	243691	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	94312	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	77038	12.348	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	49.400%	
7) Chloroethane-d5	2.891	69	61467	15.720	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	62.880%	
11) 1,1-Dichloroethene-d2	4.019	63	82974m	10.253	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	41.000%#	
21) 2-Butanone-d5	7.080	46	72368	66.437	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	132.880%	
24) Chloroform-d	7.653	84	176568	20.016	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	80.080%	
26) 1,2-Dichloroethane-d4	8.305	65	110698	21.963	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	87.840%	
32) Benzene-d6	8.275	84	299869	20.141	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	80.560%	
36) 1,2-Dichloropropane-d6	9.274	67	99269	23.040	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	92.160%	
41) Toluene-d8	10.323	98	253321	17.372	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	69.480%	
43) trans-1,3-Dichloroprop...	10.579	79	39295	19.325	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	77.280%	
47) 2-Hexanone-d5	10.927	63	57725	72.010	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	144.020%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	111652	30.477	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	121.920%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	76795	22.989	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	91.960%	
Target Compounds						Qvalue
13) Acetone	4.135	43	3991m	5.381	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022626.D
Acq On : 26 Apr 2022 15:50
Operator : SY/VA
Sample : N2562-06
Misc : 8.07g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW467

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:40:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

