




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022627.D
 Acq On : 26 Apr 2022 16:14
 Operator : SY/VA
 Sample : N2562-07
 Misc : 8.29g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW468

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:40:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

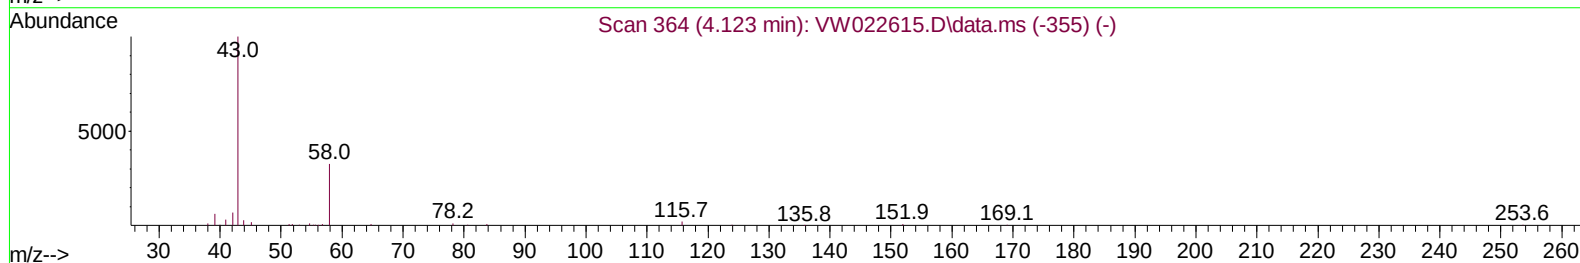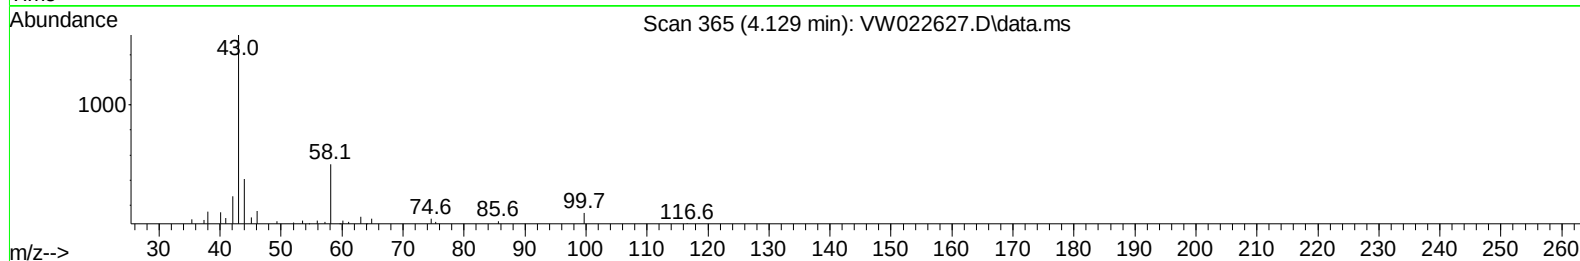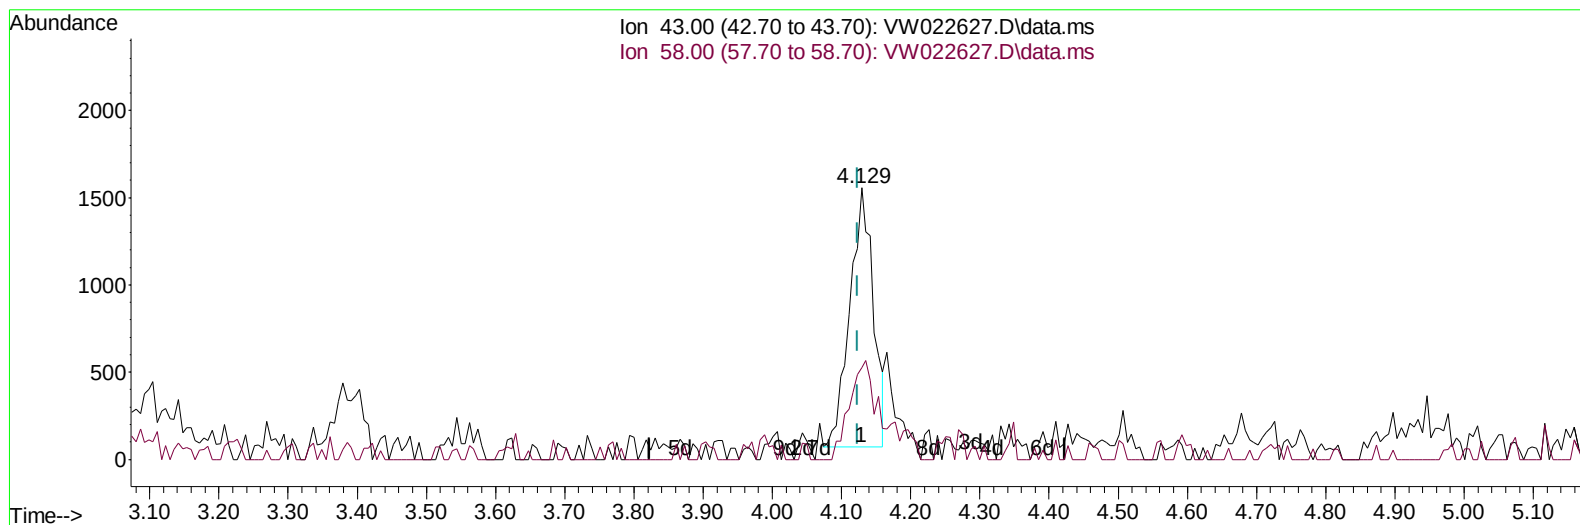

TIC: VW022627.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 5.08 ug/L

response 3519

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	43.08
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022627.D
 Acq On : 26 Apr 2022 16:14
 Operator : SY/VA
 Sample : N2562-07
 Misc : 8.29g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW468

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:40:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

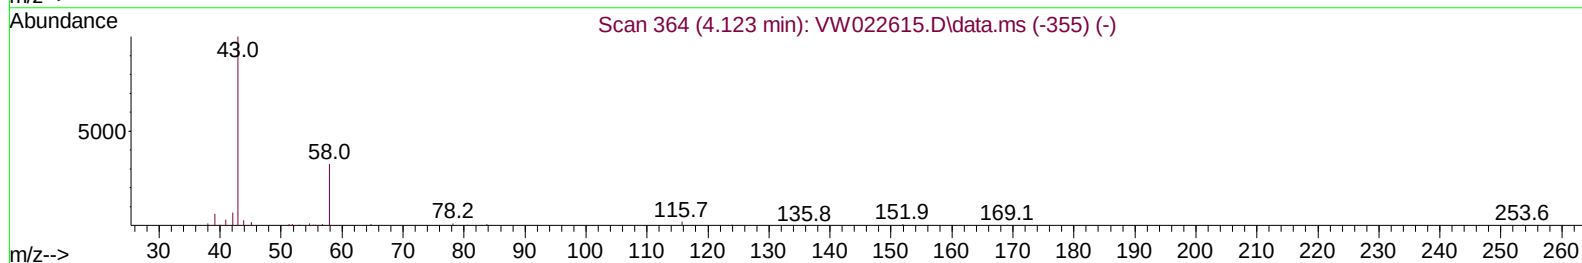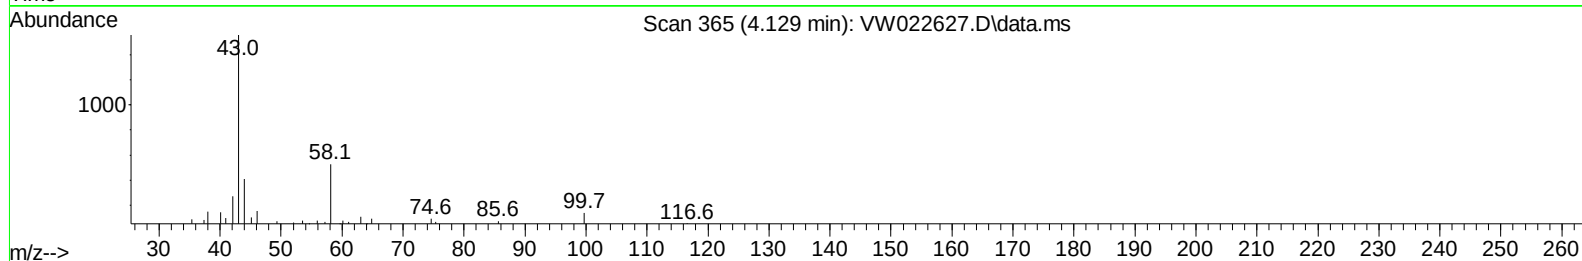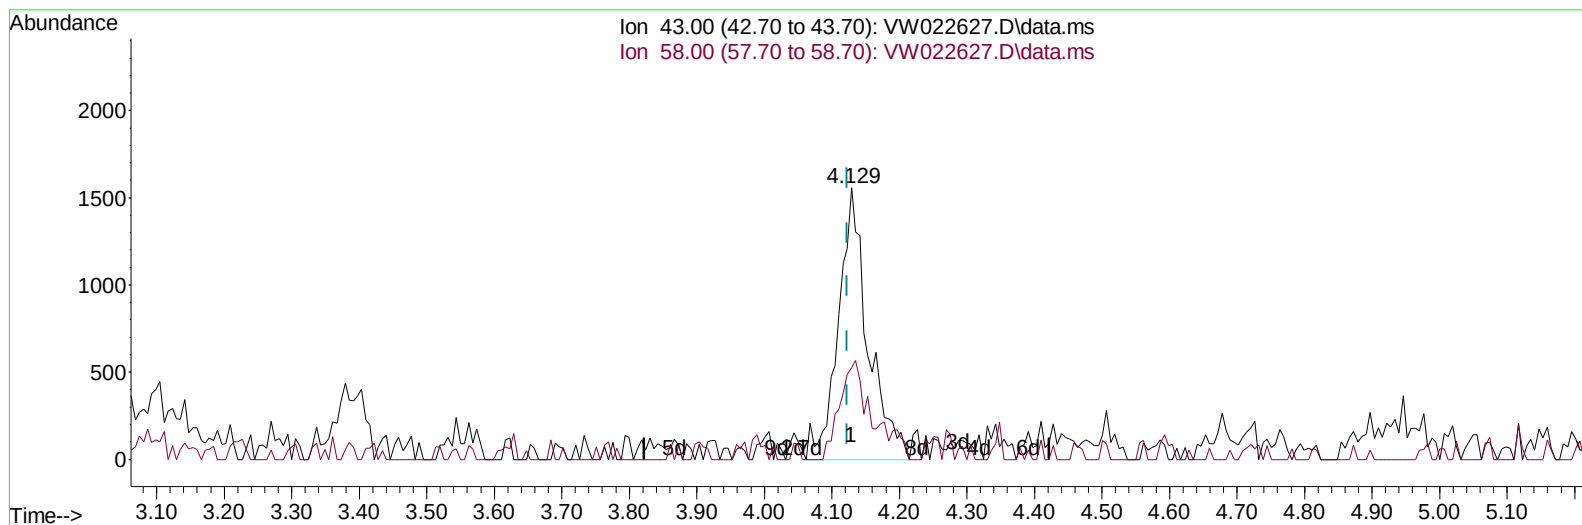

TIC: VW022627.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 6.82 ug/L m

response 4727

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	32.07
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022627.D
 Acq On : 26 Apr 2022 16:14
 Operator : SY/VA
 Sample : N2562-07
 Misc : 8.29g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW468

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:40:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

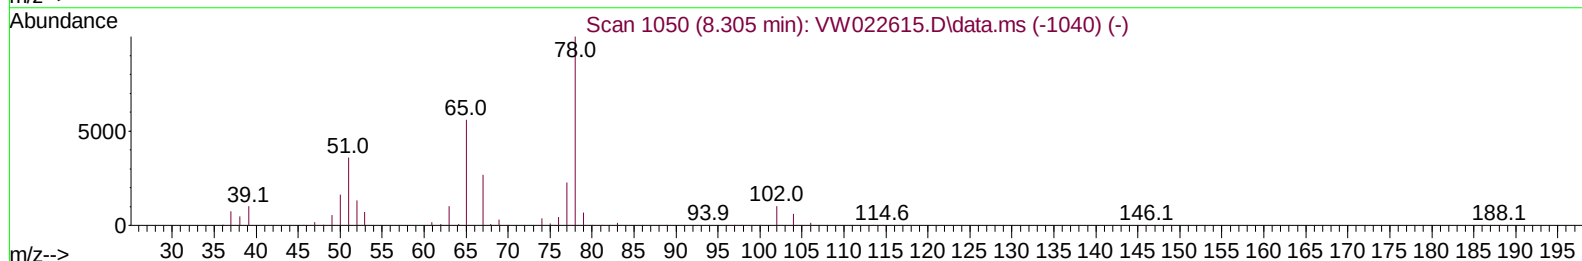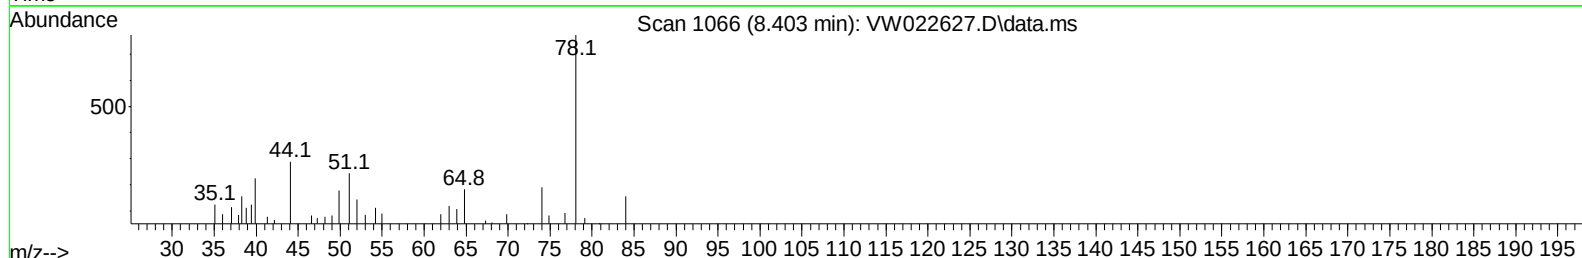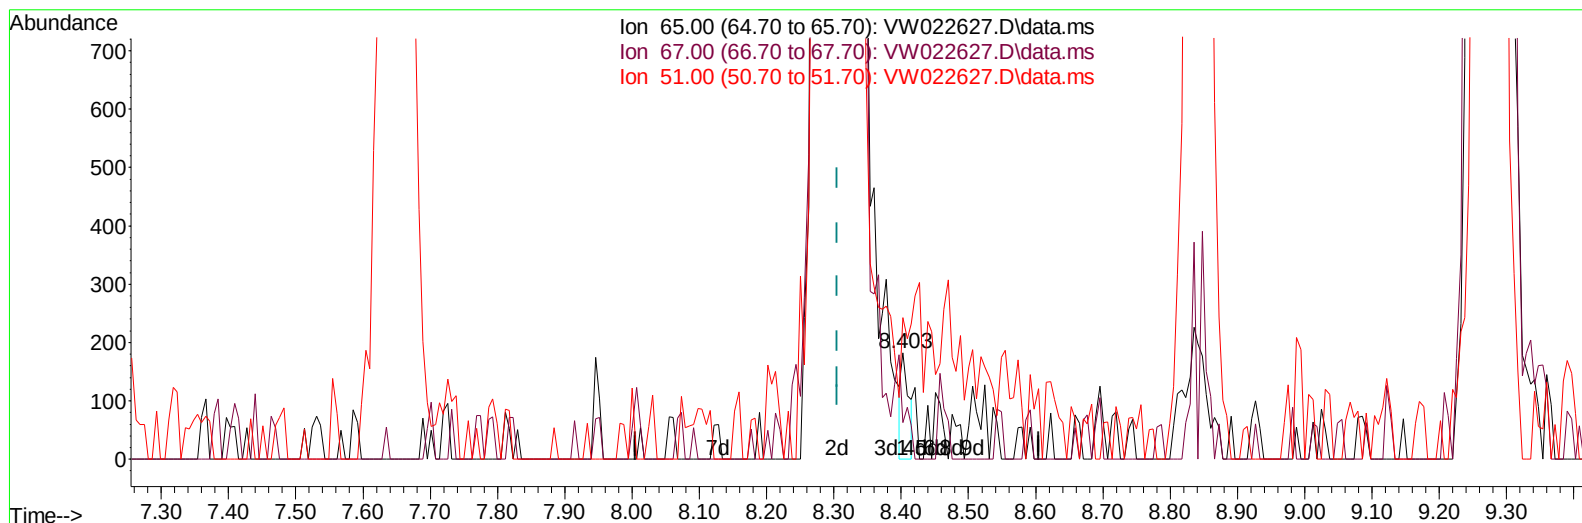

TIC: VW022627.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.403min (+ 0.098) 0.03 ug/L

response 144

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	37.50
51.00	99.30	87.50
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022627.D
 Acq On : 26 Apr 2022 16:14
 Operator : SY/VA
 Sample : N2562-07
 Misc : 8.29g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW468

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:40:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

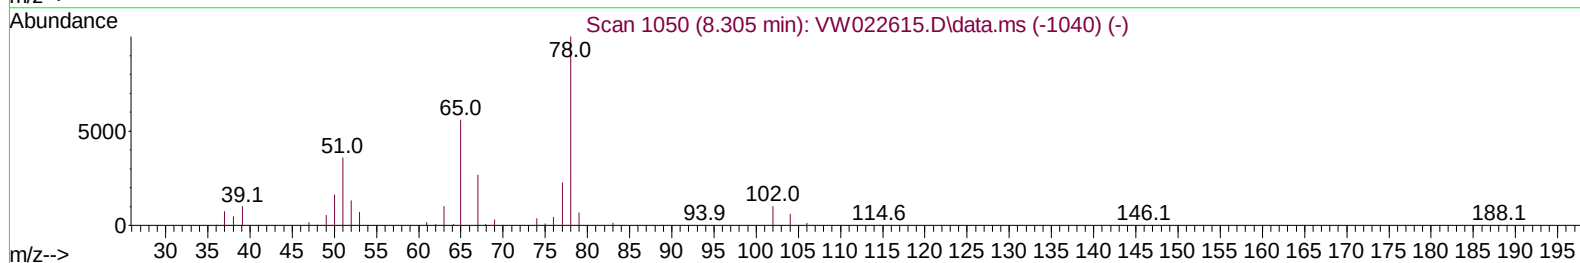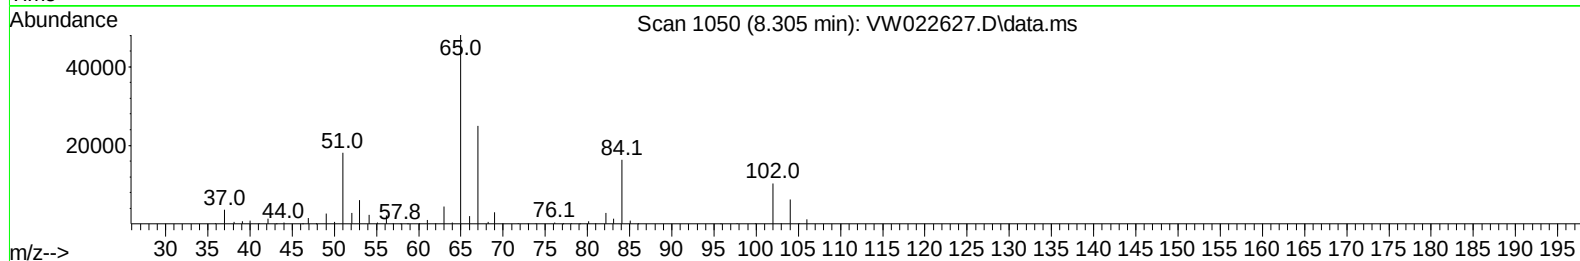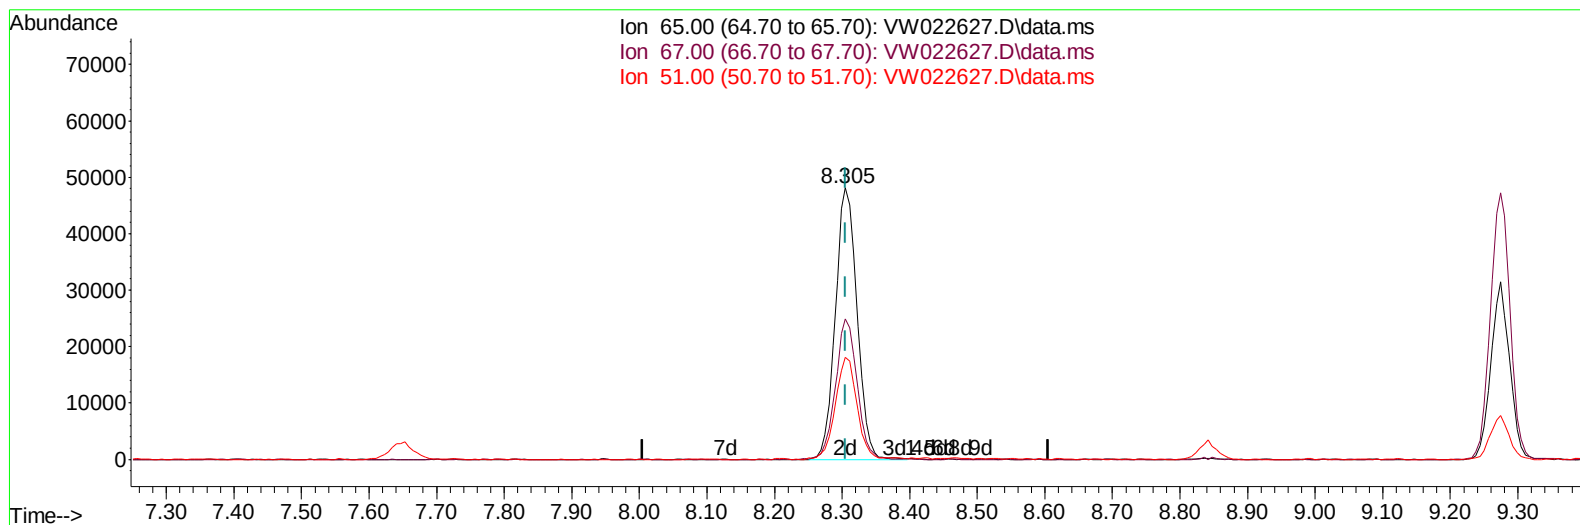

TIC: VW022627.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 22.79 ug/L m

response 107301

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.05#
51.00	99.30	0.12#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022627.D
 Acq On : 26 Apr 2022 16:14
 Operator : SY/VA
 Sample : N2562-07
 Misc : 8.29g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW468

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:40:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		263609	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		216850	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		72114	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		74350	12.758	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	51.040%		
7) Chloroethane-d5	2.885	69		58102	15.908	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	63.640%		
11) 1,1-Dichloroethene-d2	4.019	63		75075	9.932	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	39.720%#		
21) 2-Butanone-d5	7.080	46		76326	75.019	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	150.040%#		
24) Chloroform-d	7.647	84		167339	20.309	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	81.240%		
26) 1,2-Dichloroethane-d4	8.305	65		107301m	22.792	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	91.160%		
32) Benzene-d6	8.275	84		285125	21.521	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	86.080%		
36) 1,2-Dichloropropane-d6	9.274	67		95693	24.959	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	99.840%		
41) Toluene-d8	10.323	98		229111	17.657	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	70.640%		
43) trans-1,3-Dichloroprop...	10.579	79		35244	19.478	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	77.920%		
47) 2-Hexanone-d5	10.920	63		61595	86.349	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	172.700%#		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		106637	32.711	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	130.840%#		
66) 1,2-Dichlorobenzene-d4	13.853	152		57609	22.554	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	90.200%		
Target Compounds							
13) Acetone	4.129	43		4727m	6.824	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022627.D
Acq On : 26 Apr 2022 16:14
Operator : SY/VA
Sample : N2562-07
Misc : 8.29g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW468

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:40:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

