




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022628.D
 Acq On : 26 Apr 2022 16:38
 Operator : SY/VA
 Sample : VIBLK435
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK435

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:40:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

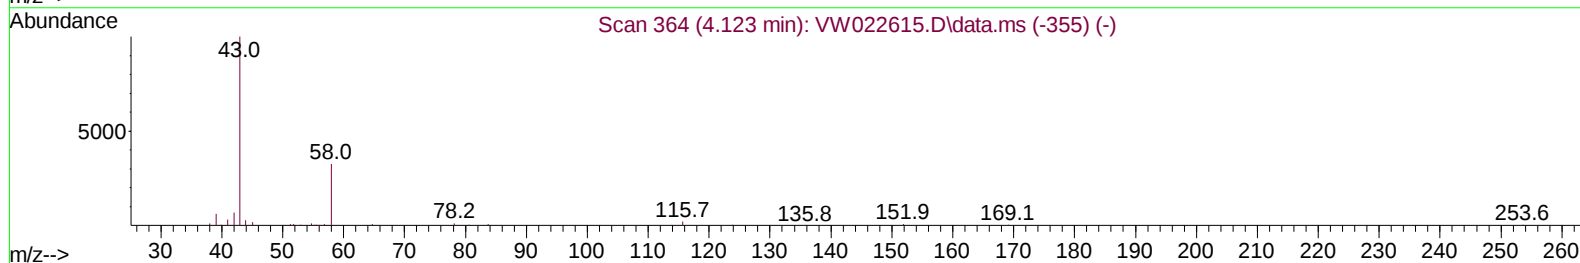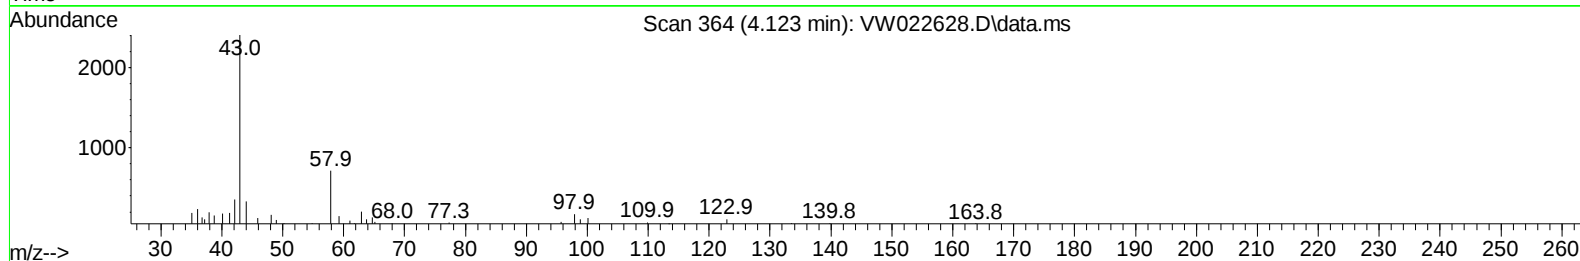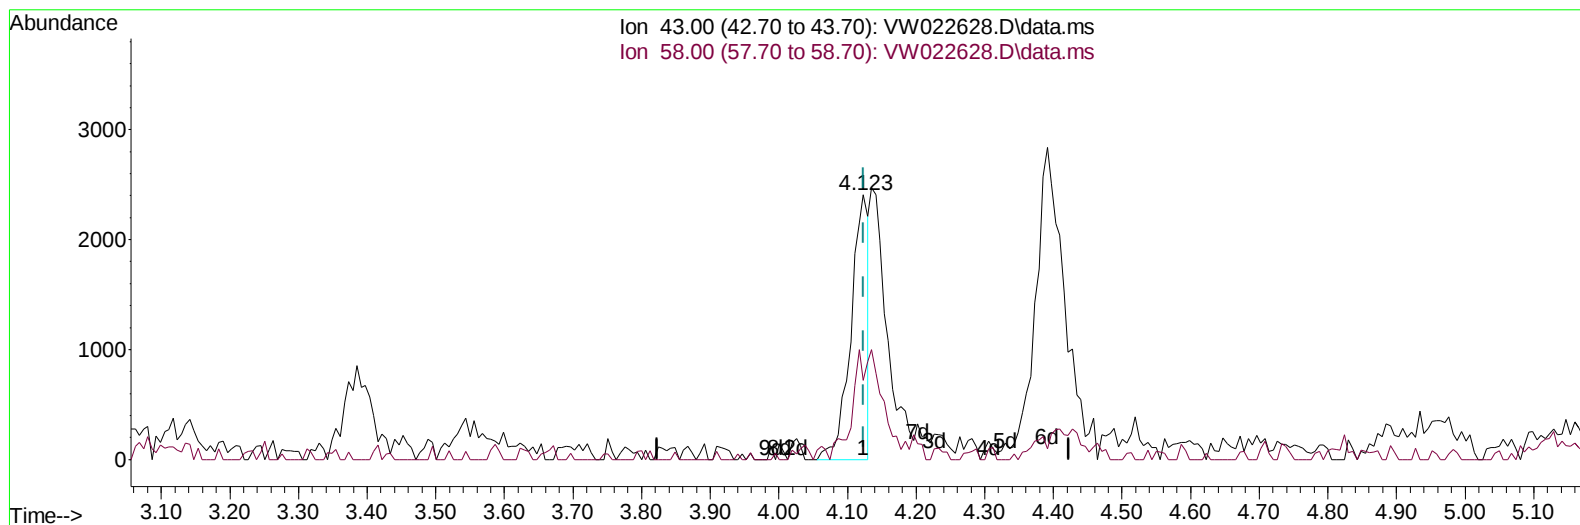

TIC: VW022628.D\data.ms

(13) Acetone (T)

4.123min (+ 0.000) 5.81 ug/L

response 4246

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	23.65
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022628.D
 Acq On : 26 Apr 2022 16:38
 Operator : SY/VA
 Sample : VIBLK435
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK435

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:40:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

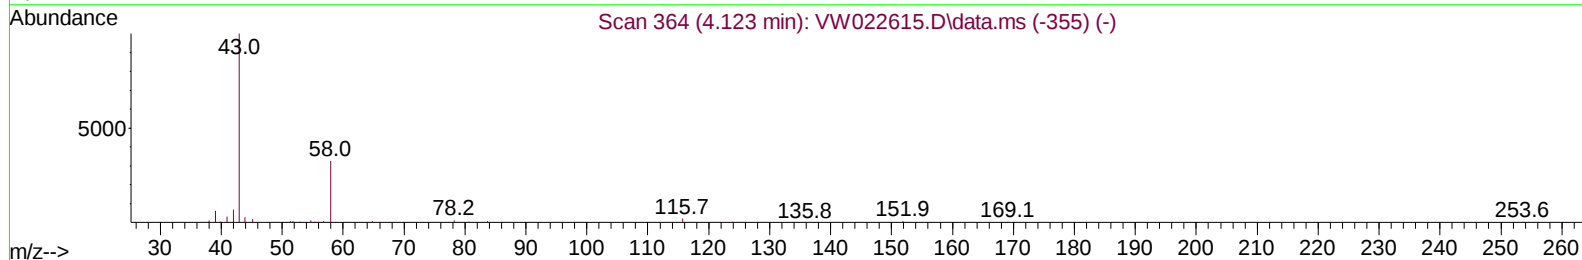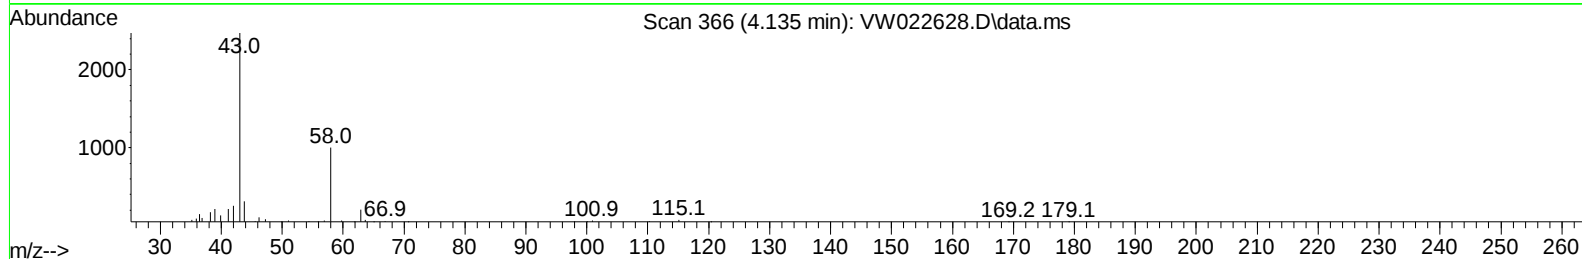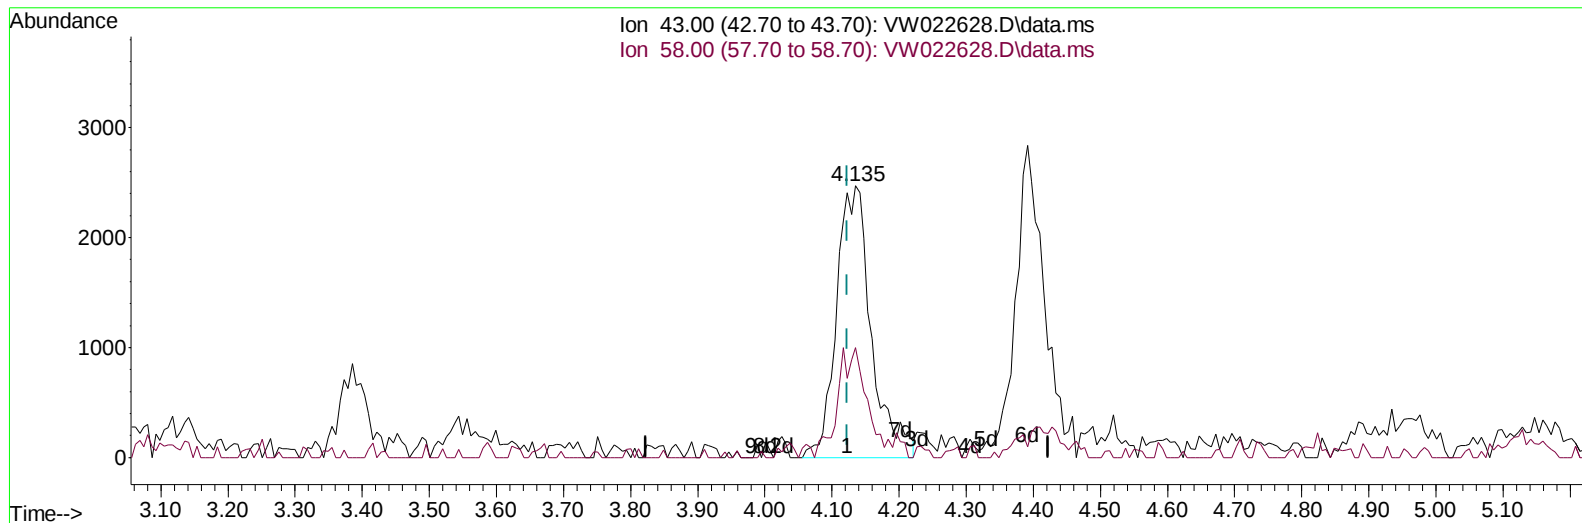

TIC: VW022628.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 12.11 ug/L m

response 8853

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	11.34
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022628.D
 Acq On : 26 Apr 2022 16:38
 Operator : SY/VA
 Sample : VIBLK435
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK435

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:40:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

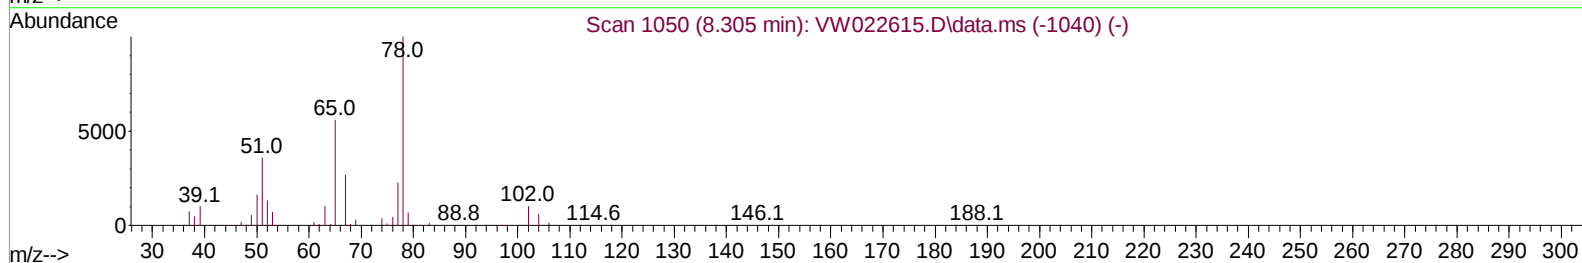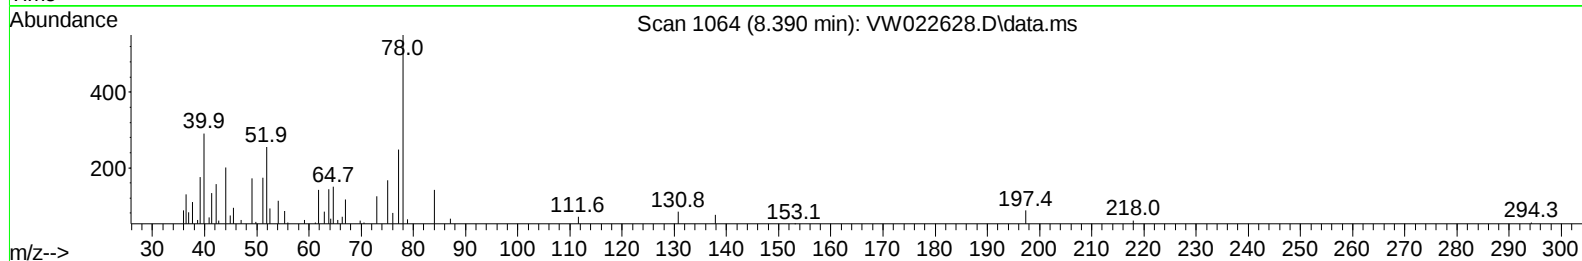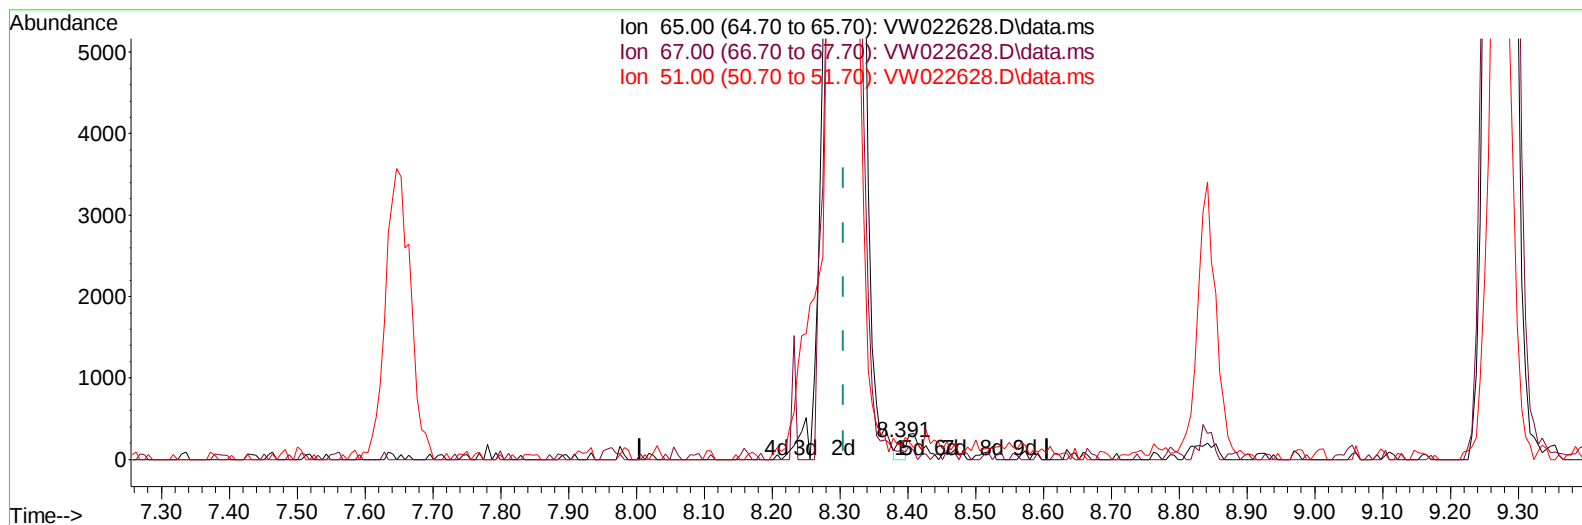

TIC: VW022628.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.390min (+ 0.085) 0.04 ug/L

response 201

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	37.31
51.00	99.30	97.51
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022628.D
Acq On : 26 Apr 2022 16:38
Operator : SY/VA
Sample : VIBLK435
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK435

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:40:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

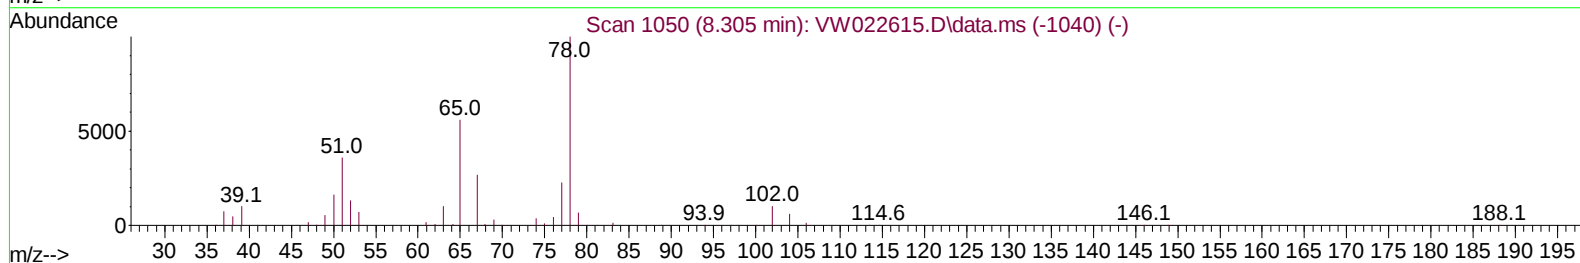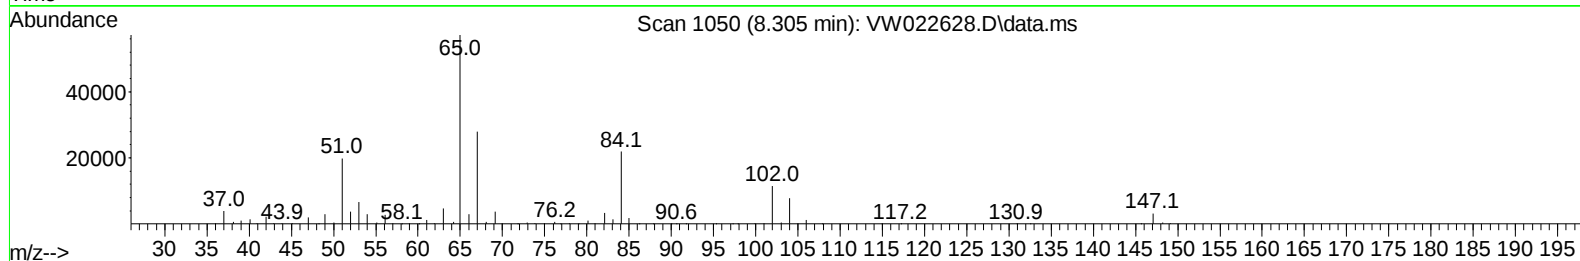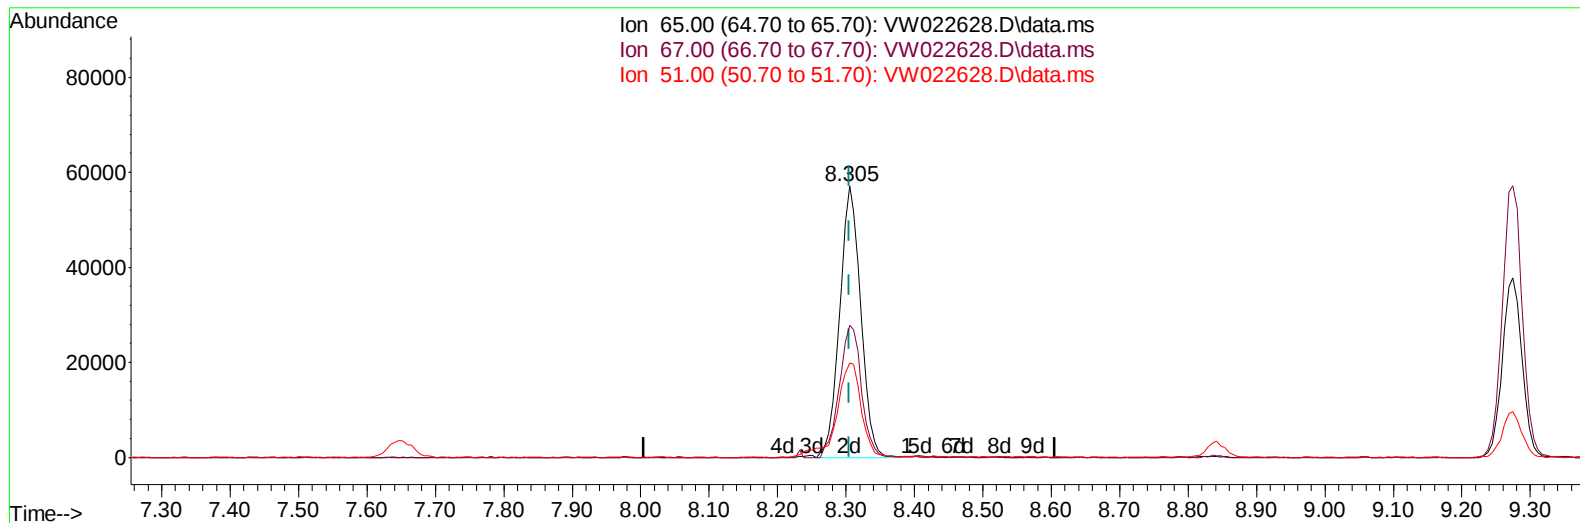

TIC: VW022628.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 24.59 ug/L m

response 122145

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.06#
51.00	99.30	0.16#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022628.D
 Acq On : 26 Apr 2022 16:38
 Operator : SY/VA
 Sample : VIBLK435
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK435

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:40:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	278111	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	274416	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	142388	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	127778	20.783	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	83.120%	
7) Chloroethane-d5	2.885	69	92938	24.120	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	96.480%	
11) 1,1-Dichloroethene-d2	4.019	63	134701	16.892	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	67.560%	
21) 2-Butanone-d5	7.074	46	60162	56.048	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	112.100%	
24) Chloroform-d	7.647	84	210348	24.198	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	96.800%	
26) 1,2-Dichloroethane-d4	8.305	65	122145m	24.593	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	98.360%	
32) Benzene-d6	8.275	84	413438	24.660	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	98.640%	
36) 1,2-Dichloropropane-d6	9.274	67	116426	23.996	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	96.000%	
41) Toluene-d8	10.323	98	388306	23.648	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	94.600%	
43) trans-1,3-Dichloroprop...	10.579	79	48489	21.176	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	84.720%	
47) 2-Hexanone-d5	10.921	63	48346	53.557	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	107.120%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	105415	25.553	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	102.200%	
66) 1,2-Dichlorobenzene-d4	13.853	152	122951	24.379	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	97.520%	
Target Compounds						
13) Acetone	4.135	43	8853m	12.114	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022628.D
Acq On : 26 Apr 2022 16:38
Operator : SY/VA
Sample : VIBLK435
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK435

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:40:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

