




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022629.D
Acq On : 26 Apr 2022 17:02
Operator : SY/VA
Sample : N2562-02RE
Misc : 7.09g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW462RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:40:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

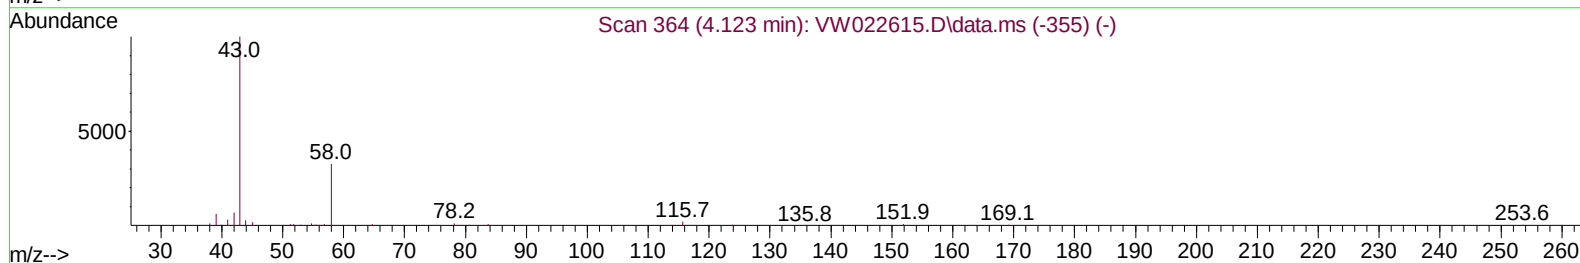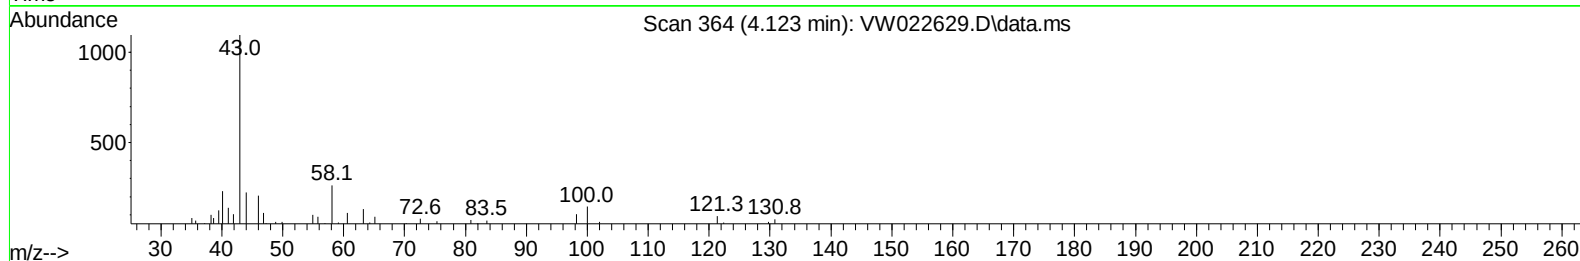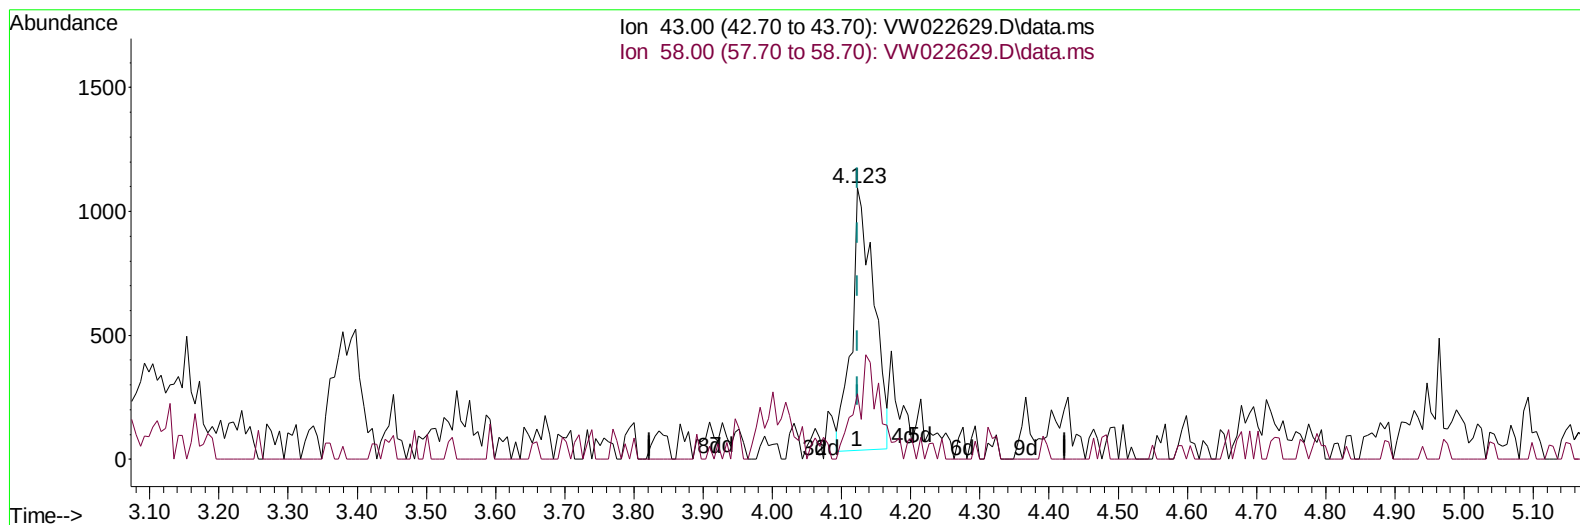

TIC: VW022629.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 3.58 ug/L

response 2348

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	14.57
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022629.D
 Acq On : 26 Apr 2022 17:02
 Operator : SY/VA
 Sample : N2562-02RE
 Misc : 7.09g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW462RE

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:40:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

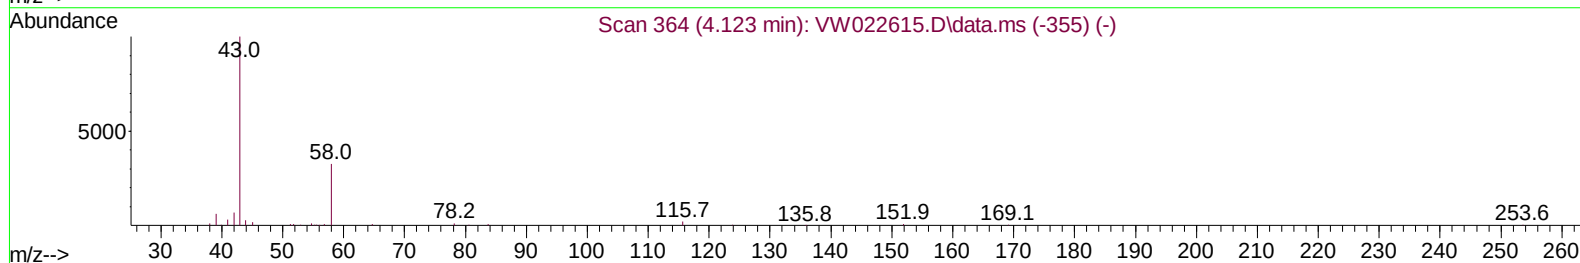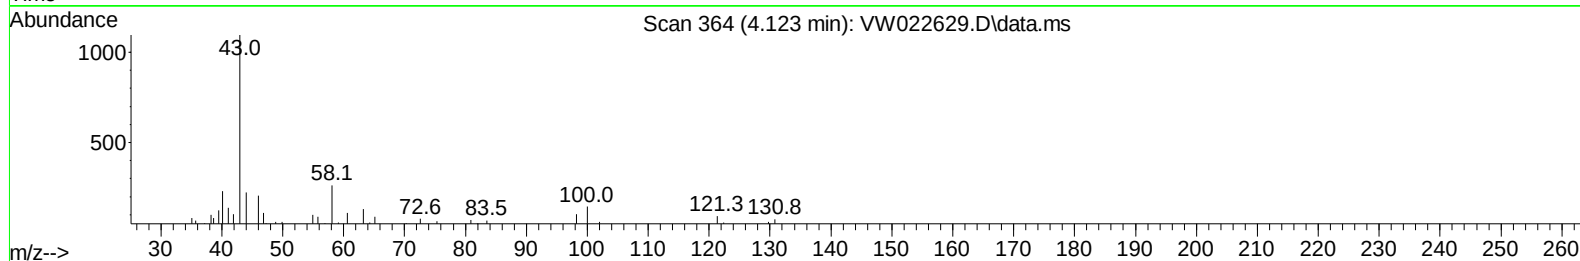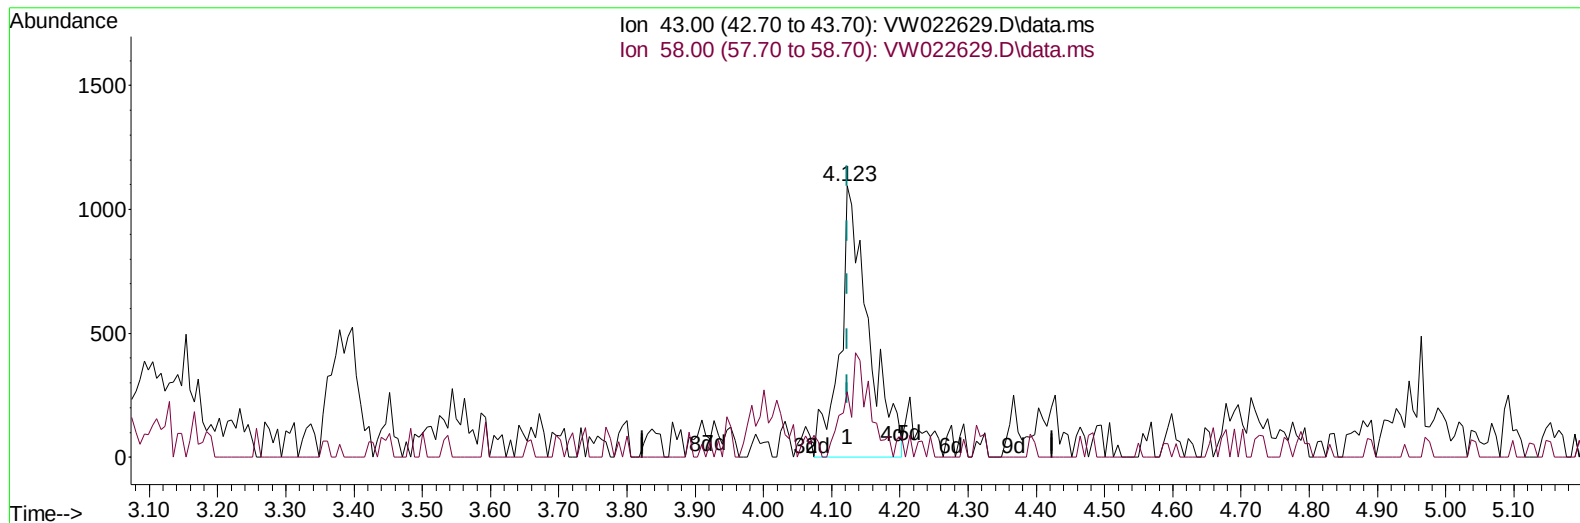

TIC: VW022629.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 4.83 ug/L m

response 3163

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	10.81
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022629.D
 Acq On : 26 Apr 2022 17:02
 Operator : SY/VA
 Sample : N2562-02RE
 Misc : 7.09g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW462RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:40:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	249459	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	152109	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	31598	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	86214	15.633	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	62.520%	
7) Chloroethane-d5	2.885	69	72317	20.924	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	83.680%	
11) 1,1-Dichloroethene-d2	4.019	63	76989	10.763	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	43.040%#	
21) 2-Butanone-d5	7.080	46	93281	96.884	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	193.760%#	
24) Chloroform-d	7.647	84	180549	23.155	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	92.640%	
26) 1,2-Dichloroethane-d4	8.311	65	114774	25.763	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	103.040%	
32) Benzene-d6	8.274	84	291951	31.415	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	125.680%	
36) 1,2-Dichloropropane-d6	9.274	67	102566	38.138	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	152.560%#	
41) Toluene-d8	10.323	98	194464	21.366	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	85.480%	
43) trans-1,3-Dichloroprop...	10.579	79	28596	22.530	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	90.120%	
47) 2-Hexanone-d5	10.920	63	65654	131.212	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	262.420%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	122746	53.678	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	214.720%#	
66) 1,2-Dichlorobenzene-d4	13.847	152	37244	33.277	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	133.120%#	
Target Compounds						
13) Acetone	4.123	43	3163m	4.825	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022629.D
Acq On : 26 Apr 2022 17:02
Operator : SY/VA
Sample : N2562-02RE
Misc : 7.09g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW462RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:40:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

