




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022631.D
 Acq On : 26 Apr 2022 17:50
 Operator : SY/VA
 Sample : VIBLK436
 Misc : 5.00g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK436

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:41:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

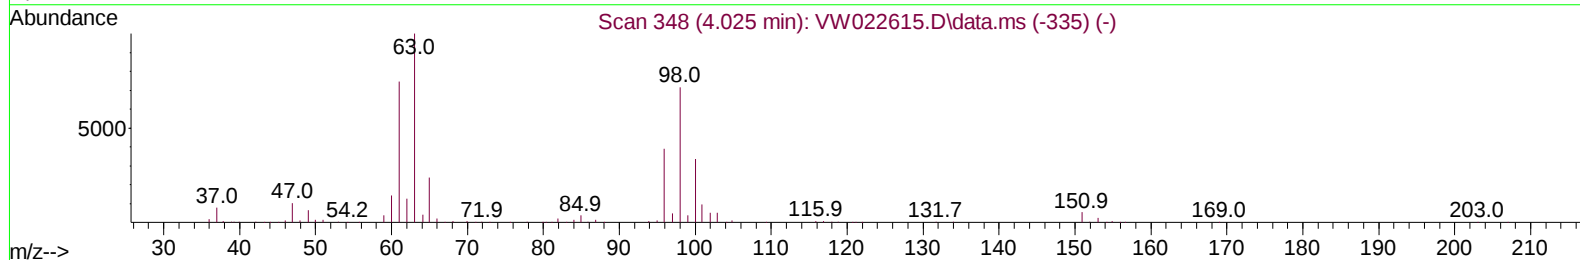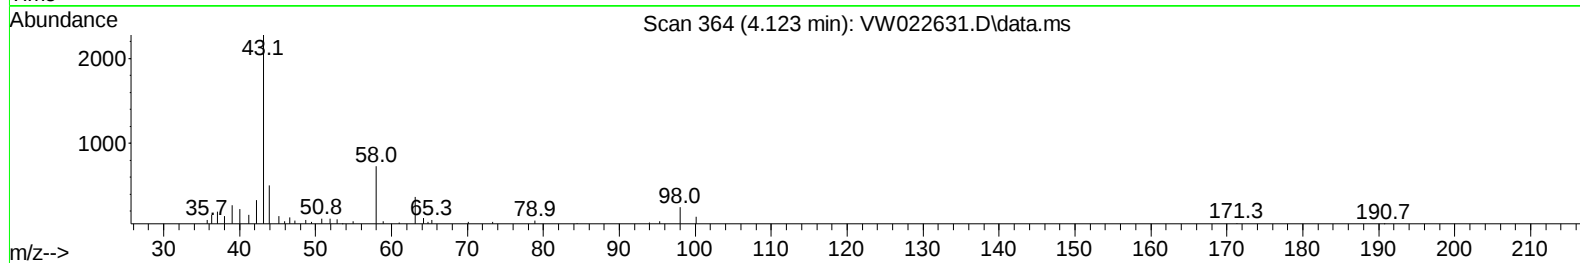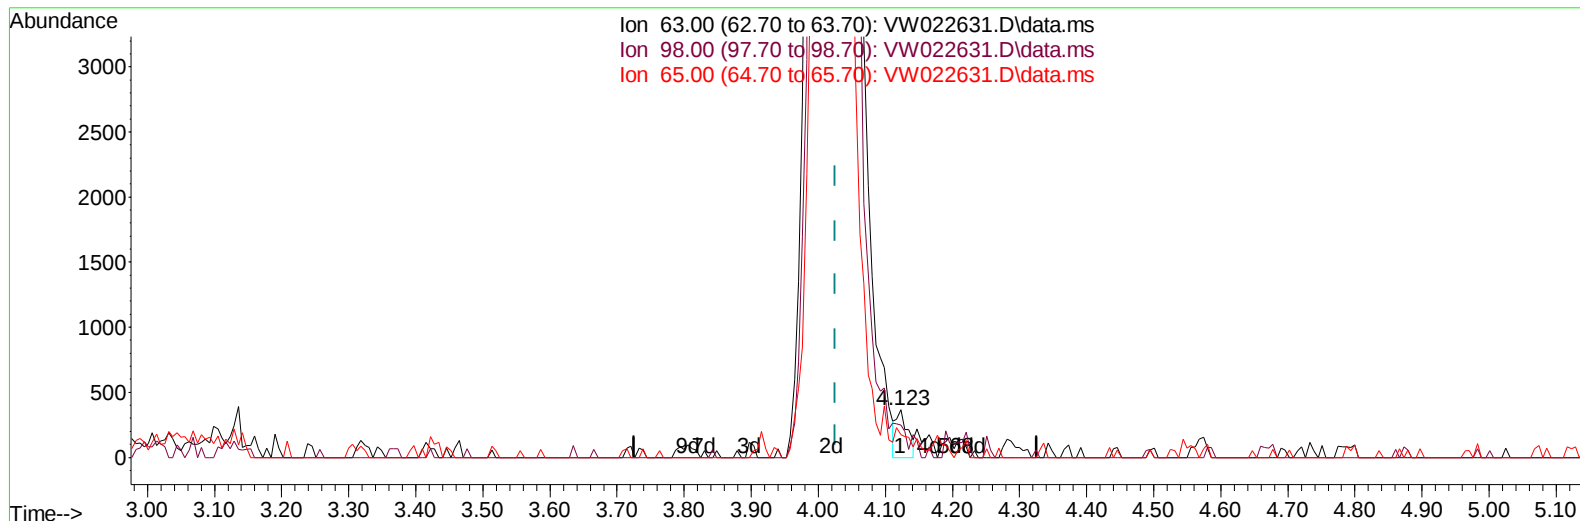

TIC: VW022631.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.123min (+ 0.097) 0.06 ug/L

response 448

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	68.50	83.48
65.00	22.80	17.86
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022631.D
 Acq On : 26 Apr 2022 17:50
 Operator : SY/VA
 Sample : VIBLK436
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK436

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:41:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

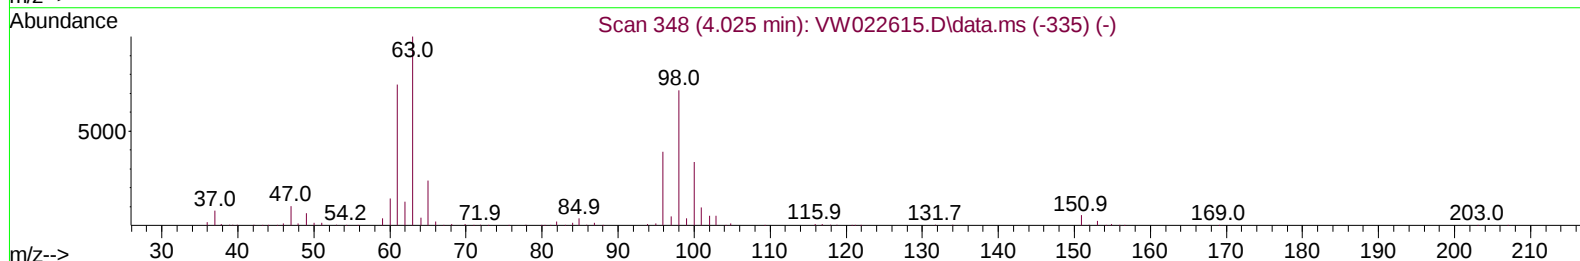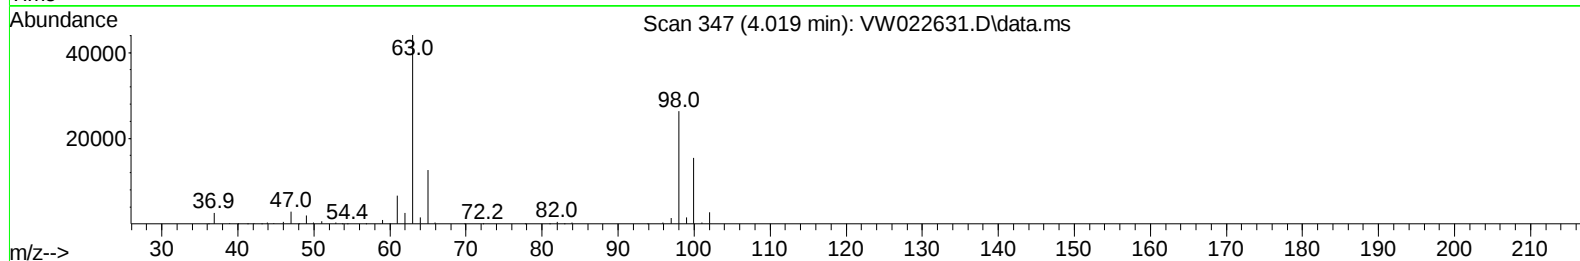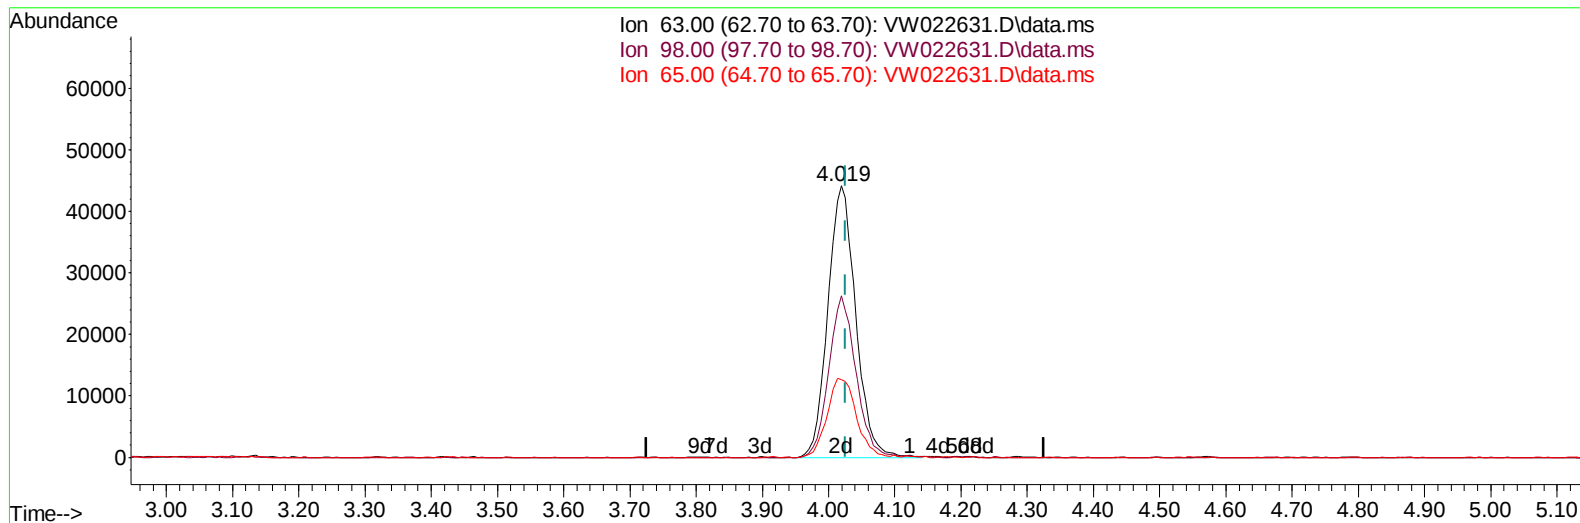

TIC: VW022631.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.019min (-0.006) 16.44 ug/L m

response 129148

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	68.50	0.29#
65.00	22.80	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022631.D
 Acq On : 26 Apr 2022 17:50
 Operator : SY/VA
 Sample : VIBLK436
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK436

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:41:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		273976	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		271362	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		138598	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		125003	20.639	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	82.560%	
7) Chloroethane-d5	2.891	69		92658	24.410	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	97.640%	
11) 1,1-Dichloroethene-d2	4.019	63		129148m	16.440	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	65.760%	
21) 2-Butanone-d5	7.074	46		55830	52.798	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	105.600%	
24) Chloroform-d	7.653	84		203368	23.748	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	95.000%	
26) 1,2-Dichloroethane-d4	8.311	65		114947	23.493	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	93.960%	
32) Benzene-d6	8.275	84		396113	23.892	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	95.560%	
36) 1,2-Dichloropropane-d6	9.274	67		112735	23.497	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	94.000%	
41) Toluene-d8	10.323	98		369199	22.737	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	90.960%	
43) trans-1,3-Dichloroprop...	10.579	79		45203	19.963	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	79.840%	
47) 2-Hexanone-d5	10.927	63		44863	50.258	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	100.520%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		100284	24.582	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	98.320%	
66) 1,2-Dichlorobenzene-d4	13.853	152		119769	24.397	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	97.600%	
Target Compounds							
13) Acetone	4.135	43		6697	9.302	ug/L	Qvalue 88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022631.D
Acq On : 26 Apr 2022 17:50
Operator : SY/VA
Sample : VIBLK436
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK436

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:41:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

