

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022618.D
 Acq On : 26 Apr 2022 11:40
 Operator : SY/VA
 Sample : N2470-04
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:38:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	305670	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	290728	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	149738	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	134754	19.942	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	79.760%		
7) Chloroethane-d5	2.885	69	91018	21.492	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	85.960%		
11) 1,1-Dichloroethene-d2	4.013	63	142058	16.208	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	64.840%		
21) 2-Butanone-d5	7.074	46	52251	44.290	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	88.580%		
24) Chloroform-d	7.647	84	217506	22.765	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	91.080%		
26) 1,2-Dichloroethane-d4	8.305	65	122919	22.517	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	90.080%		
32) Benzene-d6	8.275	84	431480	24.292	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	97.160%		
36) 1,2-Dichloropropane-d6	9.274	67	122462	23.824	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	95.280%		
41) Toluene-d8	10.323	98	405392	23.303	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	93.200%		
43) trans-1,3-Dichloroprop...	10.579	79	48509	19.996	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	80.000%		
47) 2-Hexanone-d5	10.921	63	44767	46.810	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	93.620%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	103071	23.583	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	94.320%		
66) 1,2-Dichlorobenzene-d4	13.853	152	135029	25.459	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	101.840%		
Target Compounds					Qvalue	
13) Acetone	4.123	43	6891m	8.579	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022618.D
Acq On : 26 Apr 2022 11:40
Operator : SY/VA
Sample : N2470-04
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 04/27/2022
Supervised By : Mahesh Dadoda 04/29/2022


Quant Time: Apr 27 01:38:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

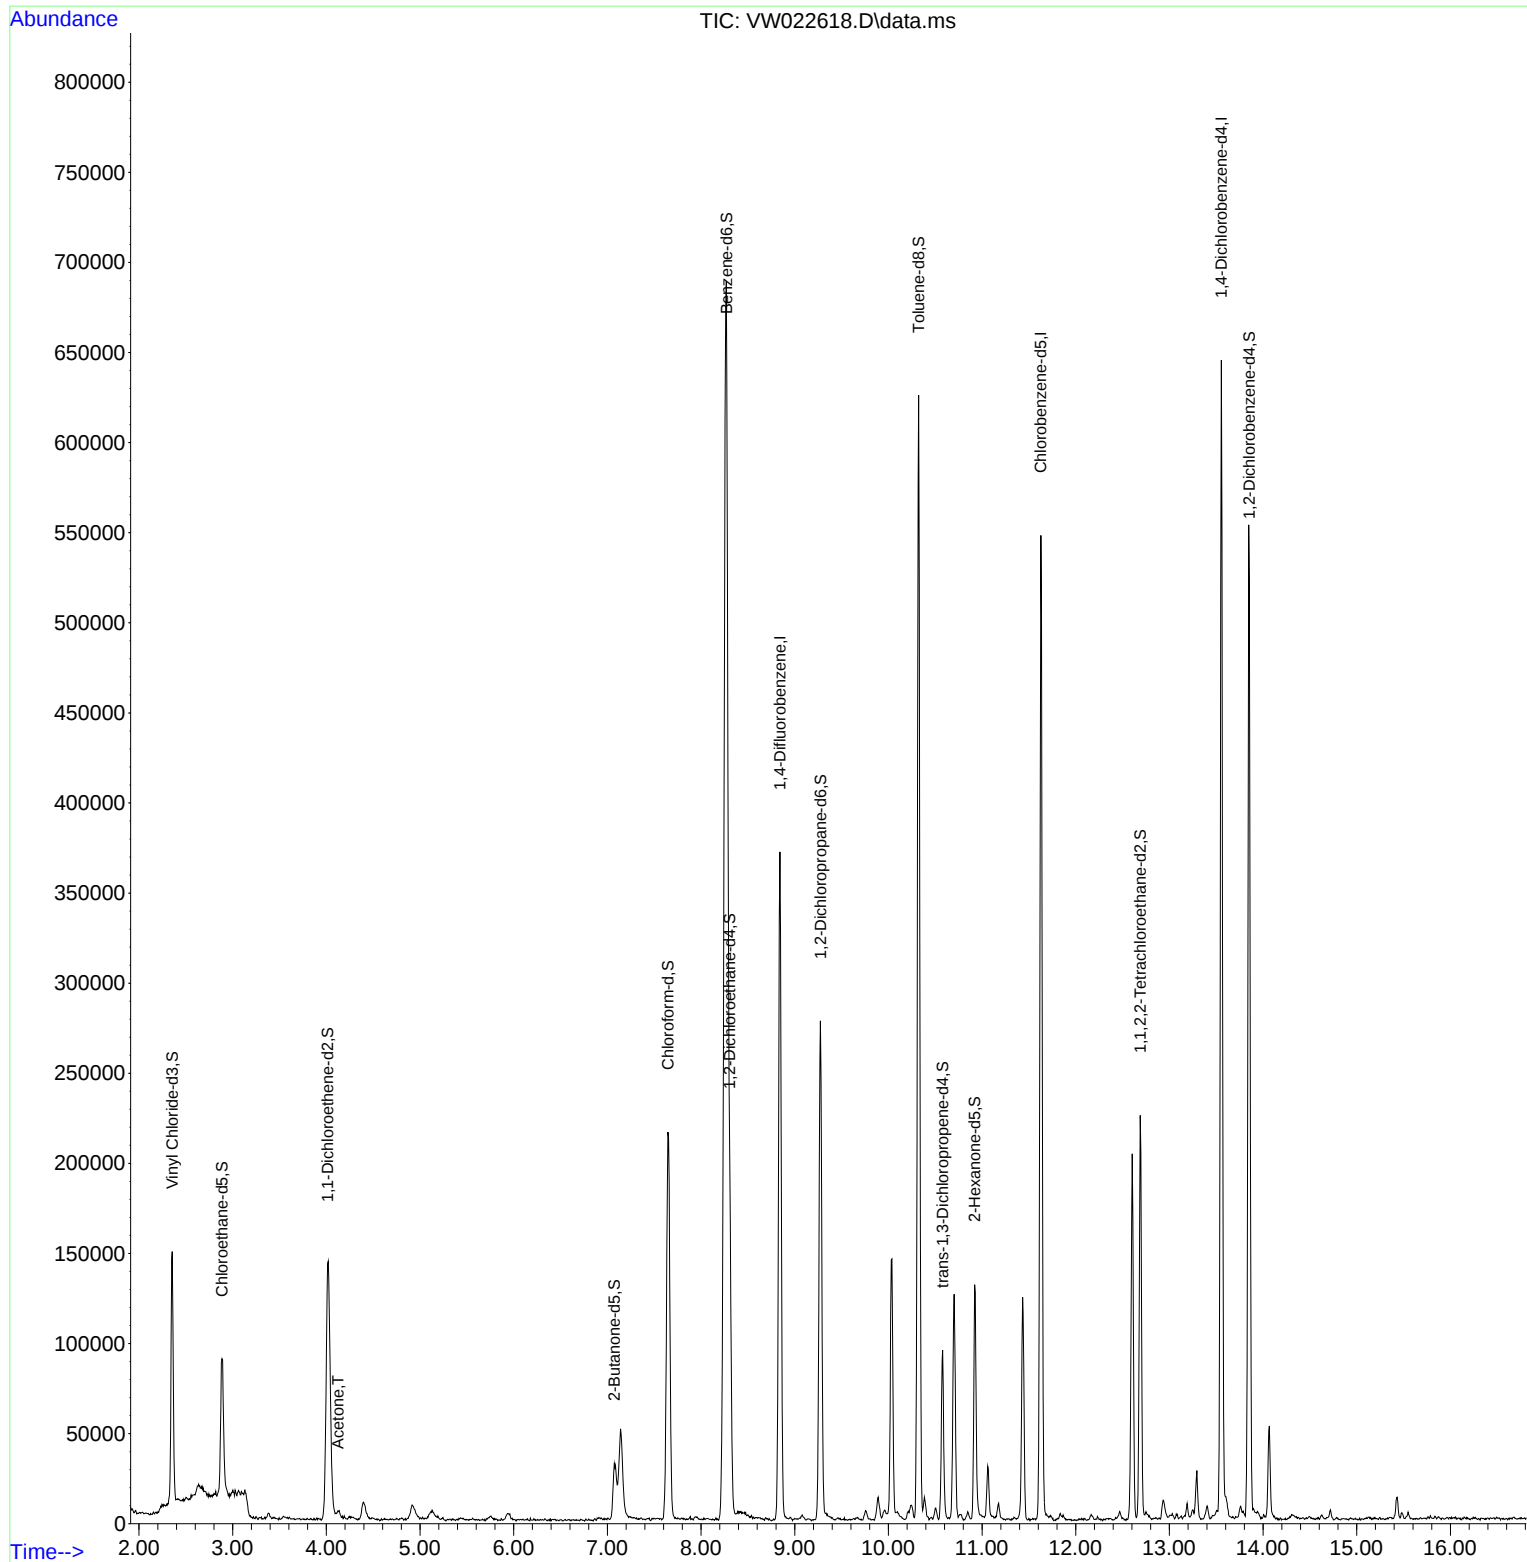

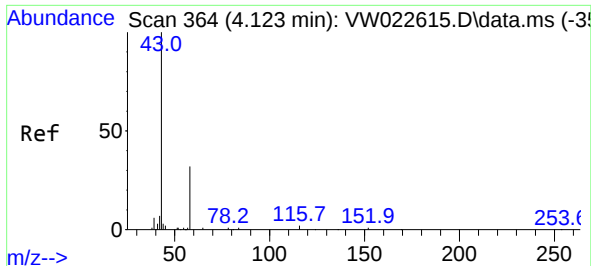

#13
Acetone
Concen: 8.579 ug/L m
RT: 4.123 min Scan# 30
Delta R.T. 0.000 min
Lab File: VW022618.D
Acq: 26 Apr 2022 11:40

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

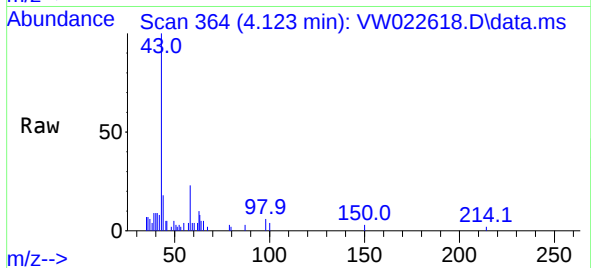

Tgt Ion: 43 Resp: 689
Ion Ratio Lower Upper
43 100
58 0.1 0.0 57.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

