

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022619.D
 Acq On : 26 Apr 2022 12:23
 Operator : SY/VA
 Sample : VIBLK434
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK434

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:38:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	310560	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	303956	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	160081	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	146513	21.340	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	85.360%		
7) Chloroethane-d5	2.885	69	96479	22.423	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	89.680%		
11) 1,1-Dichloroethene-d2	4.019	63	159699	17.934	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	71.720%		
21) 2-Butanone-d5	7.074	46	53712	44.811	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	89.620%		
24) Chloroform-d	7.647	84	232827	23.985	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	95.960%		
26) 1,2-Dichloroethane-d4	8.305	65	129240m	23.302	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	93.200%		
32) Benzene-d6	8.275	84	461388	24.845	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	99.400%		
36) 1,2-Dichloropropane-d6	9.274	67	129163	24.034	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	96.120%		
41) Toluene-d8	10.323	98	438019	24.083	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	96.320%		
43) trans-1,3-Dichloroprop...	10.579	79	51011	20.113	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	80.440%		
47) 2-Hexanone-d5	10.920	63	41826	41.832	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	83.660%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	103345	22.616	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	90.480%		
66) 1,2-Dichlorobenzene-d4	13.847	152	133964	23.626	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	94.520%		
Target Compounds					Qvalue	
13) Acetone	4.129	43	6134	7.516	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022619.D
Acq On : 26 Apr 2022 12:23
Operator : SY/VA
Sample : VIBLK434
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VIBLK434

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:38:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

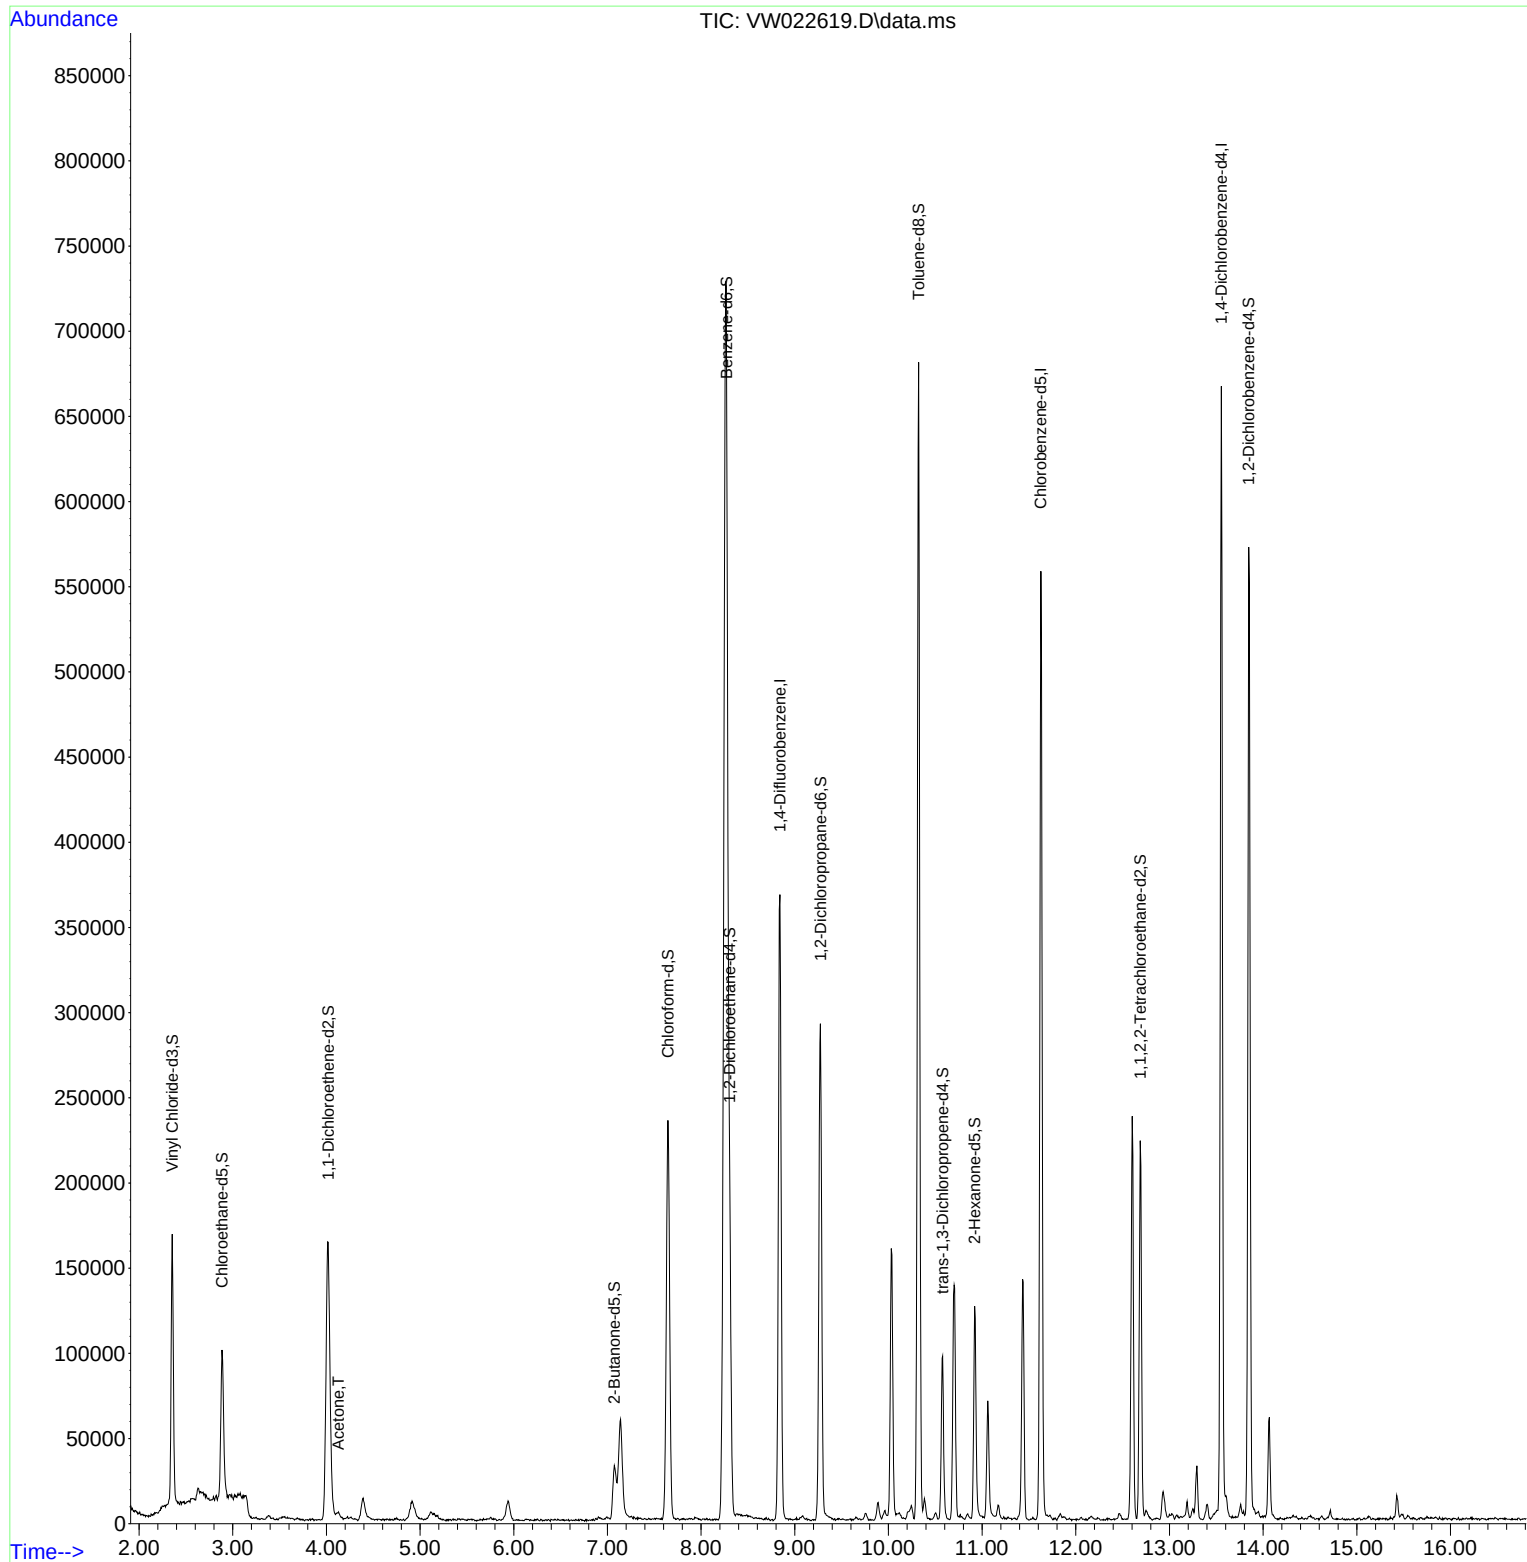

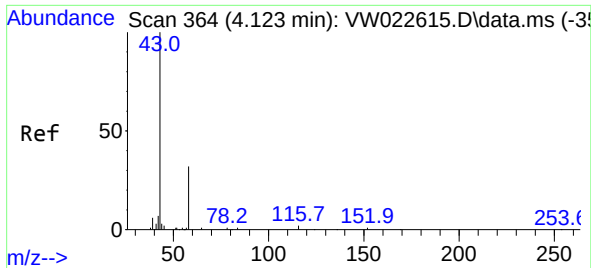

#13
 Acetone
 Concen: 7.516 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW022619.D
 Acq: 26 Apr 2022 12:23

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK434

Tgt Ion: 43 Resp: 6134
 Ion Ratio Lower Upper
 43 100
 58 33.9 0.0 57.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

