

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022626.D
 Acq On : 26 Apr 2022 15:50
 Operator : SY/VA
 Sample : N2562-06
 Misc : 8.07g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW467

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/27/2022
 Supervised By : Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:40:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	282225	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	243691	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	94312	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	77038	12.348	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	49.400%		
7) Chloroethane-d5	2.891	69	61467	15.720	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	62.880%		
11) 1,1-Dichloroethene-d2	4.019	63	82974m	10.253	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	41.000%#		
21) 2-Butanone-d5	7.080	46	72368	66.437	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	132.880%		
24) Chloroform-d	7.653	84	176568	20.016	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	80.080%		
26) 1,2-Dichloroethane-d4	8.305	65	110698	21.963	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	87.840%		
32) Benzene-d6	8.275	84	299869	20.141	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	80.560%		
36) 1,2-Dichloropropane-d6	9.274	67	99269	23.040	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	92.160%		
41) Toluene-d8	10.323	98	253321	17.372	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	69.480%		
43) trans-1,3-Dichloroprop...	10.579	79	39295	19.325	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	77.280%		
47) 2-Hexanone-d5	10.927	63	57725	72.010	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	144.020%#		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	111652	30.477	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	121.920%#		
66) 1,2-Dichlorobenzene-d4	13.853	152	76795	22.989	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	91.960%		
Target Compounds					Qvalue	
13) Acetone	4.135	43	3991m	5.381	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022626.D
Acq On : 26 Apr 2022 15:50
Operator : SY/VA
Sample : N2562-06
Misc : 8.07g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW467

Quant Time: Apr 27 01:40:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

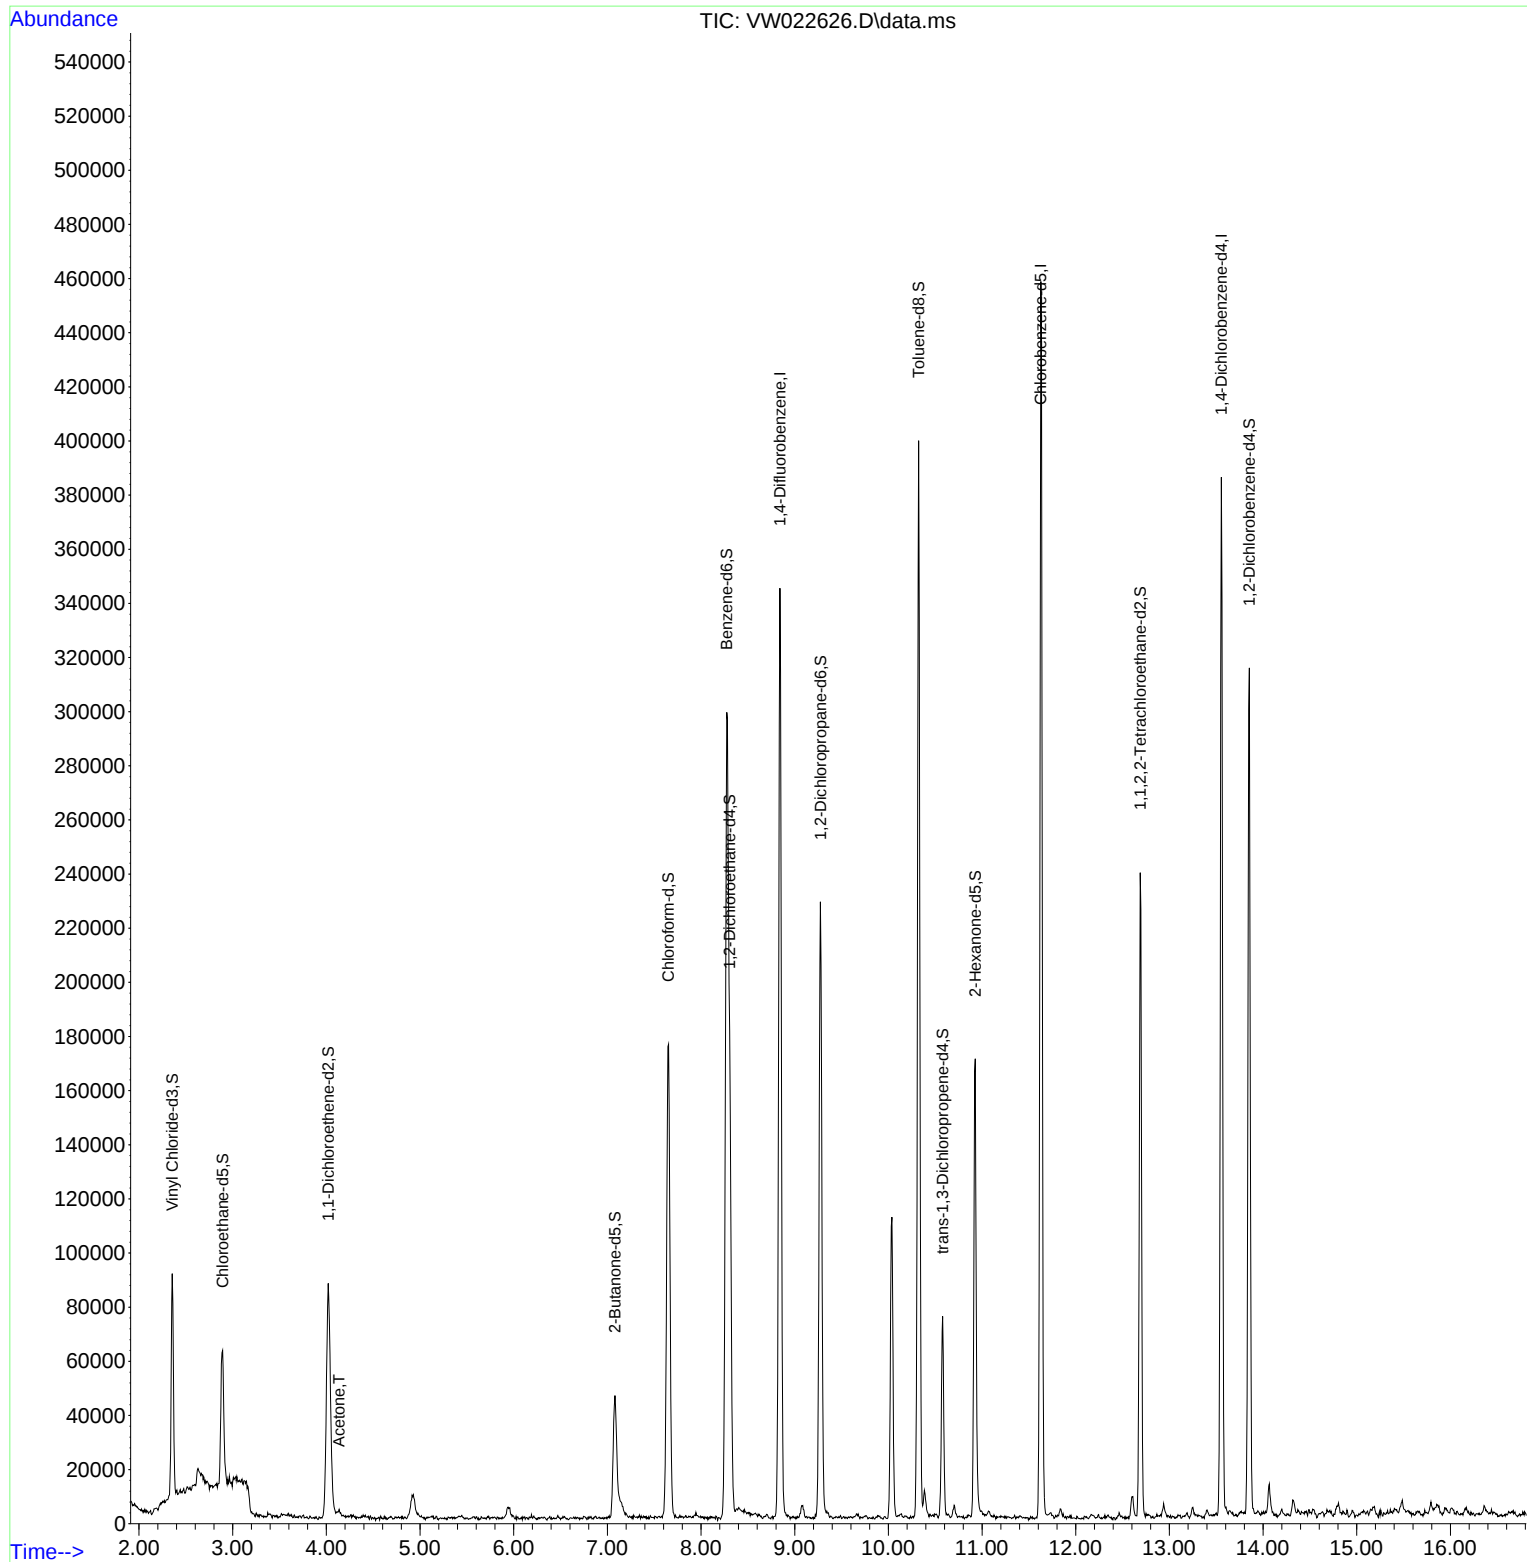

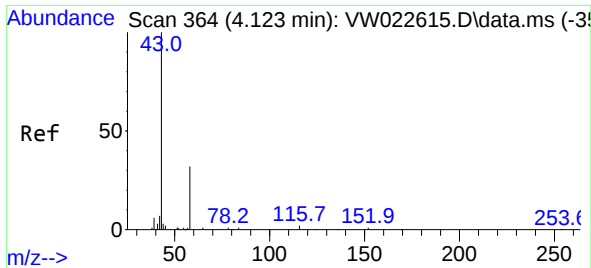

#13
 Acetone
 Concen: 5.381 ug/L m
 RT: 4.135 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW022626.D
 Acq: 26 Apr 2022 15:50

Instrument :
 MSVOA_W
 ClientSampleId :
 EW467

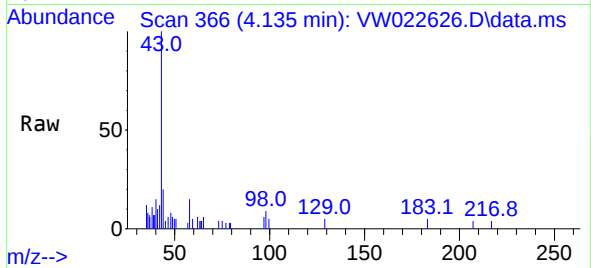

Tgt Ion: 43 Resp: 399
 Ion Ratio Lower Upper
 43 100
 58 12.7 0.0 57.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

