

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022629.D
 Acq On : 26 Apr 2022 17:02
 Operator : SY/VA
 Sample : N2562-02RE
 Misc : 7.09g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW462RE

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/27/2022
 Supervised By : Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:40:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	249459	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	152109	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	31598	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	86214	15.633	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.520%
7) Chloroethane-d5	2.885	69	72317	20.924	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.680%
11) 1,1-Dichloroethene-d2	4.019	63	76989	10.763	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	43.040%#
21) 2-Butanone-d5	7.080	46	93281	96.884	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	193.760%#
24) Chloroform-d	7.647	84	180549	23.155	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.640%
26) 1,2-Dichloroethane-d4	8.311	65	114774	25.763	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.040%
32) Benzene-d6	8.274	84	291951	31.415	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	125.680%
36) 1,2-Dichloropropane-d6	9.274	67	102566	38.138	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	152.560%#
41) Toluene-d8	10.323	98	194464	21.366	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.480%
43) trans-1,3-Dichloroprop...	10.579	79	28596	22.530	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.120%
47) 2-Hexanone-d5	10.920	63	65654	131.212	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	262.420%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	122746	53.678	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	214.720%#
66) 1,2-Dichlorobenzene-d4	13.847	152	37244	33.277	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	133.120%#
Target Compounds					Qvalue	
13) Acetone	4.123	43	3163m	4.825	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022629.D
Acq On : 26 Apr 2022 17:02
Operator : SY/VA
Sample : N2562-02RE
Misc : 7.09g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW462RE

Quant Time: Apr 27 01:40:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

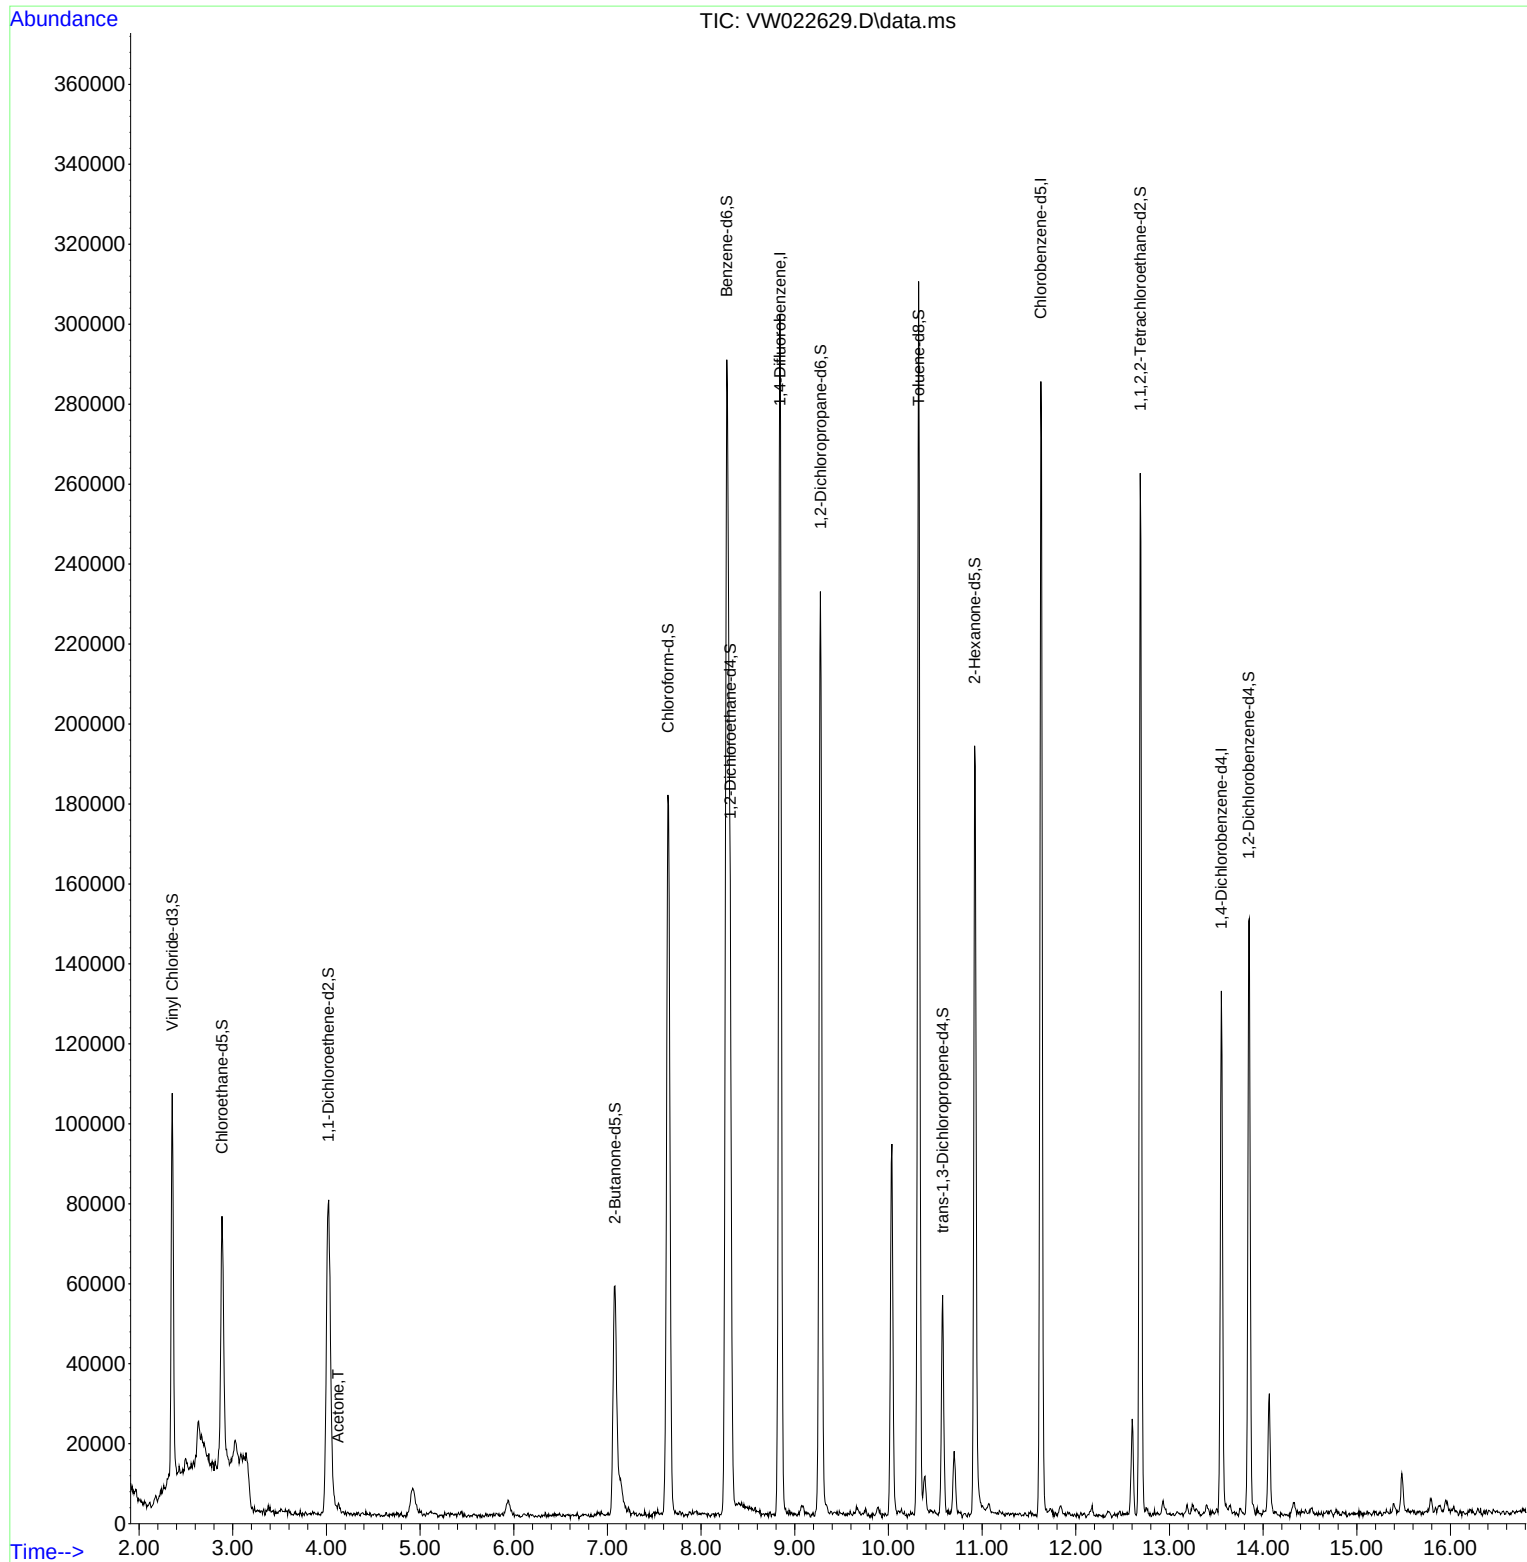

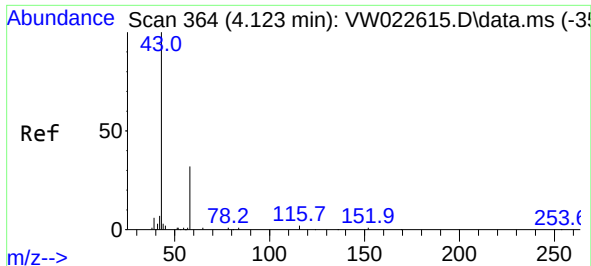

#13
Acetone
Concen: 4.825 ug/L m
RT: 4.123 min Scan# 30
Delta R.T. -0.000 min
Lab File: VW022629.D
Acq: 26 Apr 2022 17:02

Instrument :
MSVOA_W
ClientSampleId :
EW462RE

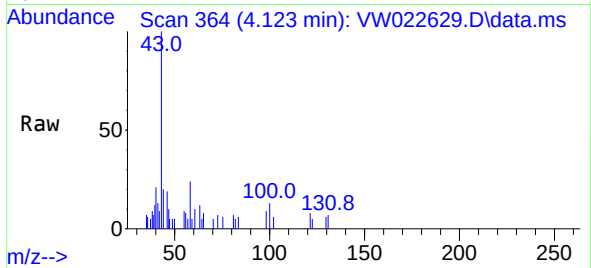

Tgt Ion: 43 Resp: 316
Ion Ratio Lower Upper
43 100
58 10.8 0.0 57.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

