

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
 Data File : VW022631.D
 Acq On : 26 Apr 2022 17:50
 Operator : SY/VA
 Sample : VIBLK436
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK436

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
 Supervised By :Mahesh Dadoda 04/29/2022

Quant Time: Apr 27 01:41:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 27 01:34:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	273976	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	271362	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	138598	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	125003	20.639	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	82.560%		
7) Chloroethane-d5	2.891	69	92658	24.410	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	97.640%		
11) 1,1-Dichloroethene-d2	4.019	63	129148m	16.440	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	65.760%		
21) 2-Butanone-d5	7.074	46	55830	52.798	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	105.600%		
24) Chloroform-d	7.653	84	203368	23.748	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	95.000%		
26) 1,2-Dichloroethane-d4	8.311	65	114947	23.493	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	93.960%		
32) Benzene-d6	8.275	84	396113	23.892	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	95.560%		
36) 1,2-Dichloropropane-d6	9.274	67	112735	23.497	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	94.000%		
41) Toluene-d8	10.323	98	369199	22.737	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	90.960%		
43) trans-1,3-Dichloroprop...	10.579	79	45203	19.963	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	79.840%		
47) 2-Hexanone-d5	10.927	63	44863	50.258	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	100.520%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	100284	24.582	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	98.320%		
66) 1,2-Dichlorobenzene-d4	13.853	152	119769	24.397	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	97.600%		
Target Compounds					Qvalue	
13) Acetone	4.135	43	6697	9.302	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042622\
Data File : VW022631.D
Acq On : 26 Apr 2022 17:50
Operator : SY/VA
Sample : VIBLK436
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VIBLK436

Quant Time: Apr 27 01:41:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 27 01:34:11 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 04/27/2022
Supervised By : Mahesh Dadoda 04/29/2022

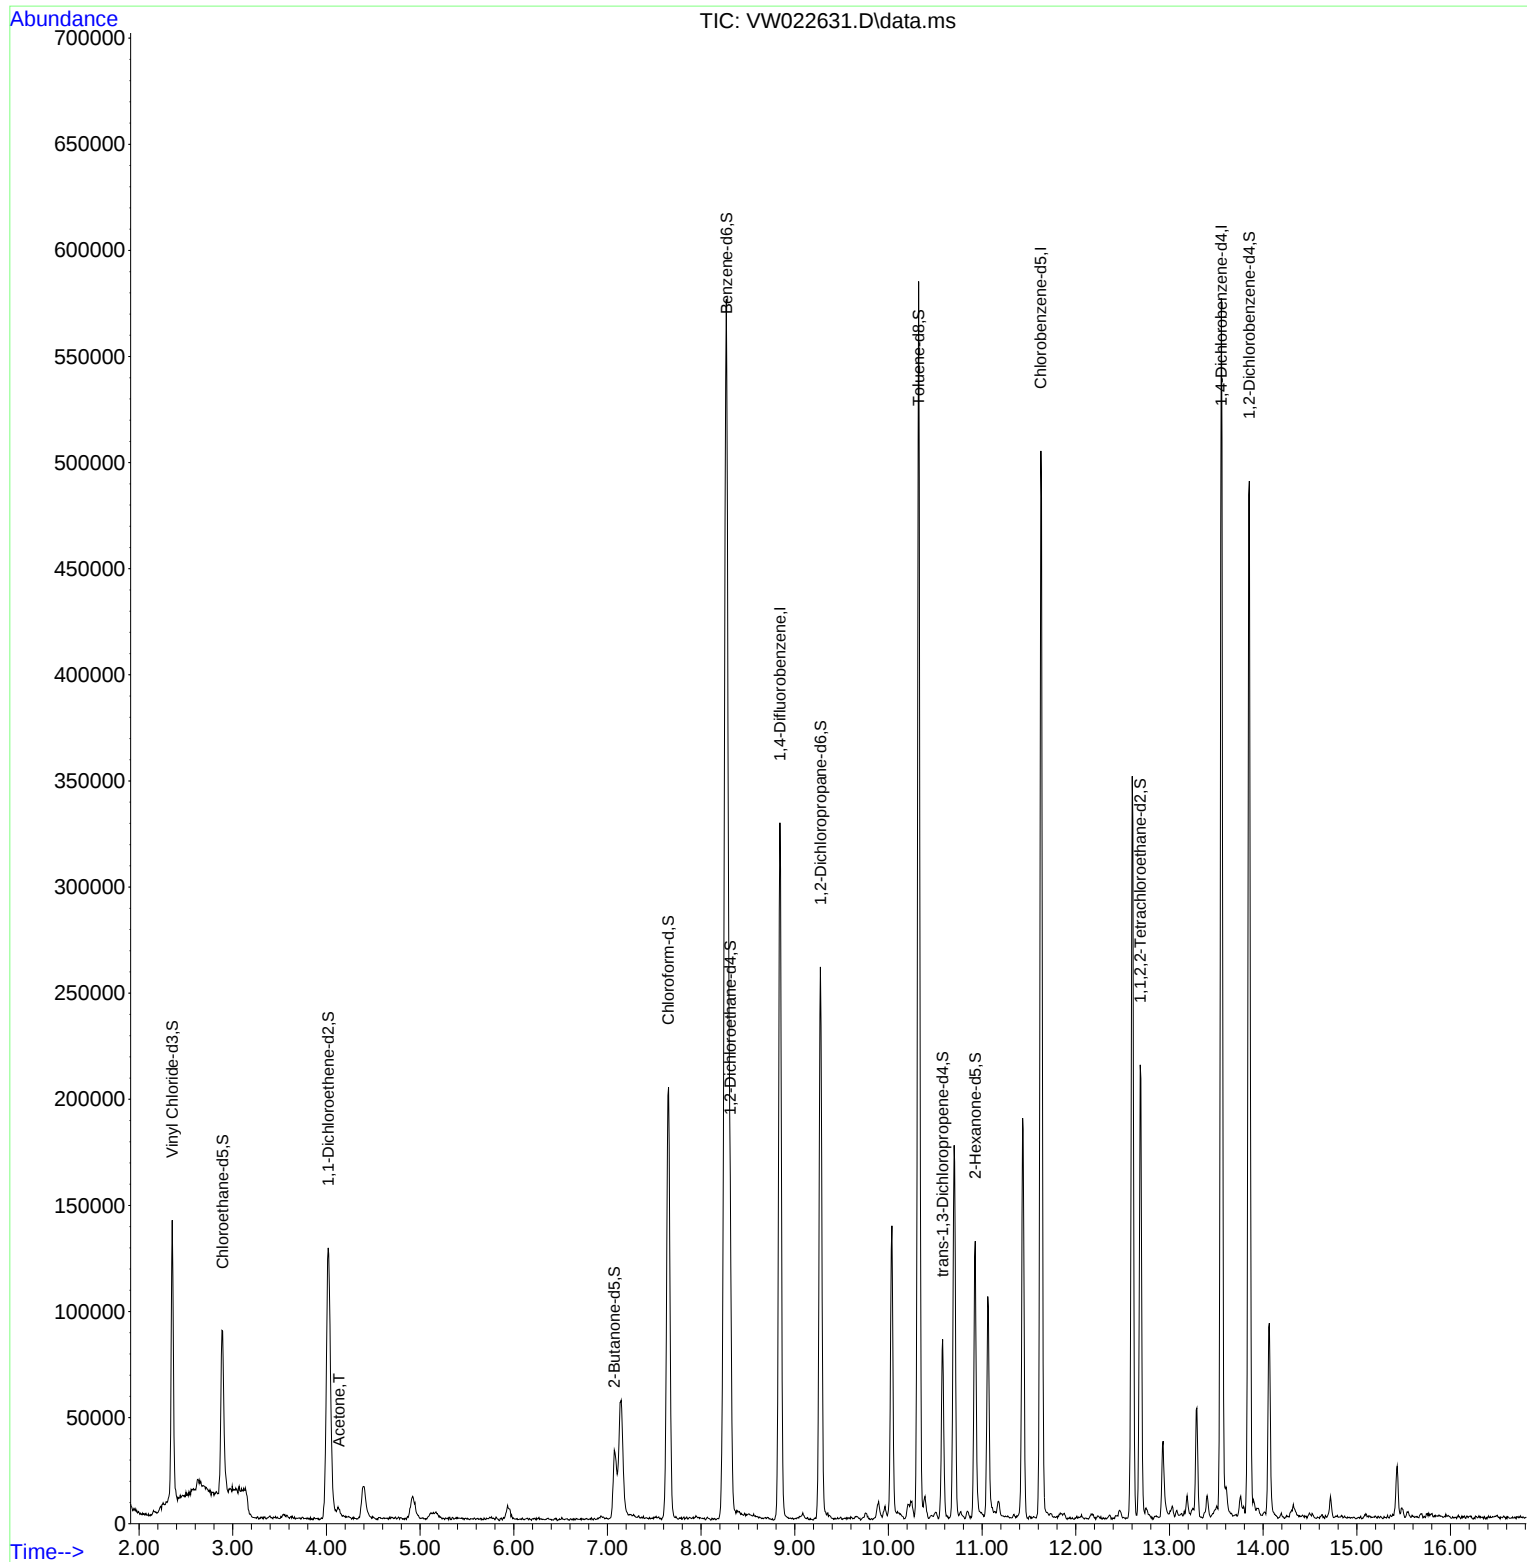

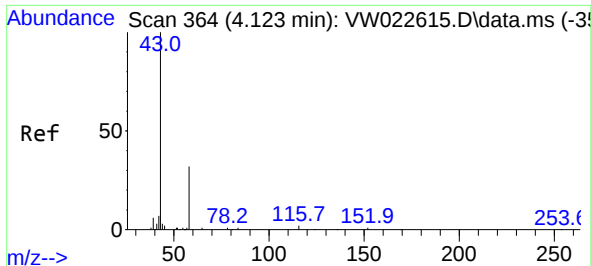

#13
Acetone
Concen: 9.302 ug/L
RT: 4.135 min Scan# 30
Delta R.T. 0.012 min
Lab File: VW022631.D
Acq: 26 Apr 2022 17:50

Instrument :
MSVOA_W
ClientSampleId :
VIBLK436

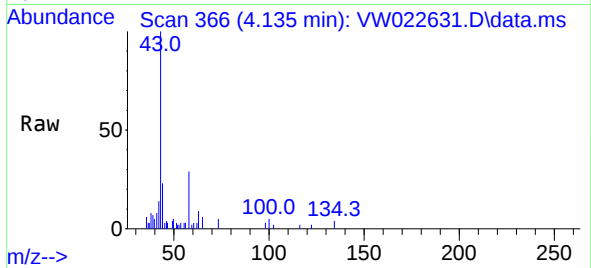

Tgt Ion: 43 Resp: 669
Ion Ratio Lower Upper
43 100
58 22.3 0.0 57.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2022
Supervised By :Mahesh Dadoda 04/29/2022

