




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042623\
 Data File : VW025710.D
 Acq On : 26 Apr 2023 18:30
 Operator : SY/MD
 Sample : 02499-09
 Misc : 6.16g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCG1

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:26:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 26 01:13:04 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/27/2023
 Supervised By :Mahesh Dadoda 05/01/2023

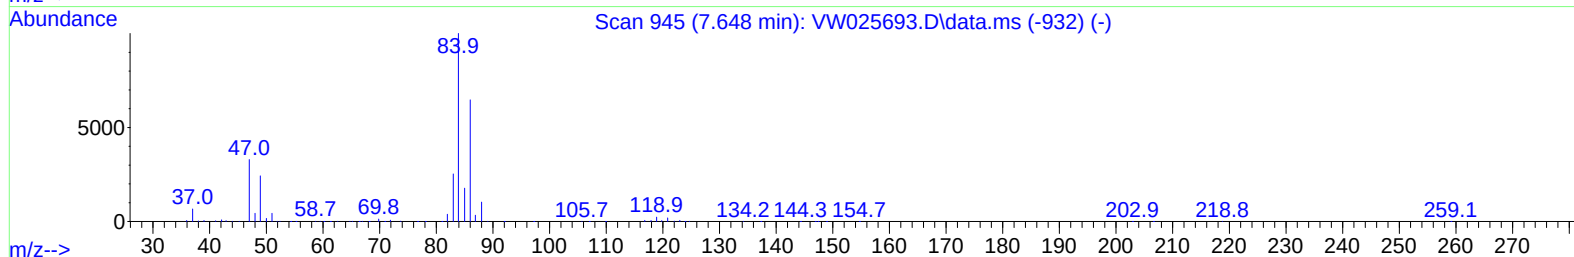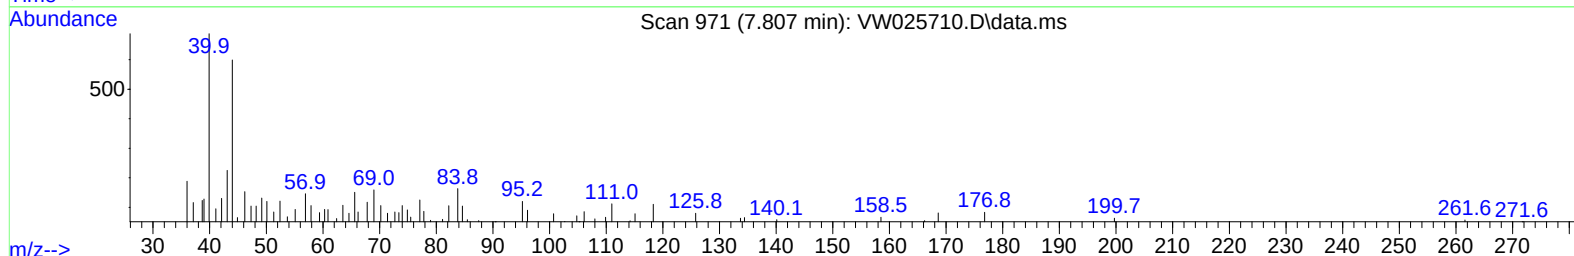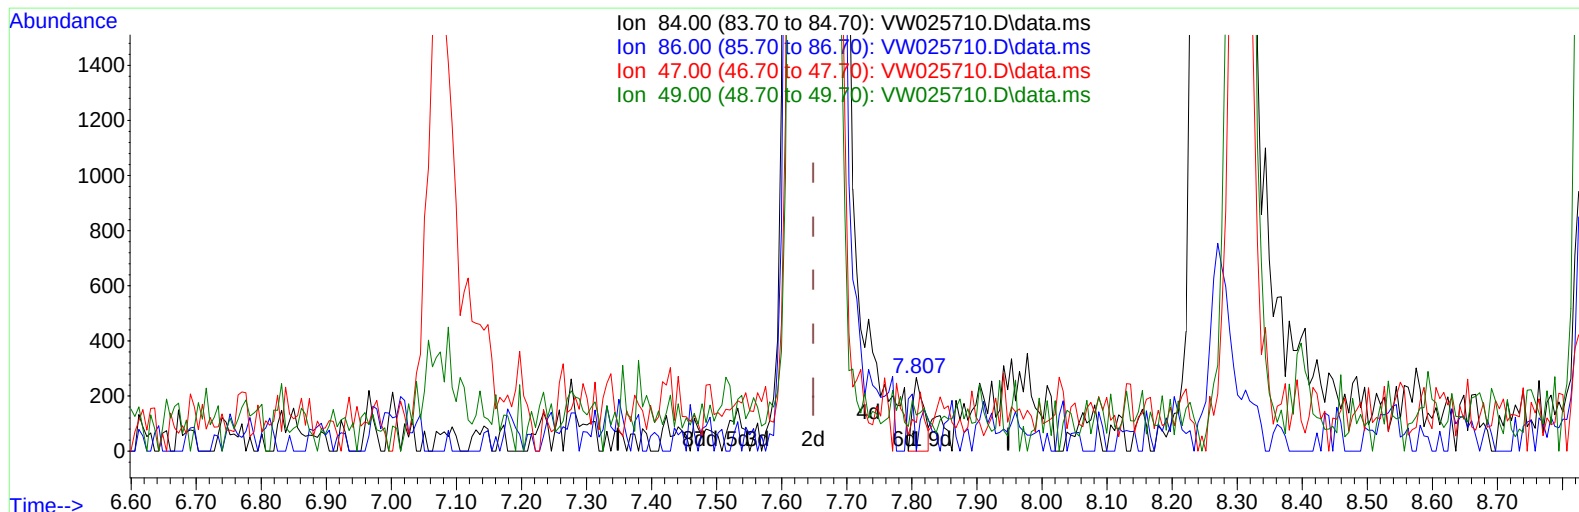

TIC: VW025710.D\data.ms

(24) Chloroform-d (S)

7.807min (+ 0.158) 0.02 ug/L

response 317

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.50	59.62
47.00	51.00	39.75
49.00	28.80	27.13




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042623\
 Data File : VW025710.D
 Acq On : 26 Apr 2023 18:30
 Operator : SY/MD
 Sample : 02499-09
 Misc : 6.16g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCG1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 27 01:26:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 26 01:13:04 2023
 Response via : Initial Calibration

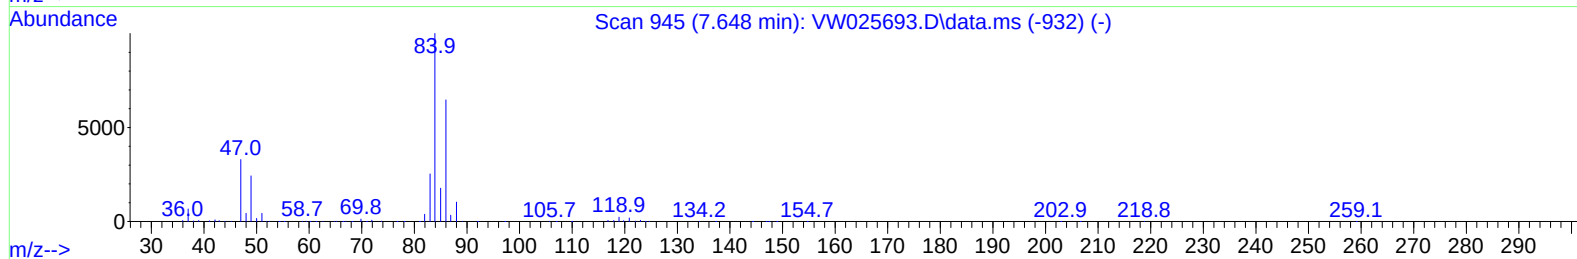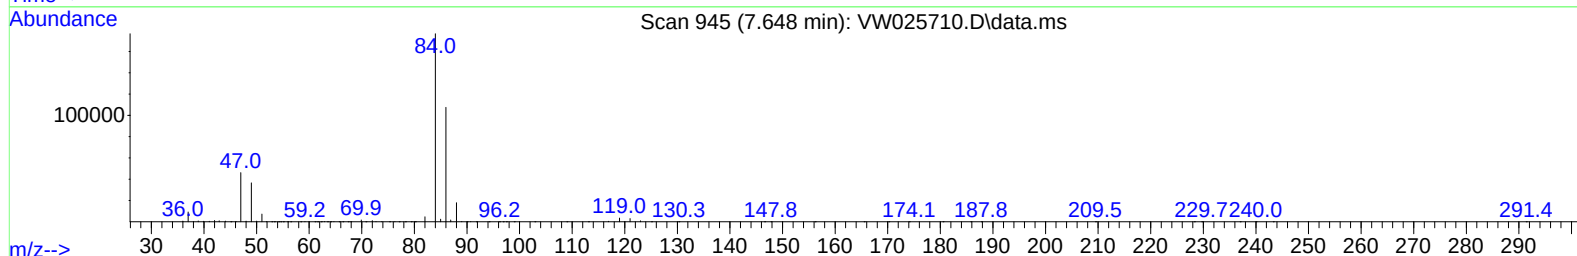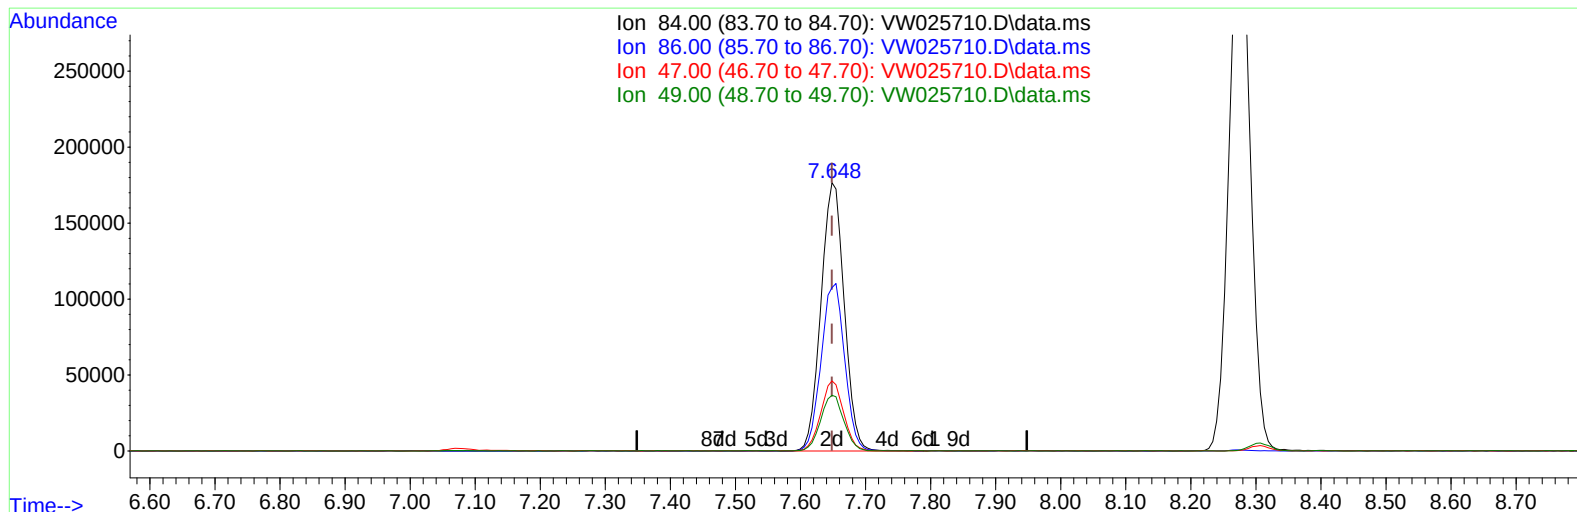

TIC: VW025710.D\data.ms

(24) Chloroform-d (S)

7.648min (-0.000) 21.16 ug/L m

response 438078

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.50	0.04#
47.00	51.00	0.03#
49.00	28.80	0.02#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042623\
 Data File : VW025710.D
 Acq On : 26 Apr 2023 18:30
 Operator : SY/MD
 Sample : 02499-09
 Misc : 6.16g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCG1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 27 01:26:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 26 01:13:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	737483	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	677227	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	302226	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	141615	11.800	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	47.200%		
7) Chloroethane-d5	2.899	69	120597	14.114	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	56.440%		
11) 1,1-Dichloroethene-d2	4.021	63	262646	10.822	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	43.280%#		
21) 2-Butanone-d5	7.075	46	196907	73.548	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	147.100%#		
24) Chloroform-d	7.648	84	438078m	21.156	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	84.640%		
26) 1,2-Dichloroethane-d4	8.307	65	264958	24.596	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	98.400%		
32) Benzene-d6	8.276	84	819257	18.683	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	74.720%		
36) 1,2-Dichloropropane-d6	9.270	67	294782	21.560	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	86.240%		
41) Toluene-d8	10.325	98	694339	18.127	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	72.520%		
43) trans-1,3-Dichloroprop...	10.581	79	107870	21.043	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	84.160%		
47) 2-Hexanone-d5	10.922	63	122196	65.384	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	130.760%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	274788	29.776	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	119.120%		
66) 1,2-Dichlorobenzene-d4	13.848	152	258288	24.876	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	99.520%		
Target Compounds					Qvalue	
13) Acetone	4.124	43	67041	29.587	ug/L	97
16) Methylene chloride	4.923	84	32933	2.809	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042623\
Data File : VW025710.D
Acq On : 26 Apr 2023 18:30
Operator : SY/MD
Sample : 02499-09
Misc : 6.16g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCG1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/27/2023
Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 27 01:26:44 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 26 01:13:04 2023
Response via : Initial Calibration

