

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042623\
 Data File : VW025694.D
 Acq On : 26 Apr 2023 10:22
 Operator : SY/MD
 Sample : VW0426SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK487

Quant Time: Apr 27 01:25:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 26 01:13:04 2023
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.843	114	644160	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.629	117	578902	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.556	152	267010	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.363	65	291185	27.779	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	111.120%	
7) Chloroethane-d5		2.899	69	204978	27.466	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	109.880%	
11) 1,1-Dichloroethene-d2		4.021	63	431203	20.341	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	81.360%	
21) 2-Butanone-d5		7.075	46	151293	64.698	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	129.400%	
24) Chloroform-d		7.648	84	488508	27.010	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	108.040%	
26) 1,2-Dichloroethane-d4		8.307	65	282764	30.051	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	120.200%	
32) Benzene-d6		8.270	84	1027401	27.409	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	109.640%	
36) 1,2-Dichloropropane-d6		9.270	67	324520	27.766	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	111.080%	
41) Toluene-d8		10.325	98	903352	27.589	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	110.360%	
43) trans-1,3-Dichloroprop...		10.575	79	127293	29.049	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	116.200%	
47) 2-Hexanone-d5		10.922	63	97121	60.793	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	121.580%	
56) 1,1,2,2-Tetrachloroeth...		12.690	84	225446	28.578	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	114.320%	
66) 1,2-Dichlorobenzene-d4		13.849	152	255061	27.805	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	111.240%	
Target Compounds							
16) Methylene chloride		4.917	84	32617	3.186	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042623\
Data File : VW025694.D
Acq On : 26 Apr 2023 10:22
Operator : SY/MD
Sample : VW0426SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK487


Quant Time: Apr 27 01:25:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 26 01:13:04 2023
Response via : Initial Calibration

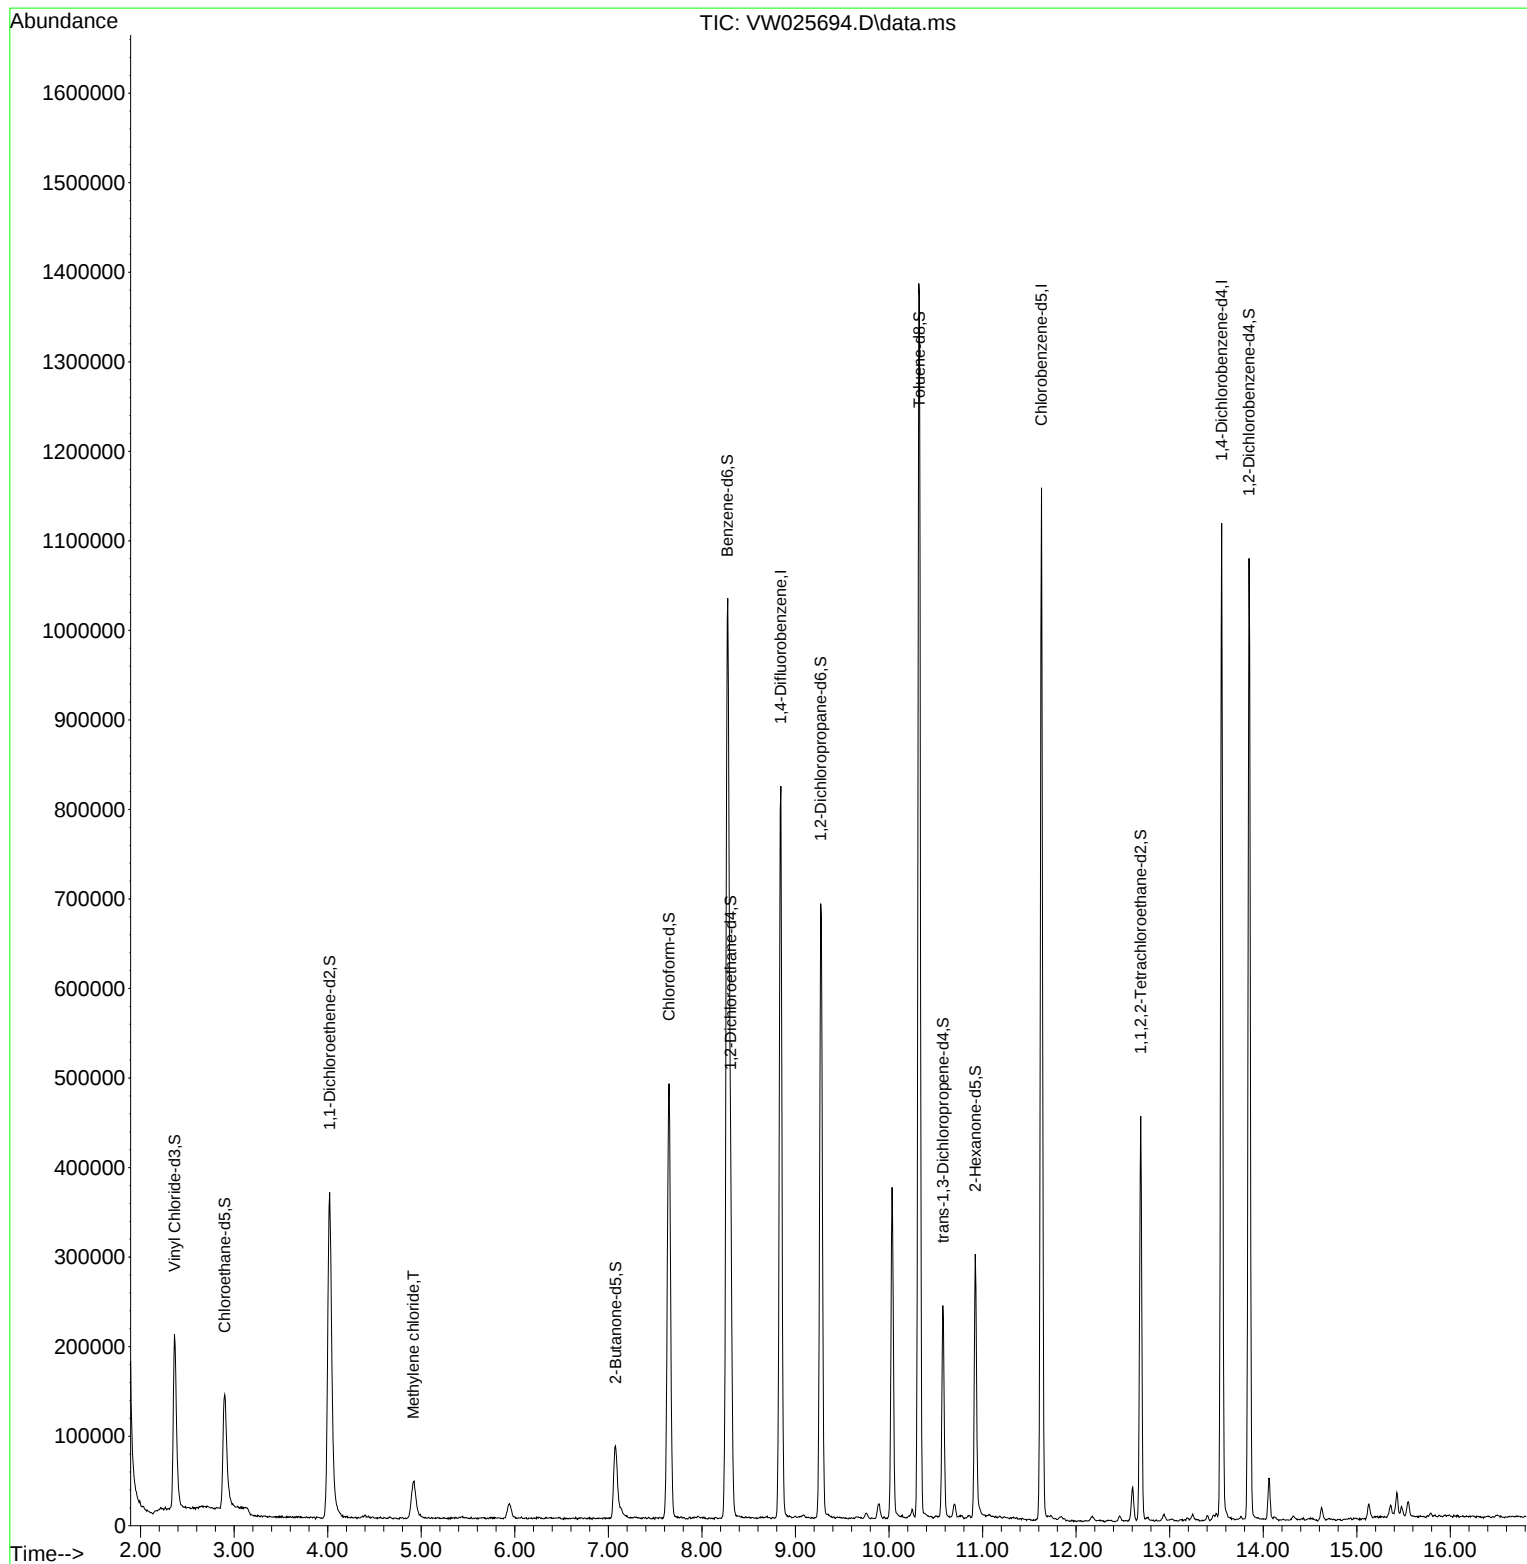

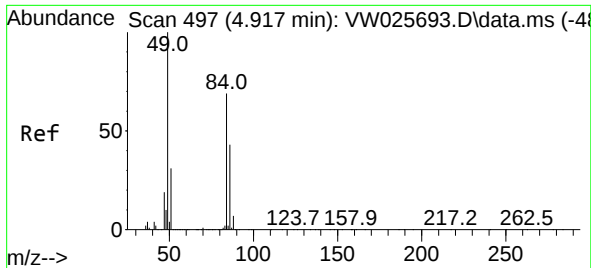

#16
Methylene chloride
Concen: 3.186 ug/L
RT: 4.917 min Scan# 49
Delta R.T. 0.000 min
Lab File: VW025694.D
Acq: 26 Apr 2023 10:22

Instrument :
MSVOA_W
ClientSampleId :
VBLK487

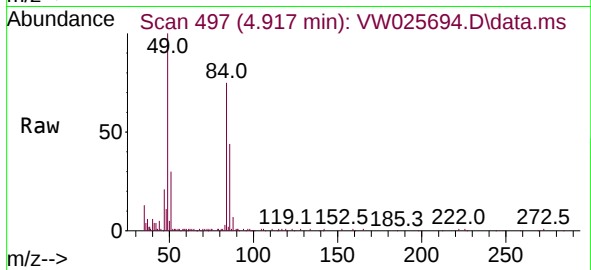

Tgt Ion: 84 Resp: 32617

Ion	Ratio	Lower	Upper
84	100		
86	58.3	44.9	83.3
49	133.7	101.4	188.4

