

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042723\
 Data File : VW025723.D
 Acq On : 27 Apr 2023 13:57
 Operator : SY/MD
 Sample : VW0427SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK489

Quant Time: Apr 28 03:00:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 28 02:55:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	668370	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	608140	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	279983	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	179587	22.027	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.120%
7) Chloroethane-d5	2.899	69	131796	22.547	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.200%
11) 1,1-Dichloroethene-d2	4.021	63	296113	15.930	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.720%
21) 2-Butanone-d5	7.075	46	129995	48.317	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.640%
24) Chloroform-d	7.648	84	424934	23.700	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.800%
26) 1,2-Dichloroethane-d4	8.307	65	242213	24.779	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.120%
32) Benzene-d6	8.276	84	874124	23.675	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.720%
36) 1,2-Dichloropropane-d6	9.270	67	283562	23.744	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.960%
41) Toluene-d8	10.319	98	772304	23.662	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.640%
43) trans-1,3-Dichloroprop...	10.581	79	106969	22.985	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.920%
47) 2-Hexanone-d5	10.922	63	91502	49.332	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.660%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	210768	23.947	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.800%
66) 1,2-Dichlorobenzene-d4	13.849	152	236201	24.624	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.480%
Target Compounds						
16) Methylene chloride	4.917	84	26088	2.066	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042723\
Data File : VW025723.D
Acq On : 27 Apr 2023 13:57
Operator : SY/MD
Sample : VW0427SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK489


Quant Time: Apr 28 03:00:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 28 02:55:08 2023
Response via : Initial Calibration

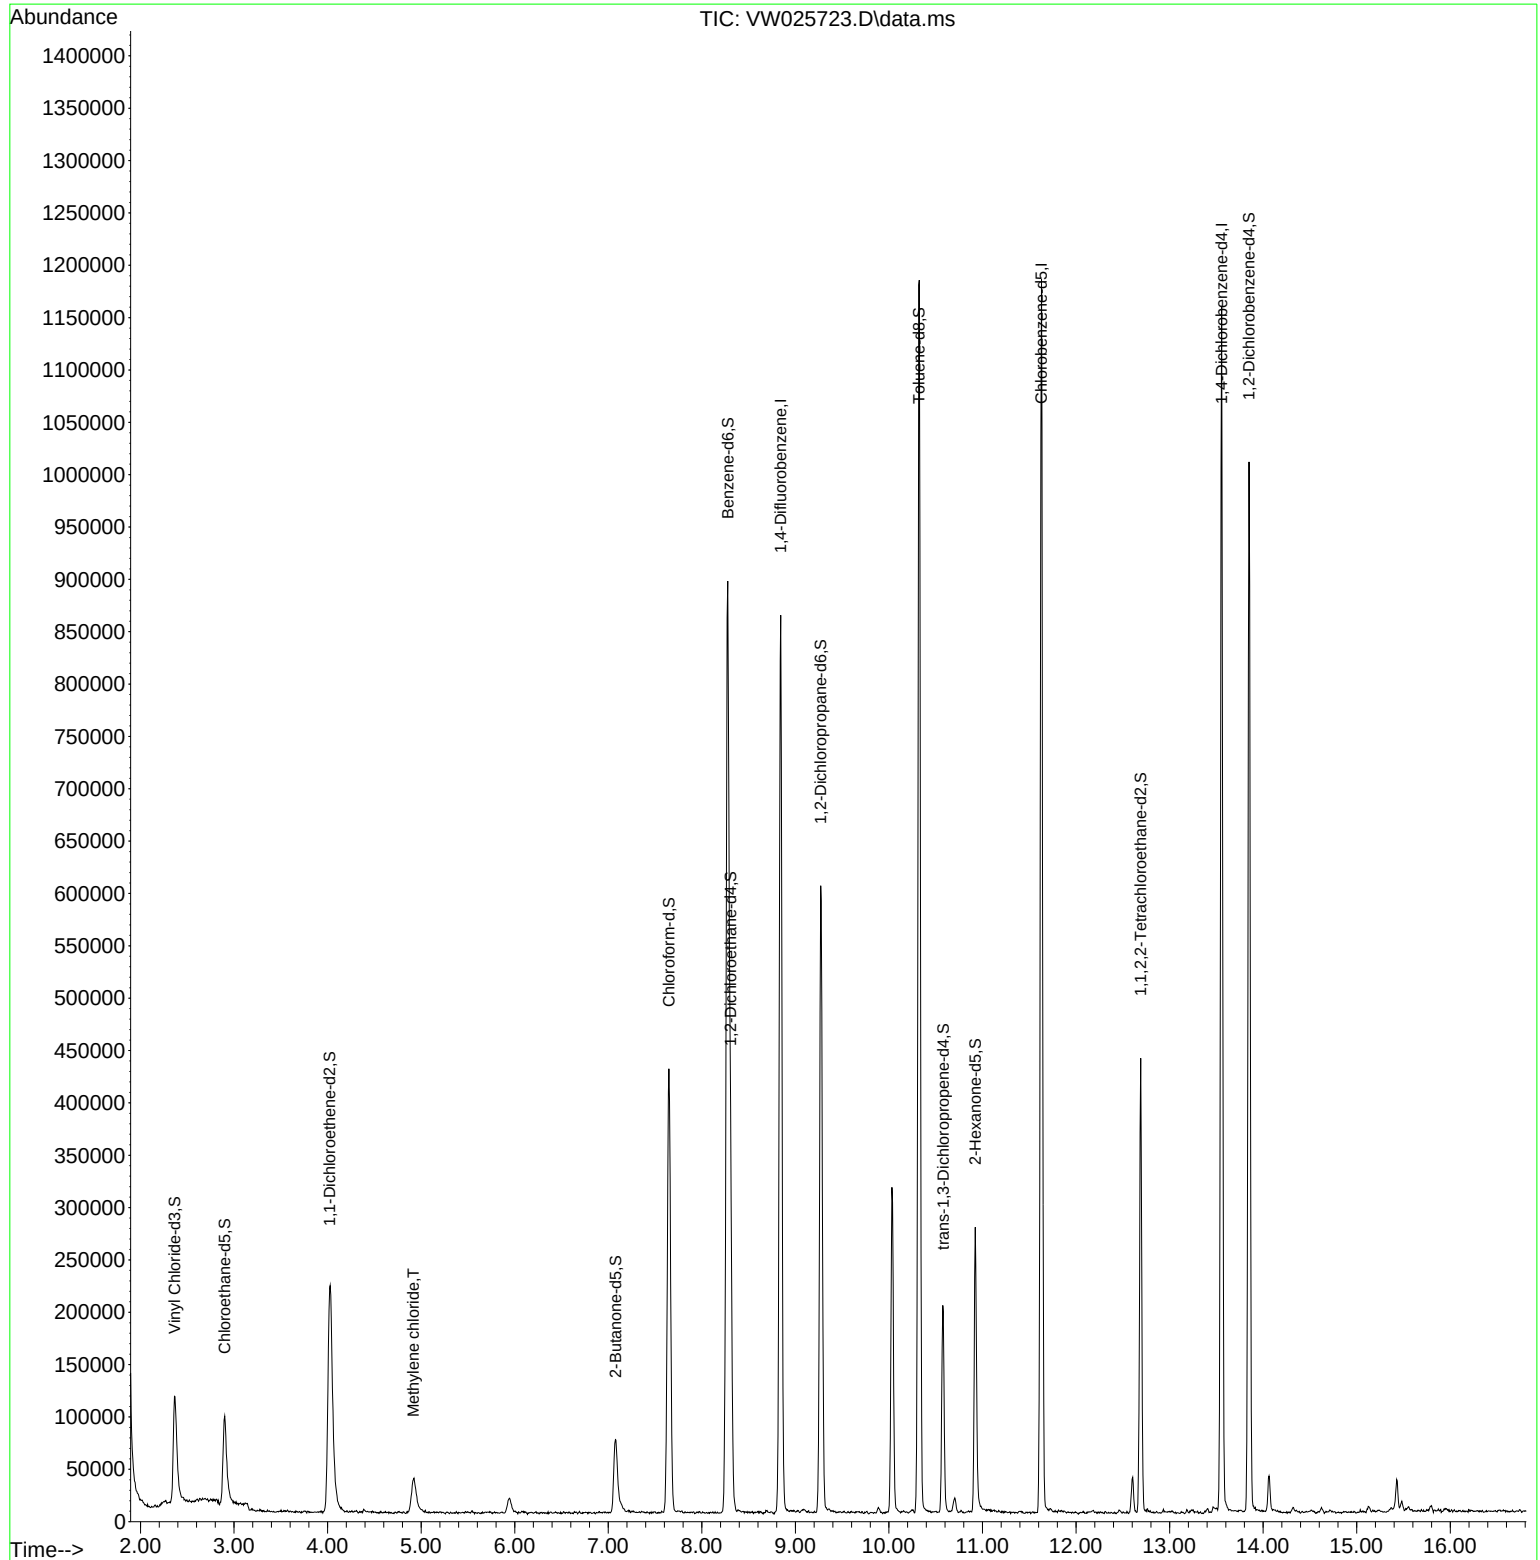

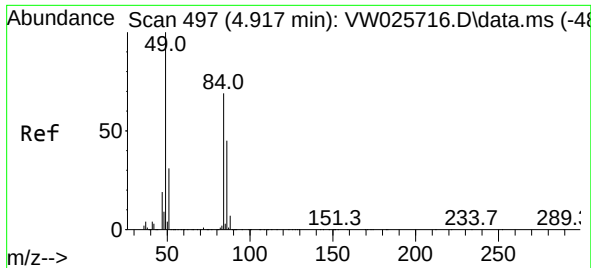

#16
Methylene chloride
Concen: 2.066 ug/L
RT: 4.917 min Scan# 49
Delta R.T. 0.000 min
Lab File: VW025723.D
Acq: 27 Apr 2023 13:57

Instrument :
MSVOA_W
ClientSampleId :
VBLK489

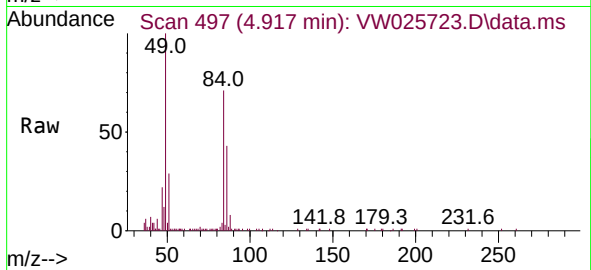

Tgt Ion	Ratio	Lower	Upper
84	100		
86	60.5	46.3	85.9
49	141.0	101.9	189.3

