

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042723\
 Data File : VW025724.D
 Acq On : 27 Apr 2023 14:21
 Operator : SY/MD
 Sample : 02499-18
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCT3

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/28/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 28 03:00:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 28 02:55:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	644235	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	573605	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	279307	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	168680	21.464	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.840%
7) Chloroethane-d5	2.899	69	119277	21.169	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.680%
11) 1,1-Dichloroethene-d2	4.027	63	374605	20.908	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	83.640%
21) 2-Butanone-d5	7.075	46	149602	57.688	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	115.380%
24) Chloroform-d	7.648	84	371127	21.474	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.880%
26) 1,2-Dichloroethane-d4	8.307	65	225523	23.936	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.760%
32) Benzene-d6	8.276	84	780813	22.421	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.680%
36) 1,2-Dichloropropane-d6	9.270	67	254475	22.591	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.360%
41) Toluene-d8	10.325	98	684821	22.244	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.960%
43) trans-1,3-Dichloroprop...	10.575	79	100768	22.956	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.840%
47) 2-Hexanone-d5	10.922	63	105292	60.184	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	120.360%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	218186	26.282	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.120%
66) 1,2-Dichlorobenzene-d4	13.848	152	226239	23.643	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.560%
Target Compounds						
					Qvalue	
3) Chloromethane	2.222	50	200039	18.563	ug/L	97
6) Bromomethane	2.783	94	39197	6.539	ug/L	96
9) Trichlorofluoromethane	3.265	101	112086	13.161	ug/L	98
12) 1,1-Dichloroethene	4.039	96	160771m	18.461	ug/L	
13) Acetone	4.118	43	219295	91.230	ug/L	100
15) Methyl Acetate	4.667	43	210972	44.314	ug/L	100
16) Methylene chloride	4.917	84	114957	9.446	ug/L	97
17) trans-1,2-Dichloroethene	5.429	96	90566	9.873	ug/L	99
18) Methyl tert-butyl Ether	5.423	73	423716	32.097	ug/L	100
20) cis-1,2-Dichloroethene	7.173	96	239427	24.883	ug/L	100
23) Bromochloromethane	7.514	128	59831	14.973	ug/L	96
27) 1,2-Dichloroethane	8.398	62	118674	10.098	ug/L	100
29) Cyclohexane	7.959	56	165135	9.254	ug/L	100
30) 1,1,1-Trichloroethane	7.874	97	129992	9.308	ug/L	100
31) Carbon tetrachloride	8.069	117	149892	11.830	ug/L	97
34) Trichloroethene	9.093	95	375646	37.151	ug/L	96
35) Methylcyclohexane	9.337	83	438324	24.390	ug/L	100
37) 1,2-Dichloropropane	9.367	63	130245	12.343	ug/L	98
38) Bromodichloromethane	9.642	83	238482	19.996	ug/L	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042723\
 Data File : VW025724.D
 Acq On : 27 Apr 2023 14:21
 Operator : SY/MD
 Sample : 02499-18
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCT3

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/28/2023
 Supervised By : Mahesh Dadoda 05/01/2023

Quant Time: Apr 28 03:00:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 28 02:55:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

39) cis-1,3-Dichloropropene	10.069	75	229599	15.195	ug/L	97
42) Toluene	10.386	91	779680	19.523	ug/L	99
44) trans-1,3-Dichloropropene	10.605	75	93196	7.507	ug/L	97
46) Tetrachloroethene	10.861	164	264368	36.920	ug/L	93
48) 2-Hexanone	10.965	43	211274	47.140	ug/L	99
49) Dibromochloromethane	11.123	129	150006	21.182	ug/L	98
52) Ethylbenzene	11.727	91	646952	14.446	ug/L	97
53) m,p-Xylene	11.843	106	157251	9.511	ug/L	97
54) o-Xylene	12.166	106	176676	11.461	ug/L	94
60) Isopropylbenzene	12.458	105	503512	11.738	ug/L	97
64) 1,3-Dichlorobenzene	13.495	146	335241	18.518	ug/L	91
67) 1,2-Dichlorobenzene	13.867	146	153101	9.586	ug/L	97
68) 1,2-Dibromo-3-chloropr...	14.476	75	30519	21.945	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042723\
 Data File : VW025724.D
 Acq On : 27 Apr 2023 14:21
 Operator : SY/MD
 Sample : 02499-18
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1


Instrument :
 MSVOA_W
 ClientSampleId :
 DCCT3

Quant Time: Apr 28 03:00:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 28 02:55:08 2023
 Response via : Initial Calibration

Manual Integrations APPROVED


Reviewed By : Semsettin Yesilyurt 04/28/2023
 Supervised By : Mahesh Dadoda 05/01/2023

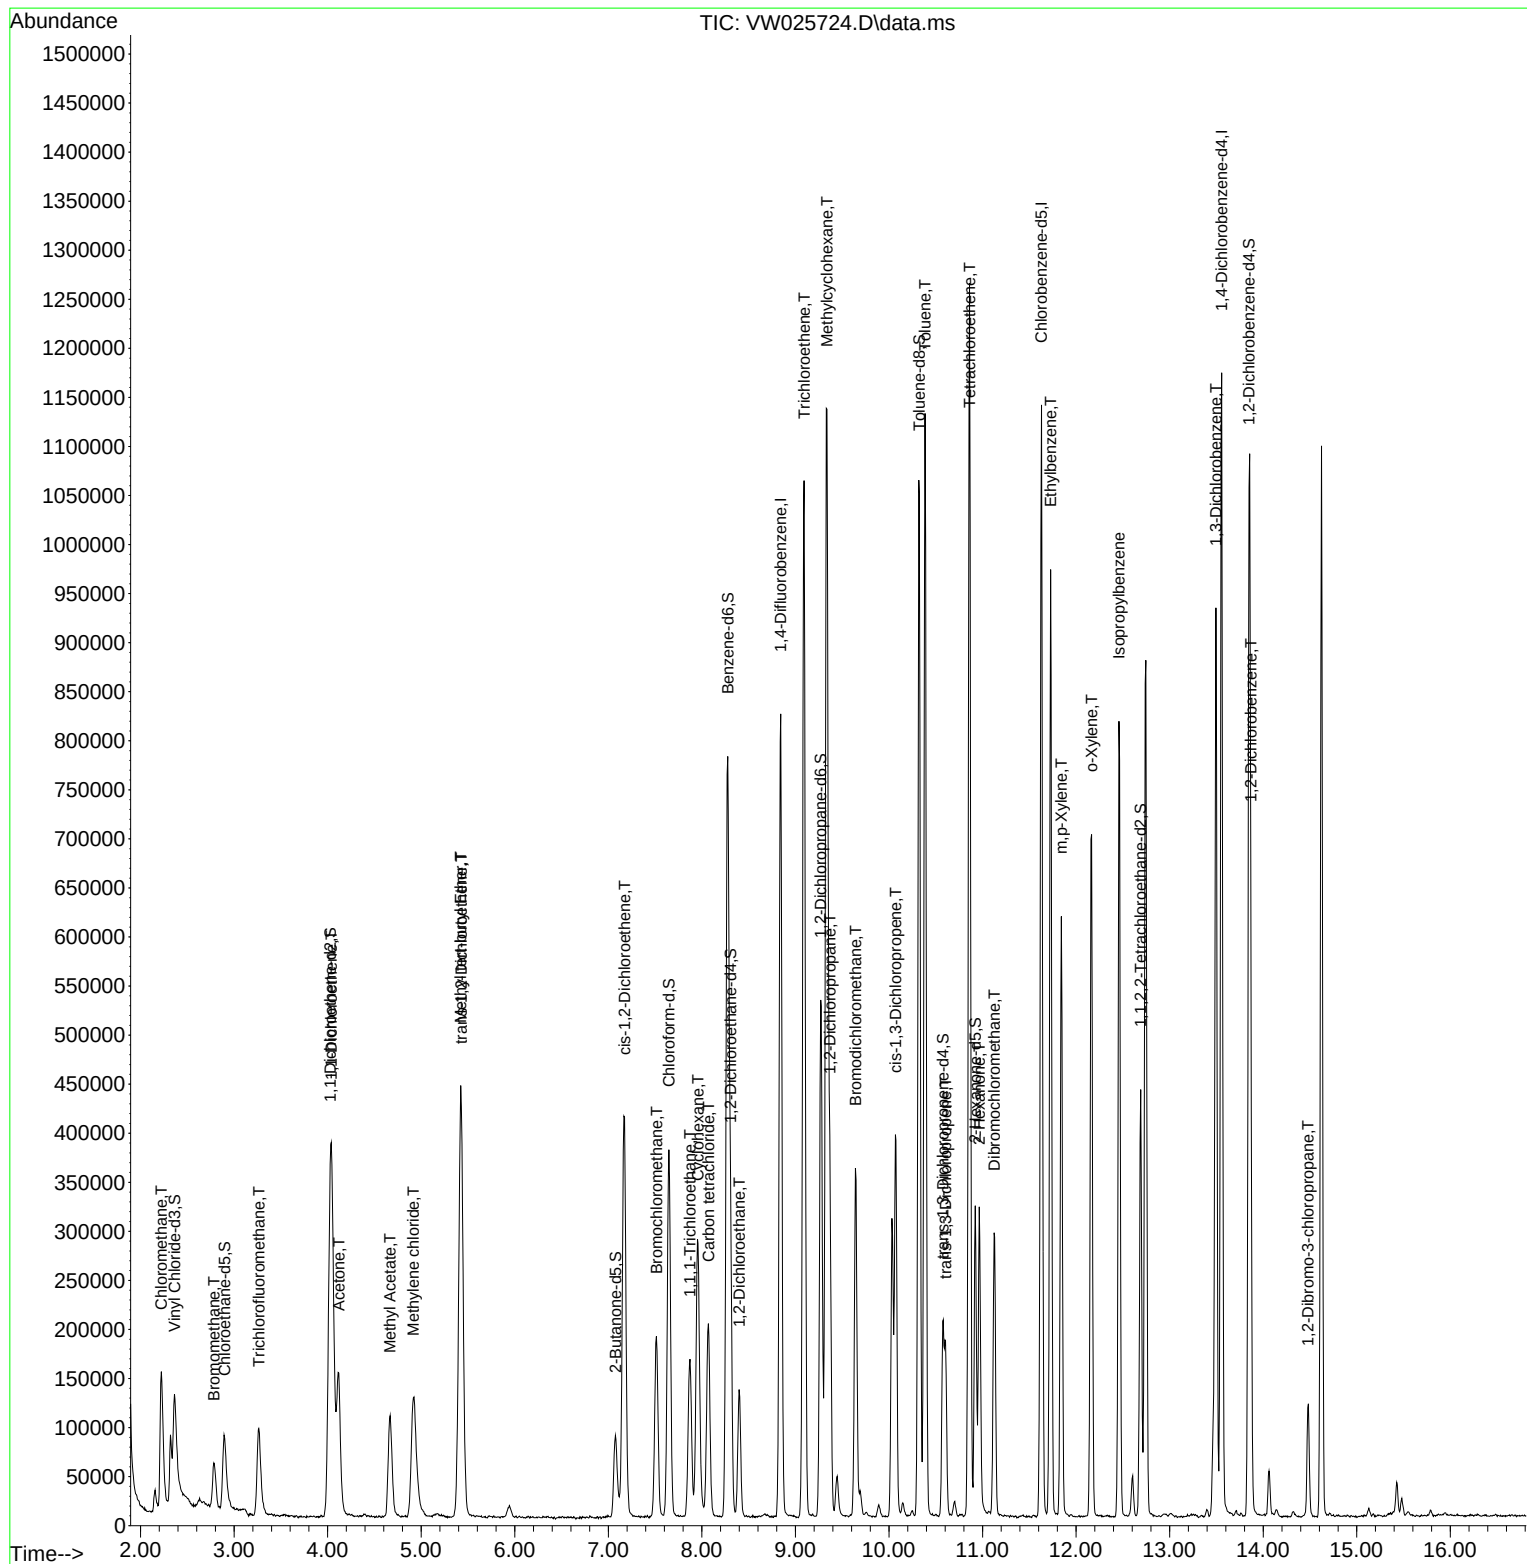



#3
Chloromethane
Concen: 18.563 ug/L
RT: 2.222 min Scan# 50
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21




Instrument :
MSVOA_W
ClientSampleId :
DCCT3




Tgt Ion: 50 Resp: 200039
Ion Ratio Lower Upper
50 100
52 31.3 22.9 42.5

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 04/28/2023
Supervised By :Mahesh Dadoda 05/01/2023

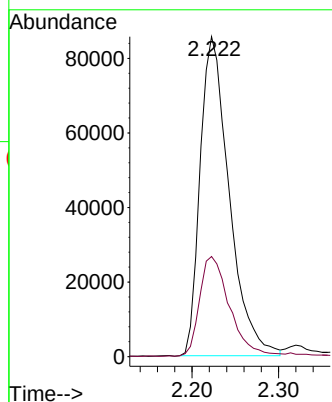


#6
Bromomethane
Concen: 6.539 ug/L
RT: 2.783 min Scan# 147
Delta R.T. -0.006 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21




Tgt Ion: 94 Resp: 39197
Ion Ratio Lower Upper
94 100
96 89.0 65.2 121.2

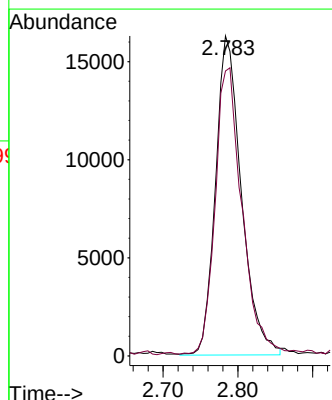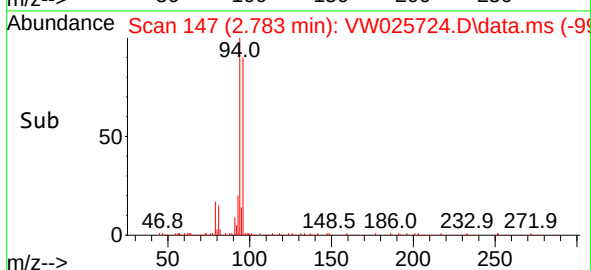



#9
 Trichlorofluoromethane
 Concen: 13.161 ug/L
 RT: 3.265 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VW025724.D
 Acq: 27 Apr 2023 14:21




Instrument :
 MSVOA_W
 ClientSampleId :
 DCCT3




Tgt Ion:101 Resp: 112086
 Ion Ratio Lower Upper
 101 100
 103 66.8 52.2 78.4

Manual Integrations
 APPROVED



Reviewed By :Semsettin Yesilyurt 04/28/2023
 Supervised By :Mahesh Dadoda 05/01/2023

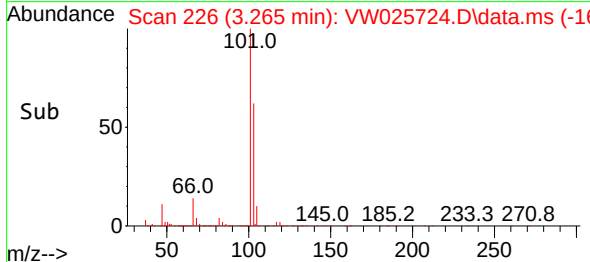


#12
 1,1-Dichloroethene
 Concen: 18.461 ug/L m
 RT: 4.039 min Scan# 353
 Delta R.T. -0.006 min
 Lab File: VW025724.D
 Acq: 27 Apr 2023 14:21

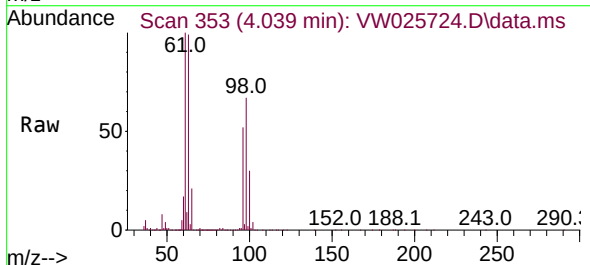


Tgt Ion: 96 Resp: 160771
 Ion Ratio Lower Upper
 96 100
 61 193.1 137.9 256.1
 63 191.2 90.5 168.1#

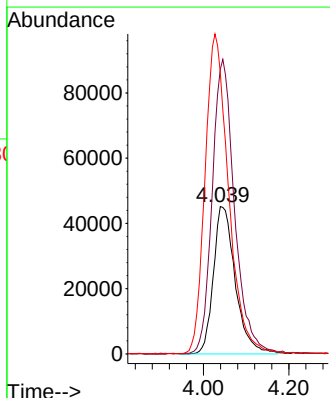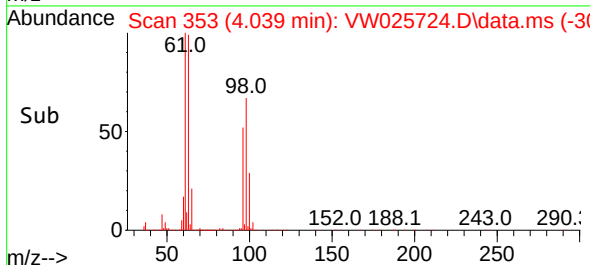



#13
Acetone
Concen: 91.230 ug/L
RT: 4.118 min Scan# 366
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21




Instrument :
MSVOA_W
Client Sample Id :
DCCT3



Tgt Ion: 43 Resp: 219295
Ion Ratio Lower Upper
43 100
58 29.1 0.0 58.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/28/2023
Supervised By :Mahesh Dadoda 05/01/2023

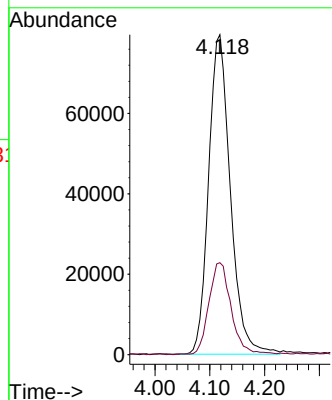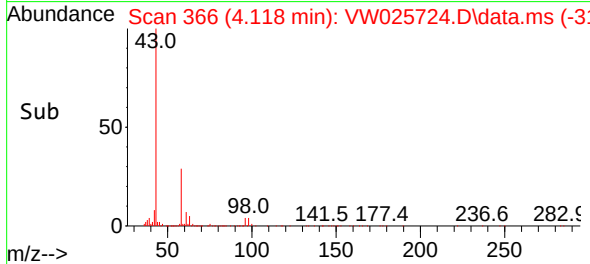

#15
Methyl Acetate
Concen: 44.314 ug/L
RT: 4.667 min Scan# 456
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21


Tgt Ion: 43 Resp: 210972
Ion Ratio Lower Upper
43 100
74 20.2 16.1 24.1

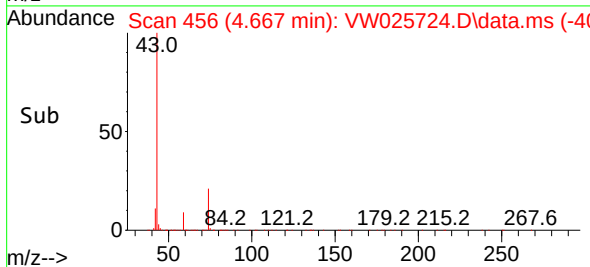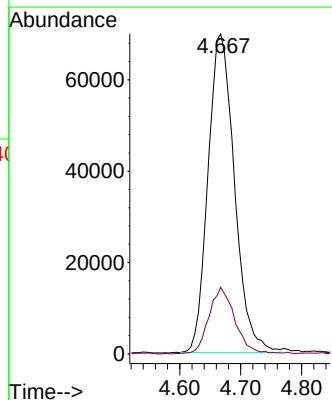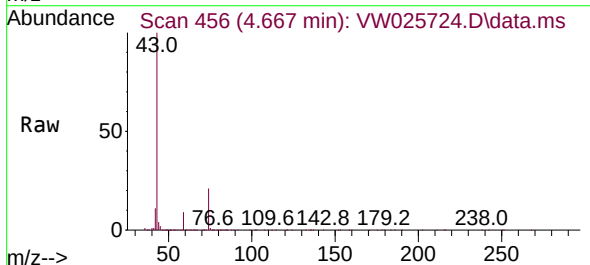



#16
Methylene chloride
Concen: 9.446 ug/L
RT: 4.917 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21




Instrument :
MSVOA_W
ClientSampleId :
DCCT3




Tgt Ion: 84 Resp: 114952
Ion Ratio Lower Upper
84 100
86 58.9 46.3 85.9
49 145.0 101.9 189.3

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 04/28/2023
Supervised By :Mahesh Dadoda 05/01/2023

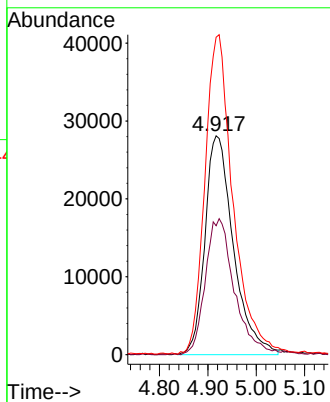


#17
trans-1,2-Dichloroethene
Concen: 9.873 ug/L
RT: 5.429 min Scan# 581
Delta R.T. 0.006 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21

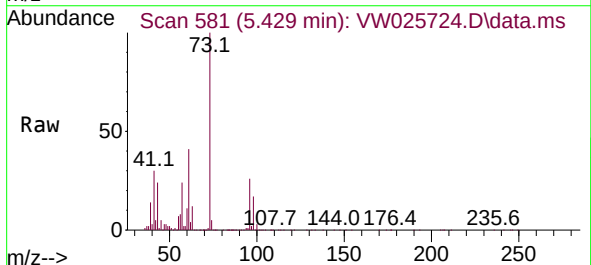


Tgt Ion: 96 Resp: 90566
Ion Ratio Lower Upper
96 100
61 158.3 110.2 204.8
98 64.4 44.8 83.2

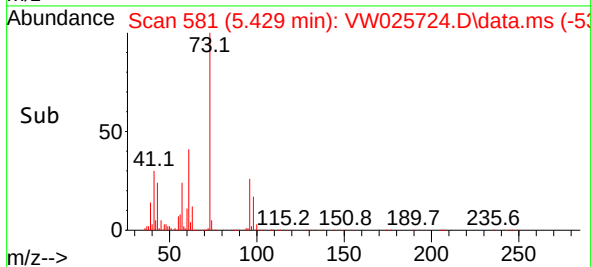



#18
Methyl tert-butyl Ether
Concen: 32.097 ug/L
RT: 5.423 min Scan# 580
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21




Instrument :
MSVOA_W
ClientSampleId :
DCCT3




Tgt Ion: 73 Resp: 423716
Ion Ratio Lower Upper
73 100
43 22.7 18.2 27.4
57 24.1 19.3 28.9

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 04/28/2023
Supervised By :Mahesh Dadoda 05/01/2023




#20
cis-1,2-Dichloroethene
Concen: 24.883 ug/L
RT: 7.173 min Scan# 867
Delta R.T. 0.006 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21




Tgt Ion: 96 Resp: 239427
Ion Ratio Lower Upper
96 100
61 145.4 101.6 188.6
68 0.1 0.1 0.1

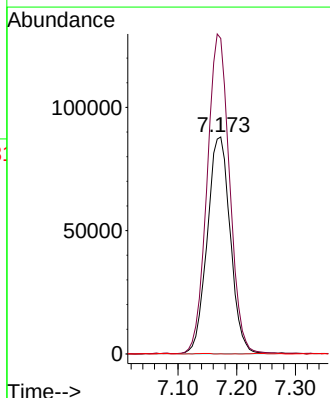



#23
Bromochloromethane
Concen: 14.973 ug/L
RT: 7.514 min Scan# 91
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21




Instrument :
MSVOA_W
ClientSampleId :
DCCT3



Tgt Ion:128 Resp: 59831
Ion Ratio Lower Upper
128 100
49 216.5 148.0 274.8
130 122.0 90.3 167.7
51 66.1 53.0 79.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/28/2023
Supervised By :Mahesh Dadoda 05/01/2023

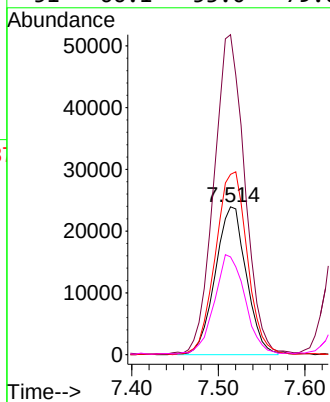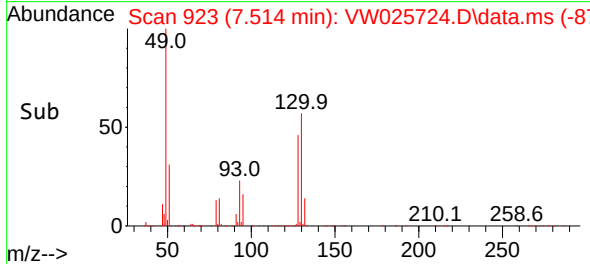

#27
1,2-Dichloroethane
Concen: 10.098 ug/L
RT: 8.398 min Scan# 1068
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21


Tgt Ion: 62 Resp: 118674
Ion Ratio Lower Upper
62 100
98 8.1 6.5 9.7

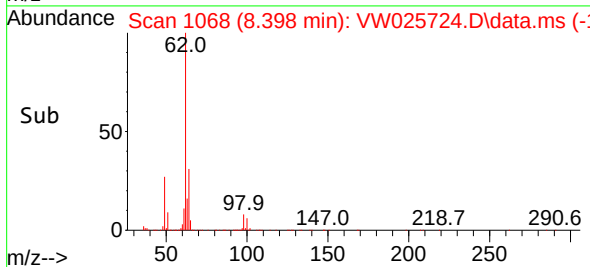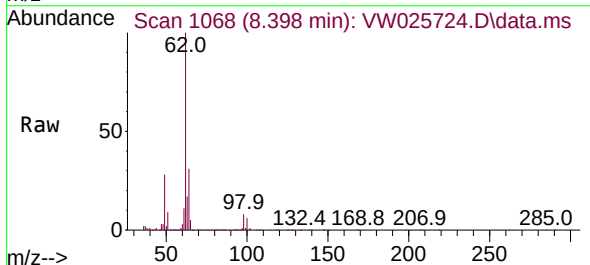



#29
Cyclohexane
Concen: 9.254 ug/L
RT: 7.959 min Scan# 996
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21




Instrument :
MSVOA_W
Client Sample Id :
DCCT3



Tgt Ion: 56 Resp: 165135
Ion Ratio Lower Upper
56 100
69 28.5 22.6 34.0
84 77.2 62.2 93.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/28/2023
Supervised By :Mahesh Dadoda 05/01/2023

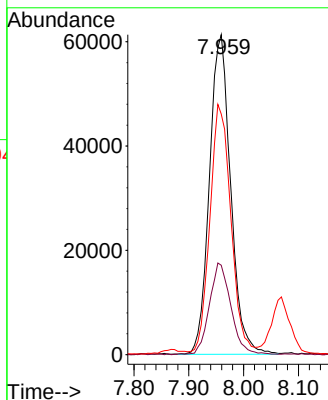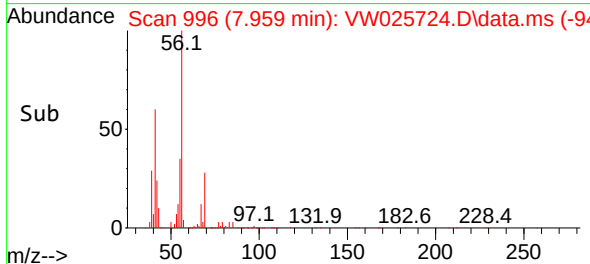

#30
1,1,1-Trichloroethane
Concen: 9.308 ug/L
RT: 7.874 min Scan# 982
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21


Tgt Ion: 97 Resp: 129992
Ion Ratio Lower Upper
97 100
99 64.0 51.0 76.4
61 53.0 42.2 63.2

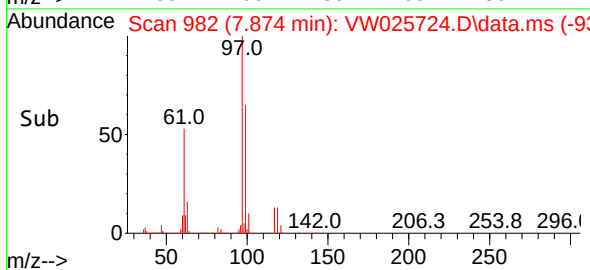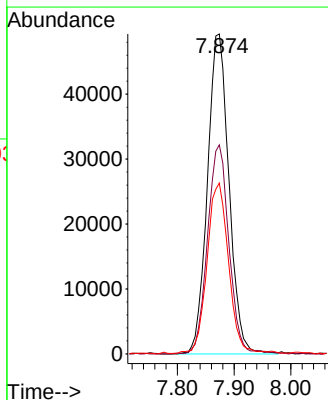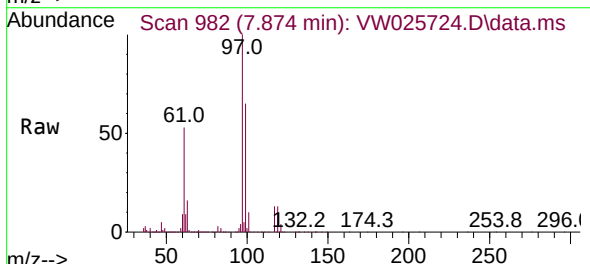

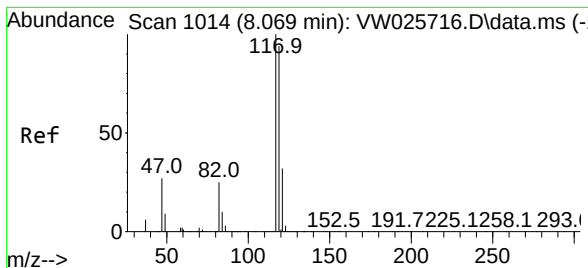

#31
Carbon tetrachloride
Concen: 11.830 ug/L
RT: 8.069 min Scan# 1014
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21




Instrument :
MSVOA_W
ClientSampleId :
DCCT3

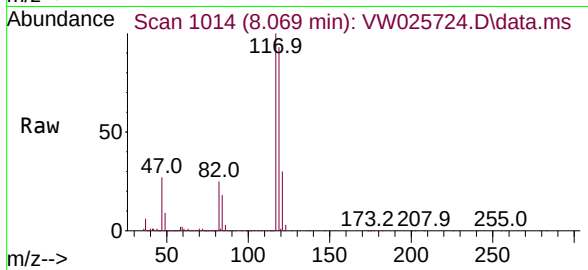

Tgt Ion: 117 Resp: 149892
Ion Ratio Lower Upper
117 100
119 93.6 77.4 116.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/28/2023
Supervised By :Mahesh Dadoda 05/01/2023

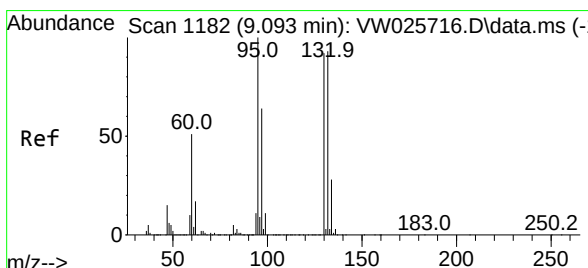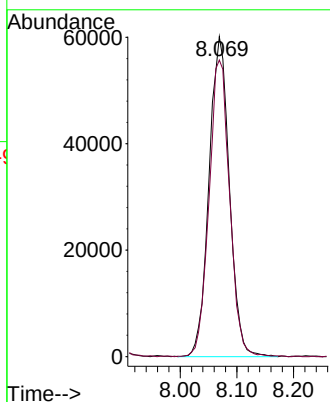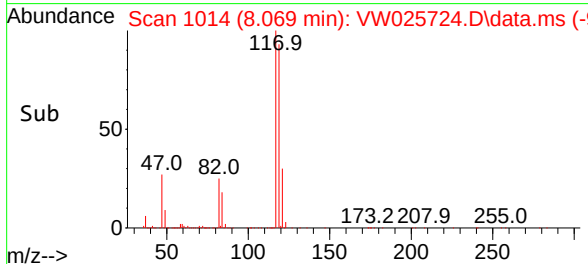

#34
Trichloroethene
Concen: 37.151 ug/L
RT: 9.093 min Scan# 1182
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21


Tgt Ion: 95 Resp: 375646
Ion Ratio Lower Upper
95 100
97 65.5 44.7 83.1
132 90.3 65.0 120.6
130 99.2 64.5 119.9

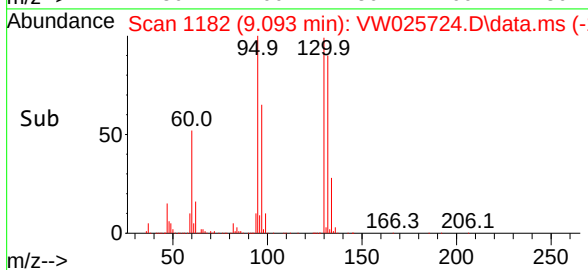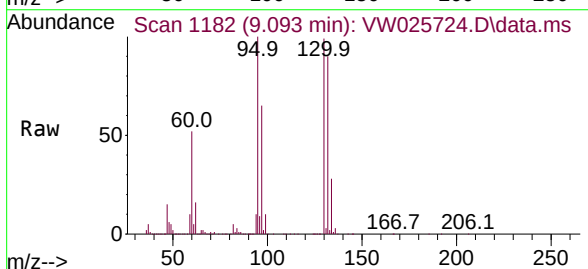



#35
Methylcyclohexane
Concen: 24.390 ug/L
RT: 9.337 min Scan# 1222
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21




Instrument :
MSVOA_W
ClientSampleId :
DCCT3




Tgt Ion: 83 Resp: 438324
Ion Ratio Lower Upper
83 100
55 86.3 68.7 103.1
98 46.8 37.4 56.2

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 04/28/2023
Supervised By :Mahesh Dadoda 05/01/2023

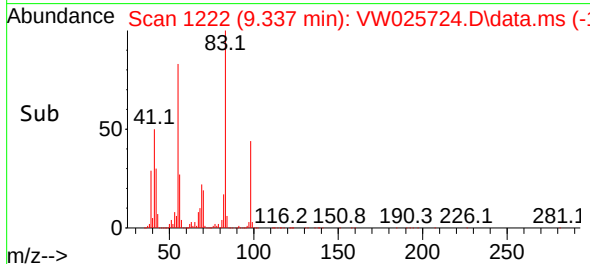


#37
1,2-Dichloropropane
Concen: 12.343 ug/L
RT: 9.367 min Scan# 1227
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21

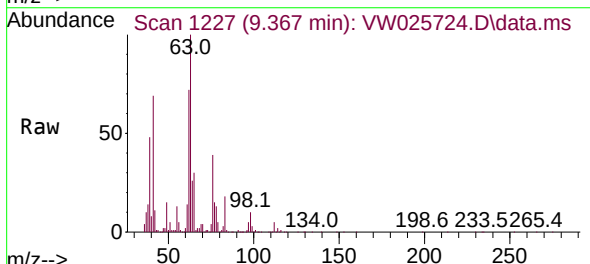


Tgt Ion: 63 Resp: 130245
Ion Ratio Lower Upper
63 100
112 4.6 3.2 4.8

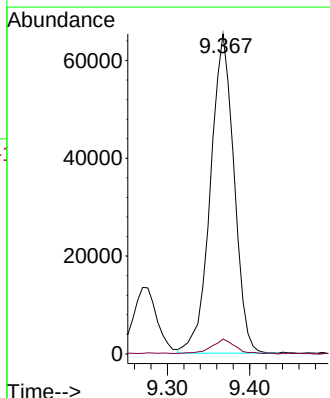



#38
Bromodichloromethane
Concen: 19.996 ug/L
RT: 9.642 min Scan# 1272
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21




Instrument :
MSVOA_W
ClientSampleId :
DCCT3



Tgt Ion: 83 Resp: 238482
Ion Ratio Lower Upper
83 100
85 62.9 44.4 82.4
127 7.0 5.5 8.3




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/28/2023
Supervised By :Mahesh Dadoda 05/01/2023

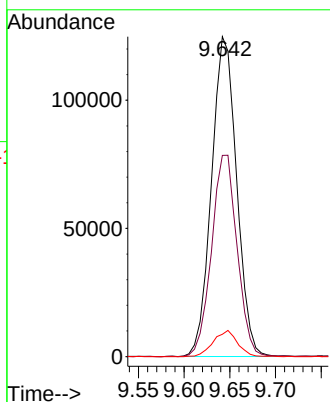

#39
cis-1,3-Dichloropropene
Concen: 15.195 ug/L
RT: 10.069 min Scan# 1342
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21


Tgt Ion: 75 Resp: 229599
Ion Ratio Lower Upper
75 100
77 30.4 22.3 41.5

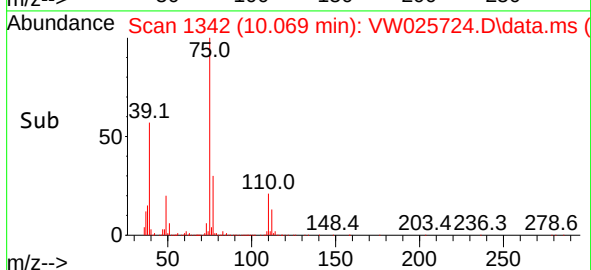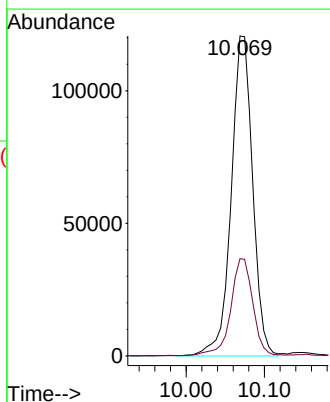



#42
Toluene
Concen: 19.523 ug/L
RT: 10.386 min Scan# 1394
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21




Instrument :
MSVOA_W
ClientSampleId :
DCCT3



Tgt Ion: 91 Resp: 779680
Ion Ratio Lower Upper
91 100
92 58.8 40.8 75.8




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/28/2023
Supervised By :Mahesh Dadoda 05/01/2023



#44
trans-1,3-Dichloropropene
Concen: 7.507 ug/L
RT: 10.605 min Scan# 1430
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21


Tgt Ion: 75 Resp: 93196
Ion Ratio Lower Upper
75 100
77 30.5 22.5 41.7

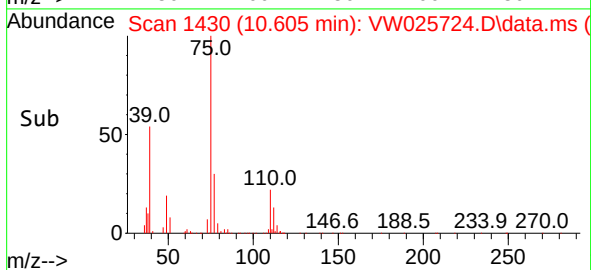



#46
Tetrachloroethene
Concen: 36.920 ug/L
RT: 10.861 min Scan# 1472
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21




Instrument :
MSVOA_W
ClientSampleId :
DCCT3




Tgt Ion:164 Resp: 264368
Ion Ratio Lower Upper
164 100
129 98.8 69.2 128.6
131 97.9 59.4 110.2
166 135.0 88.5 164.4

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 04/28/2023
Supervised By :Mahesh Dadoda 05/01/2023




#48
2-Hexanone
Concen: 47.140 ug/L
RT: 10.965 min Scan# 1489
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21




Tgt Ion: 43 Resp: 211274
Ion Ratio Lower Upper
43 100
58 49.8 40.3 60.5
57 17.3 13.8 20.8
100 10.0 7.8 11.6

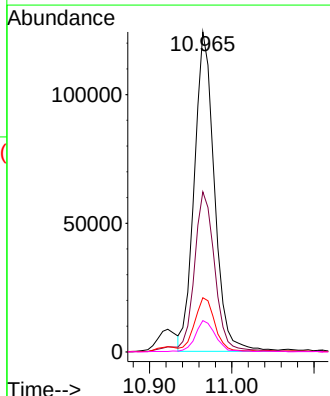



#49
Dibromochloromethane
Concen: 21.182 ug/L
RT: 11.123 min Scan# 1515
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21




Instrument :
MSVOA_W
ClientSampleId :
DCCT3




Tgt Ion:129 Resp: 150000
Ion Ratio Lower Upper
129 100
127 75.8 51.9 96.5

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 04/28/2023
Supervised By :Mahesh Dadoda 05/01/2023




#52
Ethylbenzene
Concen: 14.446 ug/L
RT: 11.727 min Scan# 1614
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21

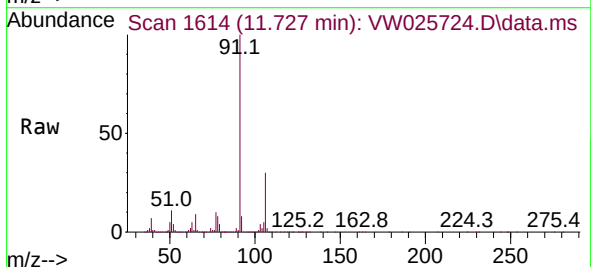


Tgt Ion: 91 Resp: 646952
Ion Ratio Lower Upper
91 100
106 30.5 20.4 37.8

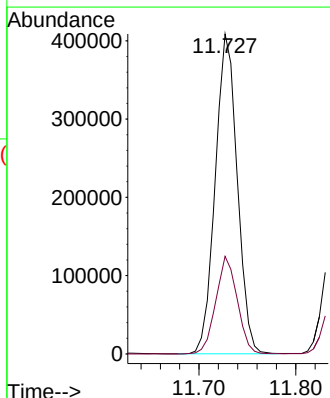



#53
m,p-Xylene
Concen: 9.511 ug/L
RT: 11.843 min Scan# 1633
Delta R.T. 0.006 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21




Instrument :
MSVOA_W
ClientSampleId :
DCCT3



Tgt Ion:106 Resp: 15725
Ion Ratio Lower Upper
106 100
91 211.1 151.1 280.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/28/2023
Supervised By :Mahesh Dadoda 05/01/2023

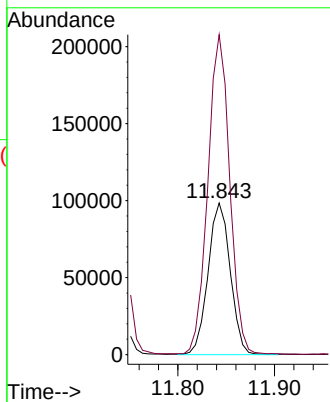

#54
o-Xylene
Concen: 11.461 ug/L
RT: 12.166 min Scan# 1686
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21


Tgt Ion:106 Resp: 176676
Ion Ratio Lower Upper
106 100
91 224.8 150.8 280.1

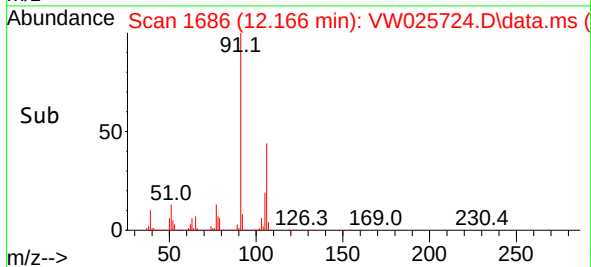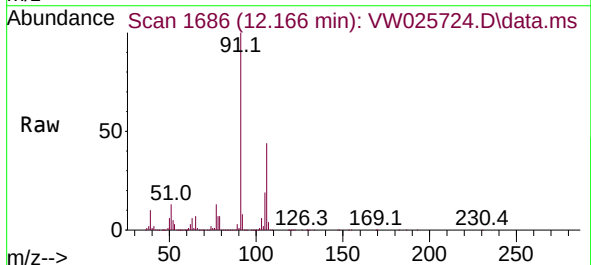



#60
Isopropylbenzene
Concen: 11.738 ug/L
RT: 12.458 min Scan# 1734
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21




Instrument :
MSVOA_W
ClientSampleId :
DCCT3



Tgt Ion:105 Resp: 503512
Ion Ratio Lower Upper
105 100
120 24.2 20.9 31.3
77 16.8 13.8 20.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/28/2023
Supervised By :Mahesh Dadoda 05/01/2023

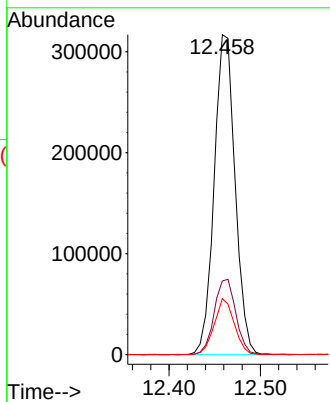

#64
1,3-Dichlorobenzene
Concen: 18.518 ug/L
RT: 13.495 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21

Tgt Ion:146 Resp: 335241
Ion Ratio Lower Upper
146 100
111 42.1 33.0 61.4
148 62.0 48.6 90.3

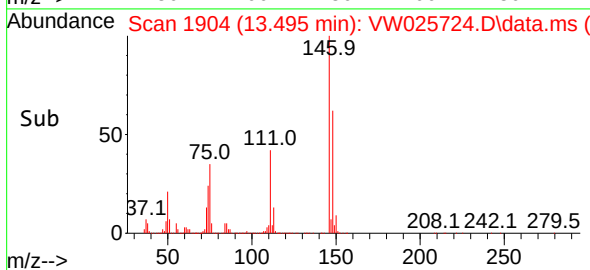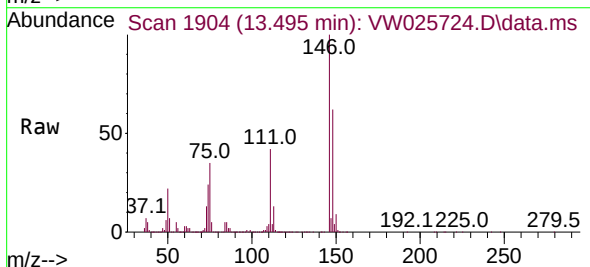







#67
1,2-Dichlorobenzene
Concen: 9.586 ug/L
RT: 13.867 min Scan# 1965
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21

Instrument :
MSVOA_W
ClientSampleId :
DCCT3

Tgt Ion:146 Resp: 153101
Ion Ratio Lower Upper
146 100
111 43.4 36.2 54.2
148 65.6 50.2 75.4

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/28/2023
Supervised By :Mahesh Dadoda 05/01/2023

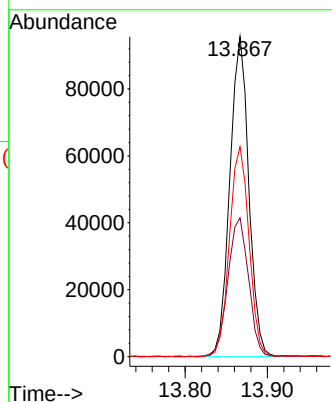

#68
1,2-Dibromo-3-chloropropane
Concen: 21.945 ug/L
RT: 14.476 min Scan# 2065
Delta R.T. -0.000 min
Lab File: VW025724.D
Acq: 27 Apr 2023 14:21

Tgt Ion: 75 Resp: 30519
Ion Ratio Lower Upper
75 100
155 58.5 50.3 75.5
157 73.9 68.4 102.6

