

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW042820\
 Data File : VW015368.D
 Acq On : 28 Apr 2020 18:50
 Operator : SY/VA
 Sample : L2392-02
 Misc : 5.60G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AF8

Quant Time: Apr 29 02:26:52 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042820S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 29 02:04:58 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	431870	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	392451	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	201699	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	82745	26.31	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	105.24%
7) Chloroethane-d5	2.89	69	81332	22.22	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.88%
10) 1,1-Dichloroethene-d2	4.01	63	132832	16.72	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.88%
20) 2-Butanone-d5	7.07	46	39967	41.36	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	82.72%
24) Chloroform-d	7.65	84	193442	20.37	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.48%
26) 1,2-Dichloroethane-d4	8.31	65	104016	21.28	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.12%
29) Benzene-d6	8.27	84	393592	21.77	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.08%
33) 1,2-Dichloropropane-d6	9.27	67	106577	21.07	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.28%
37) Toluene-d8	10.32	98	396847	21.51	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.04%
38) trans-1,3-Dichloropropene-	10.58	79	51685	19.96	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.84%
39) 2-Hexanone-d5	10.92	63	37377	40.47	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.94%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	83886	19.59	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	78.36%
61) 1,2-Dichlorobenzene-d4	13.85	152	143150	20.42	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	81.68%


Target Compounds					Ovalue
13) Acetone	4.12	43	2259	2.775 ug/L	84




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW042820\
Data File : VW015368.D
Acq On : 28 Apr 2020 18:50
Operator : SY/VA
Sample : L2392-02
Misc : 5.60G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AF8

Quant Time: Apr 29 02:26:52 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042820S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 29 02:04:58 2020
Response via : Initial Calibration

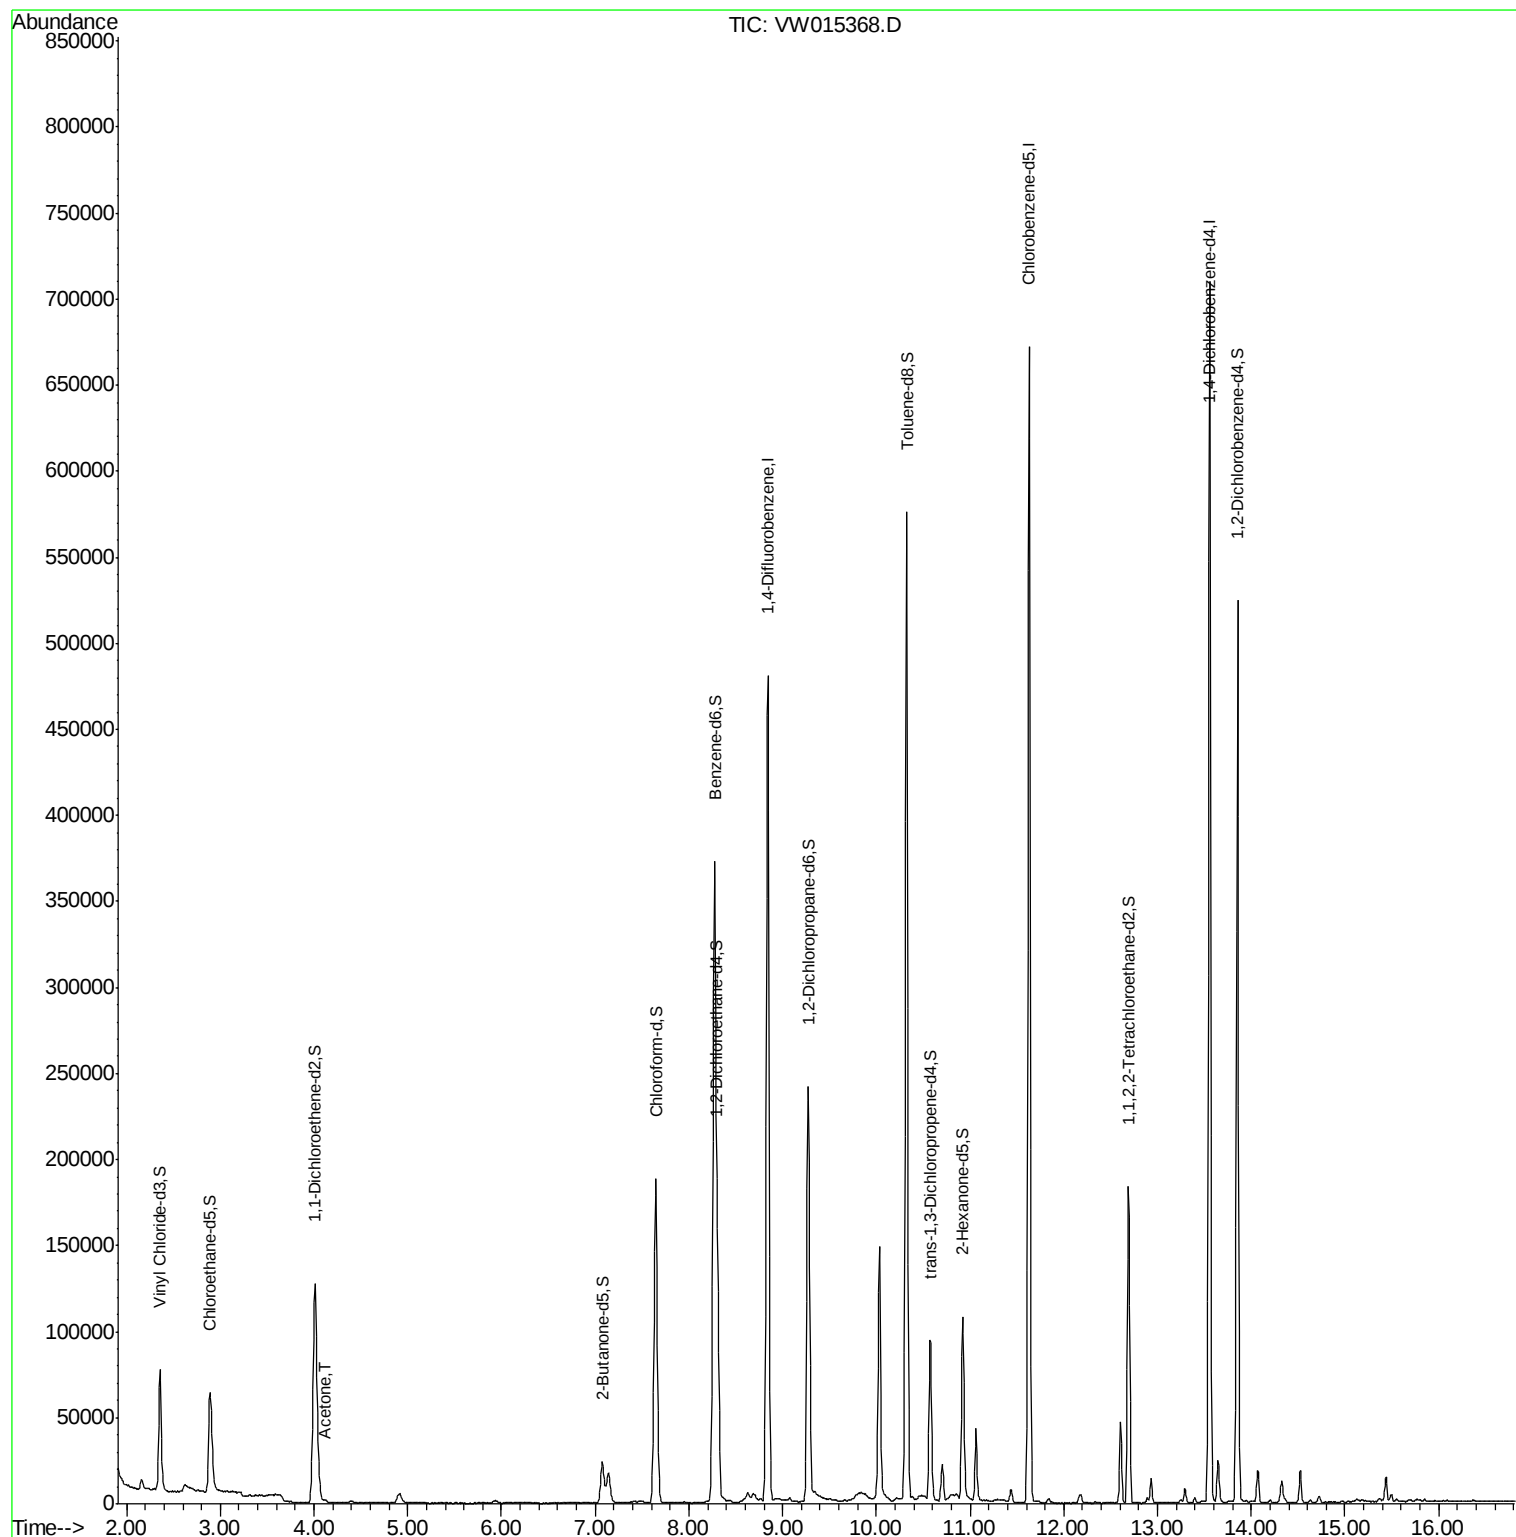

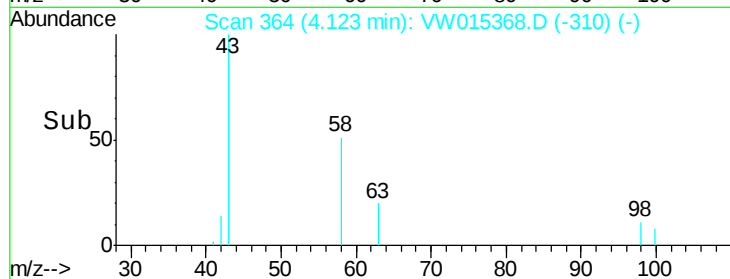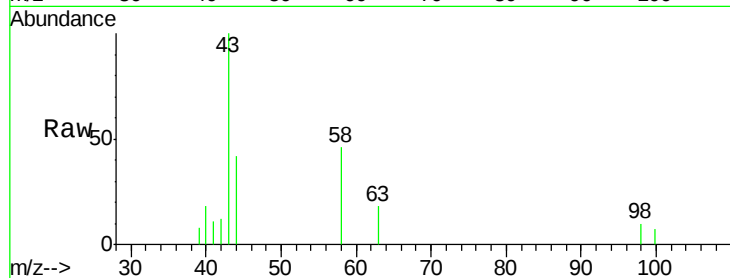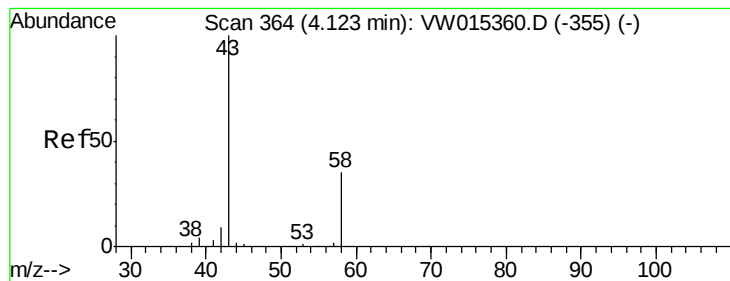

#13

Acetone

Concen: 2.775 ug/L

RT: 4.12 min Scan# 364

Delta R.T. -0.00 min

Lab File: VW015368.D

Acq: 28 Apr 2020 18:50

Instrument :

MSVOA_W

ClientSampleId :

C0AF8

Tot Ion: 43 Resp: 2259

Ion Ratio Lower Upper

43 100

58 25.0 0.0 68.0

