

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
 Data File : VW025757.D
 Acq On : 28 Apr 2023 14:05
 Operator : SY/MD
 Sample : 02526-22
 Misc : 4.15g/10mL/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCL6

Quant Time: Apr 29 00:24:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 28 02:55:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	623489	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	563812	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	280604	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	137257	18.047	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.200%
7) Chloroethane-d5	2.899	69	117026	21.461	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.840%
11) 1,1-Dichloroethene-d2	4.015	63	266765	15.384	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.520%
21) 2-Butanone-d5	7.075	46	141702	56.460	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.920%
24) Chloroform-d	7.648	84	394751	23.601	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.400%
26) 1,2-Dichloroethane-d4	8.300	65	229236	25.140	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.560%
32) Benzene-d6	8.276	84	751336	21.950	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.800%
36) 1,2-Dichloropropane-d6	9.276	67	254644	22.999	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.000%
41) Toluene-d8	10.325	98	663292	21.919	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.680%
43) trans-1,3-Dichloroprop...	10.574	79	97556	22.610	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.440%
47) 2-Hexanone-d5	10.922	63	96741	56.257	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.520%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	214080	26.235	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	104.960%
66) 1,2-Dichlorobenzene-d4	13.848	152	233609	24.300	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.200%
Target Compounds					Qvalue	
13) Acetone	4.118	43	27322	11.745	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
Data File : VW025757.D
Acq On : 28 Apr 2023 14:05
Operator : SY/MD
Sample : 02526-22
Misc : 4.15g/10mL/MSVOA_W/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCL6


Quant Time: Apr 29 00:24:11 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 28 02:55:08 2023
Response via : Initial Calibration

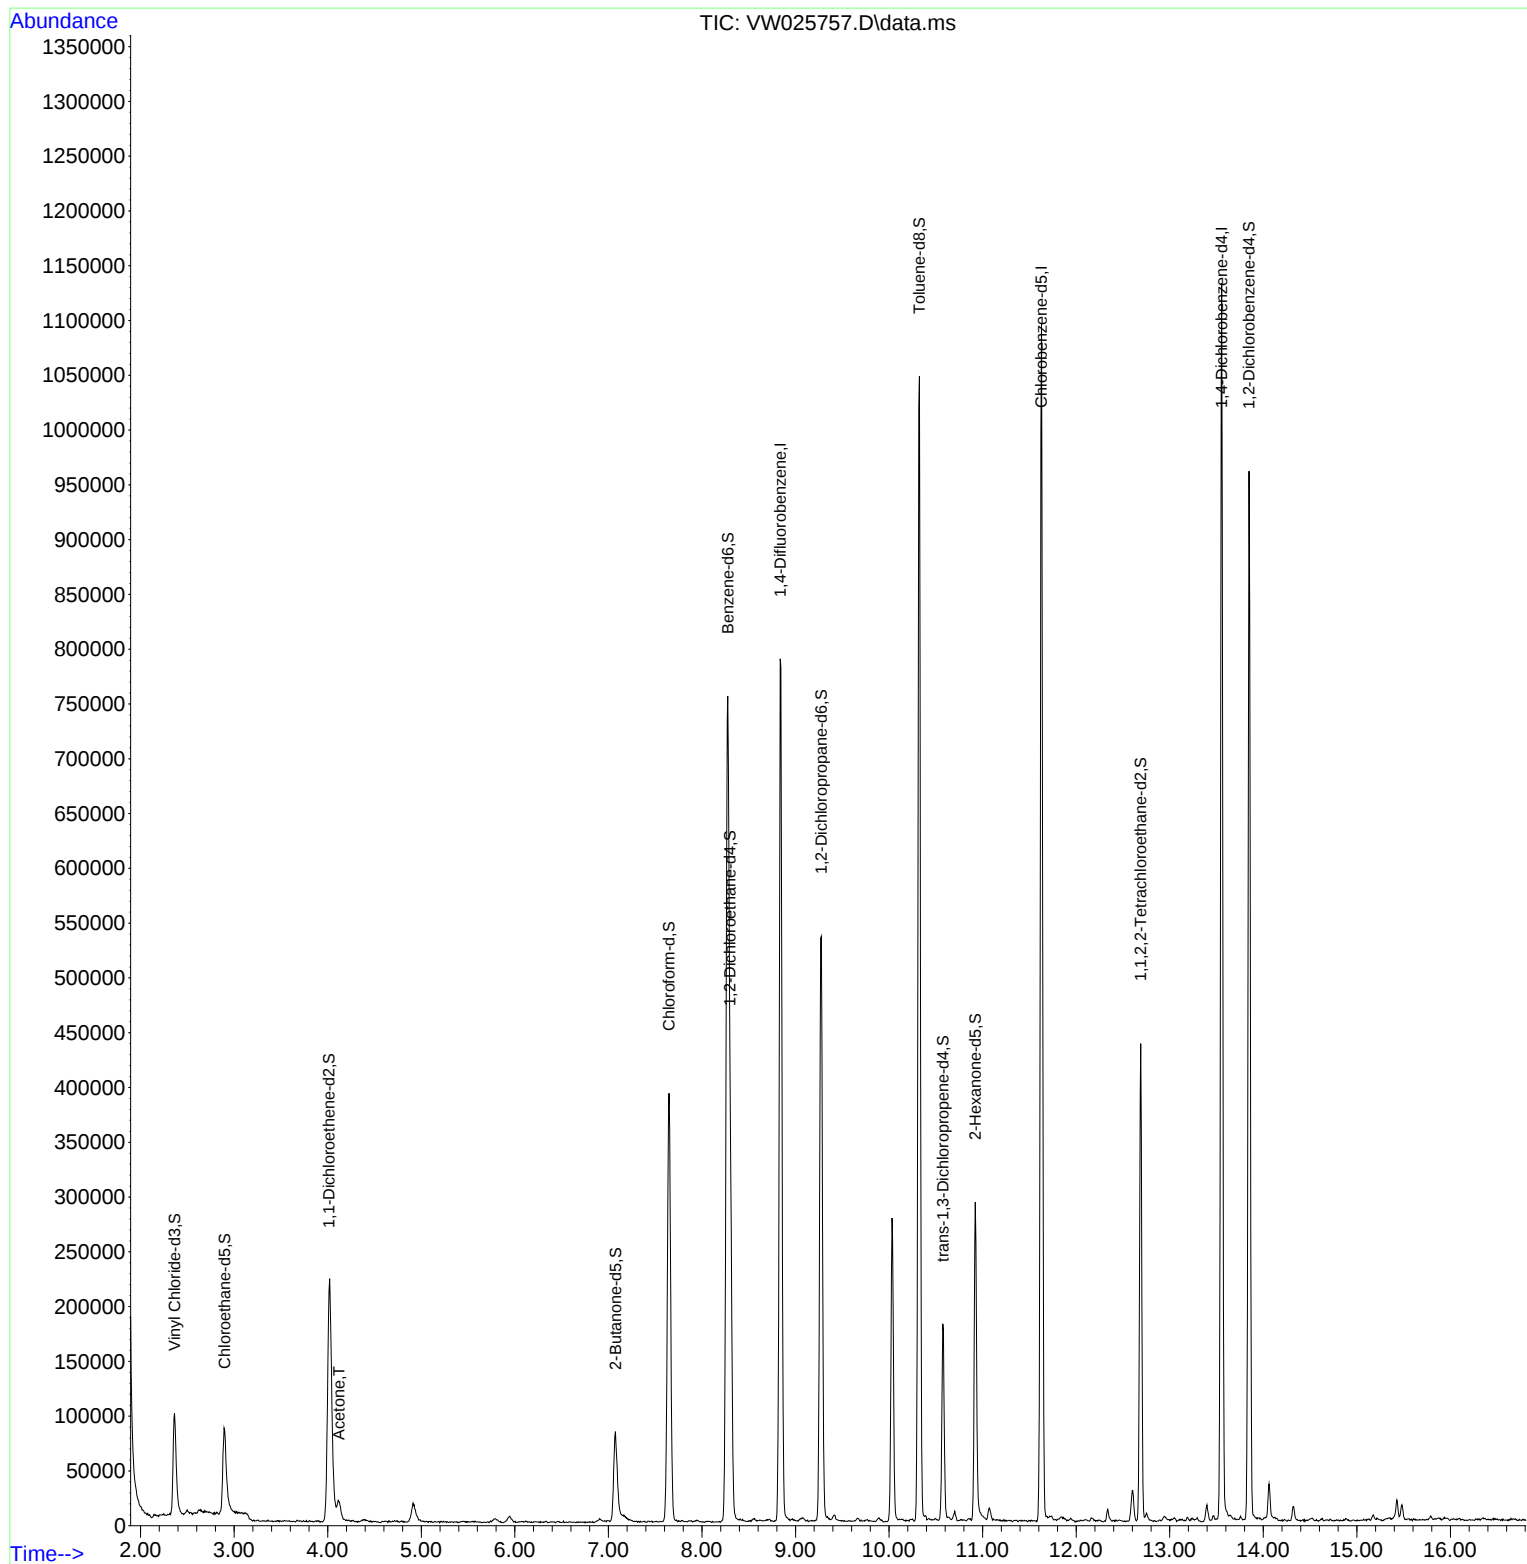

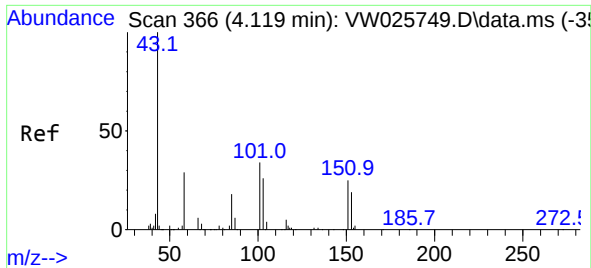

#13
 Acetone
 Concen: 11.745 ug/L
 RT: 4.118 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW025757.D
 Acq: 28 Apr 2023 14:05

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCL6

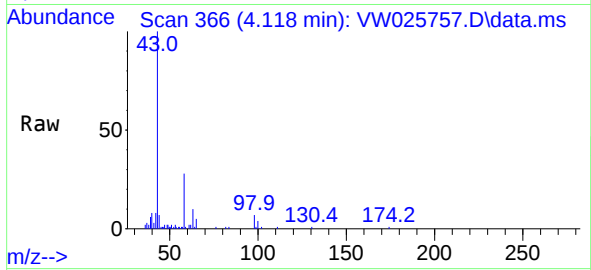

Tgt Ion: 43 Resp: 27322
 Ion Ratio Lower Upper
 43 100
 58 30.9 0.0 58.6

