




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
 Data File : VW025751.D
 Acq On : 28 Apr 2023 10:03
 Operator : SY/MD
 Sample : 02526-05
 Misc : 1.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCS3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/29/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 29 00:23:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 28 02:55:08 2023
 Response via : Initial Calibration

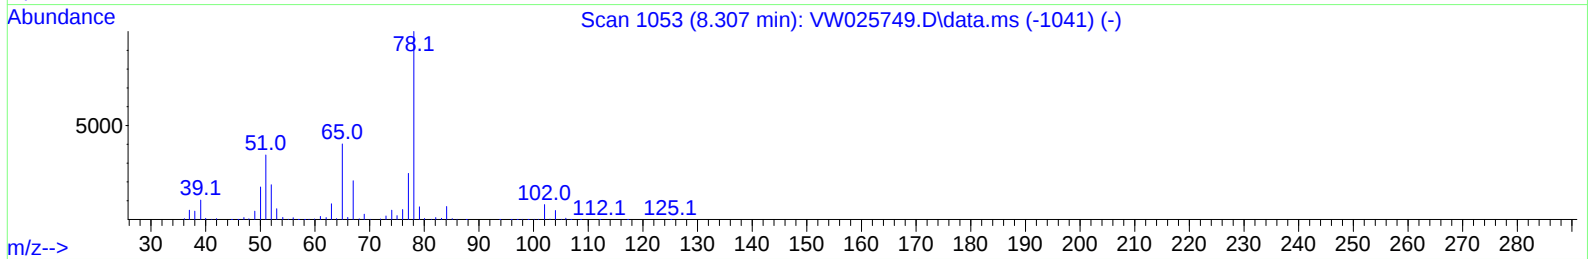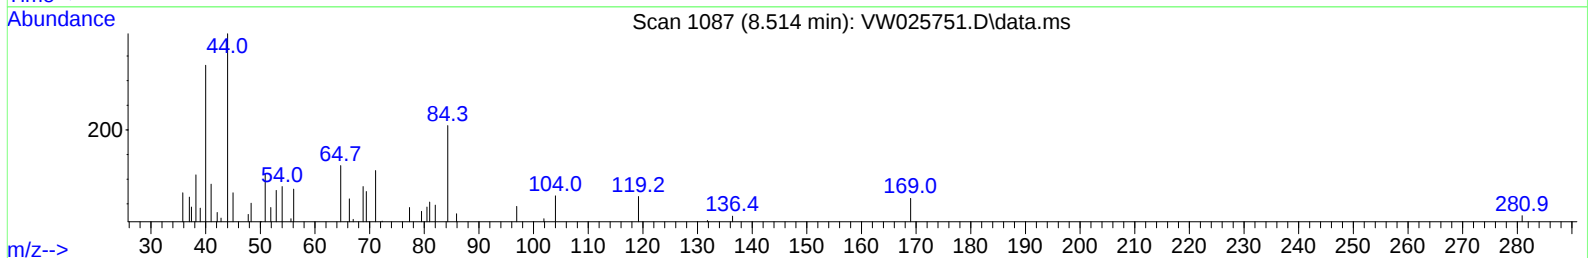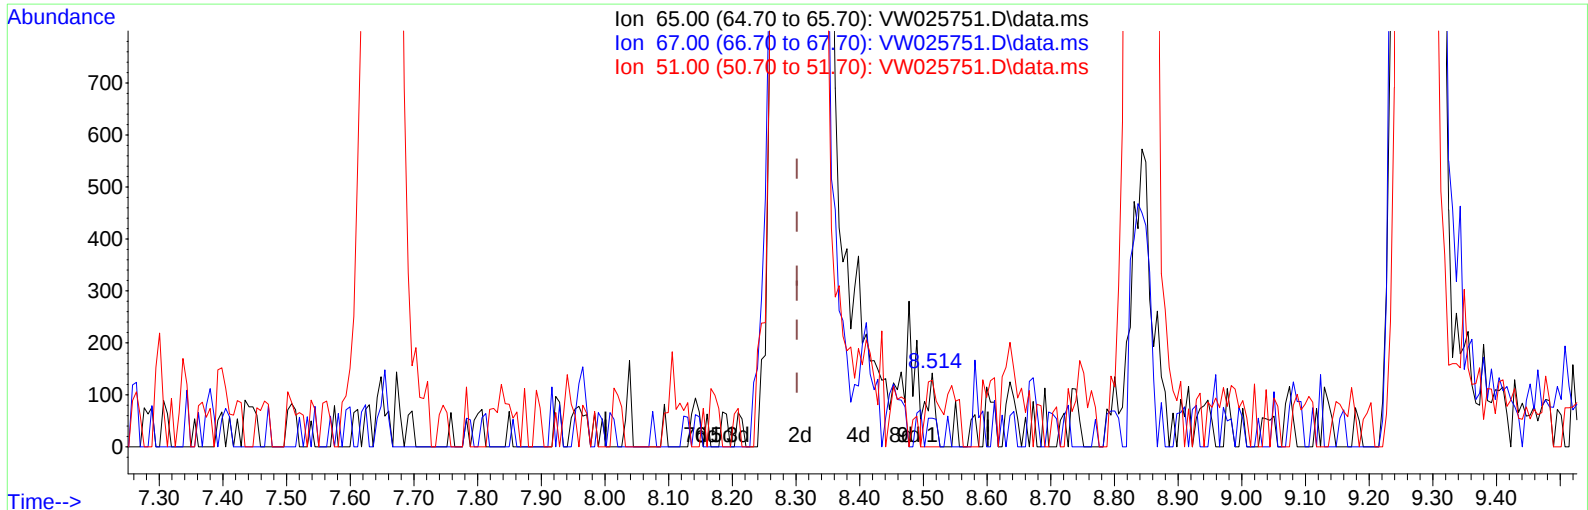

TIC: VW025751.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.514min (+ 0.213) 0.01 ug/L

response 128

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.40	46.88
51.00	121.60	152.34
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
 Data File : VW025751.D
 Acq On : 28 Apr 2023 10:03
 Operator : SY/MD
 Sample : 02526-05
 Misc : 1.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCS3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/29/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 29 00:23:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 28 02:55:08 2023
 Response via : Initial Calibration

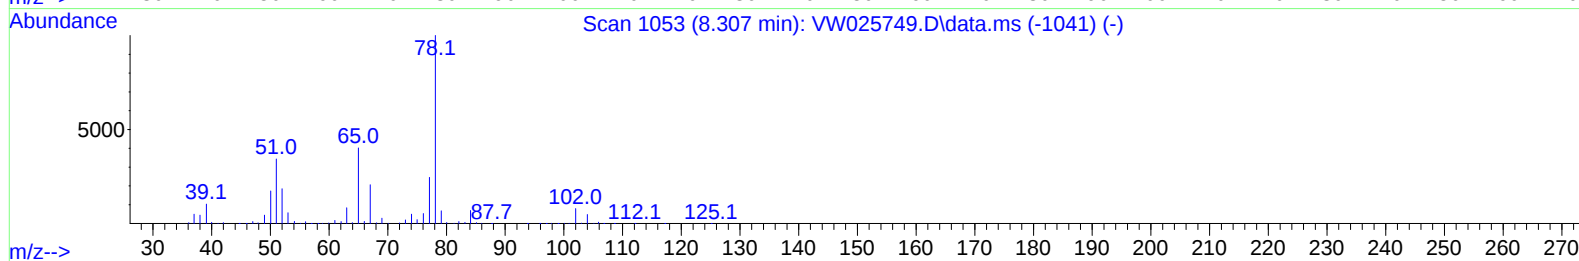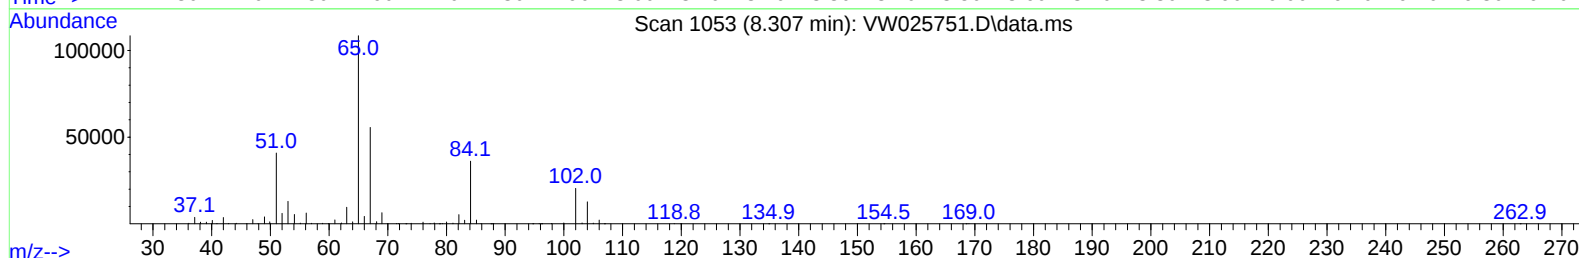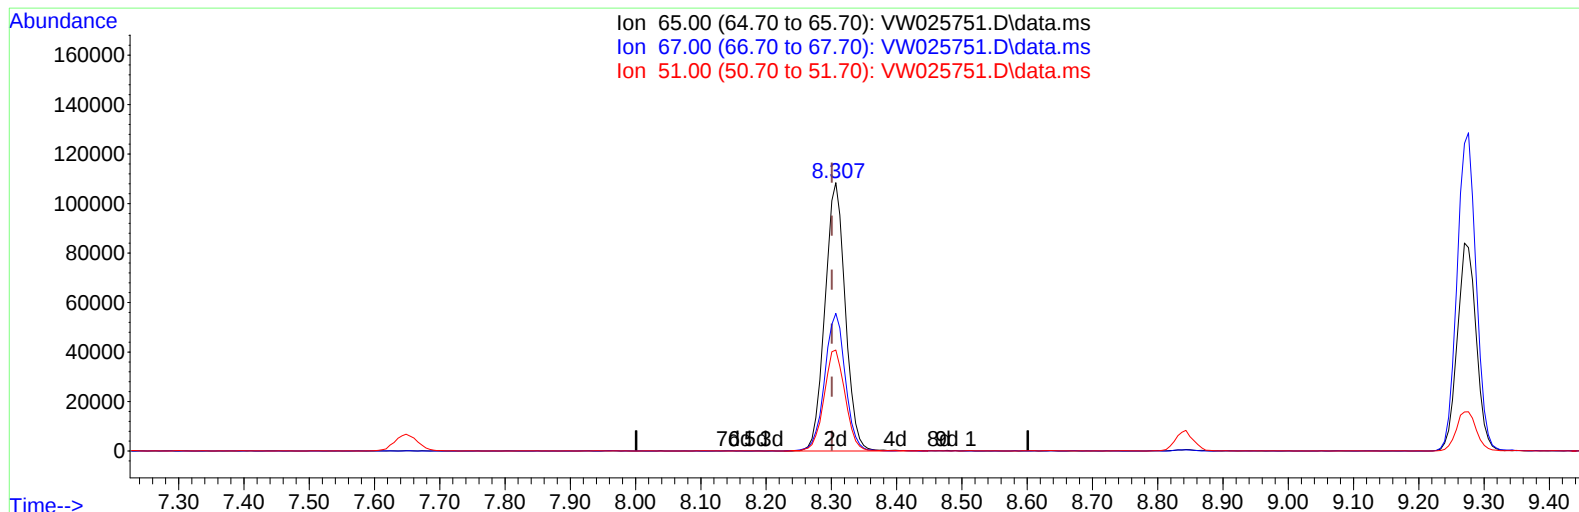

TIC: VW025751.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.006) 23.01 ug/L m

response 234995

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.40	0.03#
51.00	121.60	0.08#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
 Data File : VW025751.D
 Acq On : 28 Apr 2023 10:03
 Operator : SY/MD
 Sample : 02526-05
 Misc : 1.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCS3

Manual IntegrationsAPPROVED

Quant Time: Apr 29 00:23:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 28 02:55:08 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/29/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	698437	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	617364	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	289004	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	163480	19.188	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	76.760%	
7) Chloroethane-d5	2.899	69	128220	20.991	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	83.960%	
11) 1,1-Dichloroethene-d2	4.021	63	298033	15.343	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	61.360%	
21) 2-Butanone-d5	7.075	46	114892	40.866	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	81.740%	
24) Chloroform-d	7.648	84	406429	21.692	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	86.760%	
26) 1,2-Dichloroethane-d4	8.307	65	234995m	23.006	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	92.040%	
32) Benzene-d6	8.270	84	825761	22.031	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	88.120%	
36) 1,2-Dichloropropane-d6	9.276	67	260509	21.488	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	85.960%	
41) Toluene-d8	10.325	98	739510	22.318	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	89.280%	
43) trans-1,3-Dichloroprop...	10.575	79	102687	21.735	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	86.960%	
47) 2-Hexanone-d5	10.922	63	81782	43.433	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	86.860%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	192509	21.545	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	86.200%	
66) 1,2-Dichlorobenzene-d4	13.848	152	230469	23.276	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	93.120%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
Data File : VW025751.D
Acq On : 28 Apr 2023 10:03
Operator : SY/MD
Sample : 02526-05
Misc : 1.99g/10mL/MSVOA_W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCS3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/29/2023
Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 29 00:23:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 28 02:55:08 2023
Response via : Initial Calibration

