

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
 Data File : VW025752.D
 Acq On : 28 Apr 2023 10:27
 Operator : SY/MD
 Sample : 02526-02
 Misc : 4.24g/10mL/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCM7

Manual IntegrationsAPPROVED

Quant Time: Apr 29 00:23:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 28 02:55:08 2023
 Response via : Initial Calibration




Reviewed By :Semsettin
 Yesilyurt

04/29/2023

Supervised By :Mahesh

Dadoda

05/01/2023

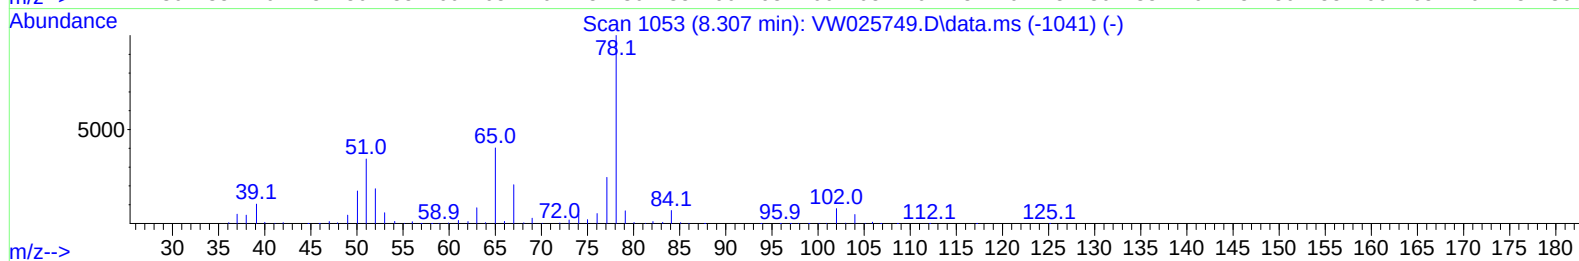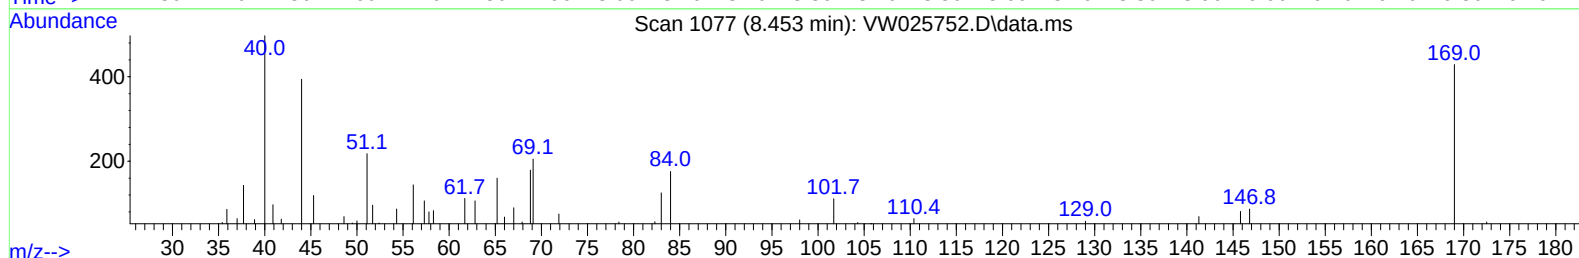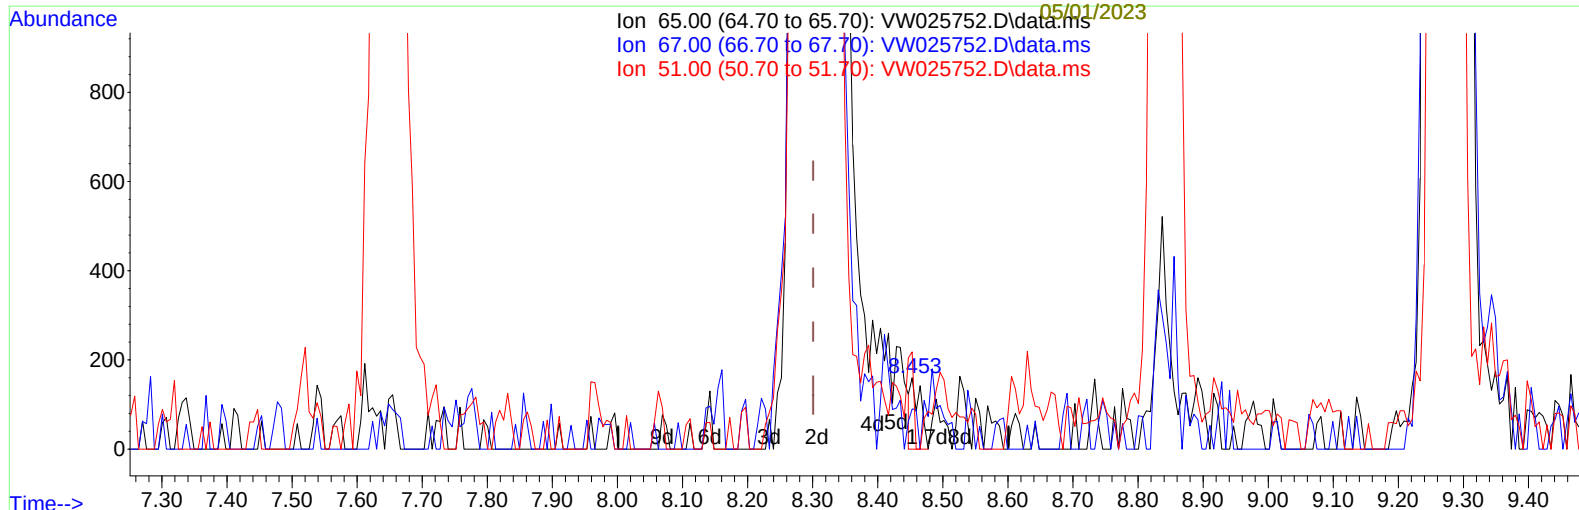

TIC: VW025752.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.453min (+ 0.152) 0.02 ug/L

response 163

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.40	53.99
51.00	121.60	94.48
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
Data File : VW025752.D
Acq On : 28 Apr 2023 10:27
Operator : SY/MD
Sample : 02526-02
Misc : 4.24g/10mL/MSVOA_W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCM7

Manual IntegrationsAPPROVED




Reviewed By :Semsettin
Yesilyurt

04/29/2023

Supervised By :Mahesh
Dadoda

05/01/2023

Quant Time: Apr 29 00:23:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 28 02:55:08 2023
Response via : Initial Calibration

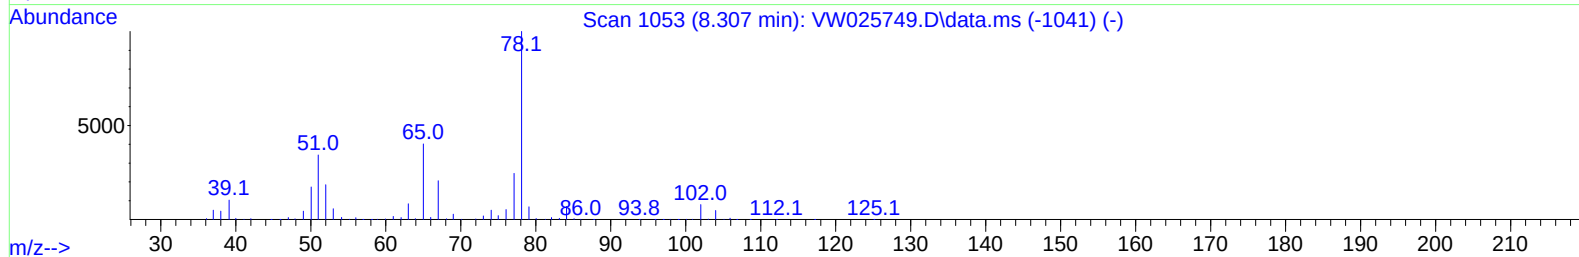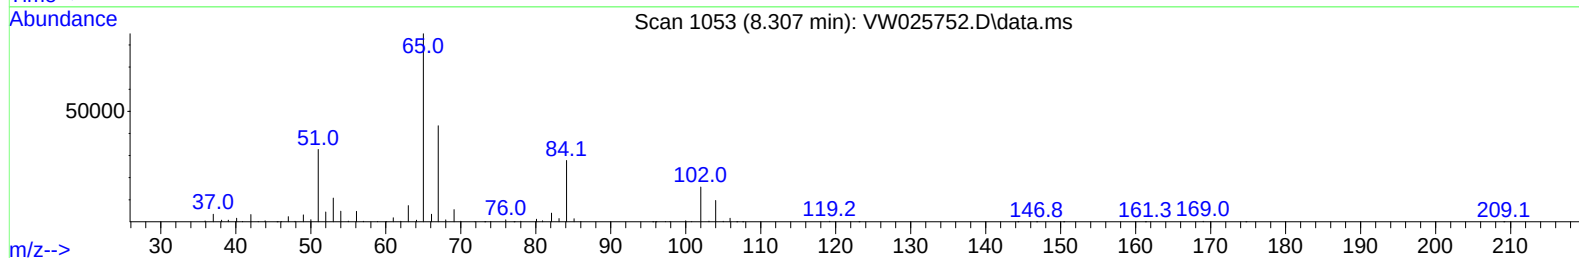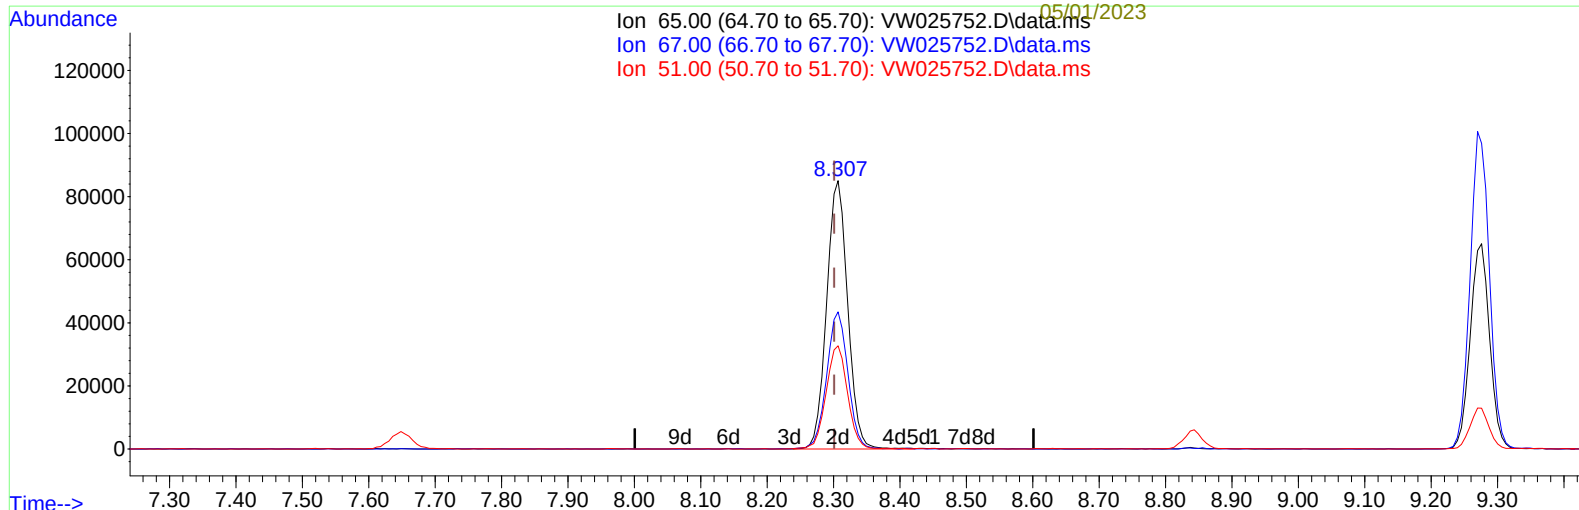

TIC: VW025752.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.006) 25.96 ug/L m

response 187273

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.40	0.05#
51.00	121.60	0.08#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
 Data File : VW025752.D
 Acq On : 28 Apr 2023 10:27
 Operator : SY/MD
 Sample : 02526-02
 Misc : 4.24g/10mL/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCM7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt
 04/29/2023
 Supervised By :Mahesh
 Dadoda
 05/01/2023

Quant Time: Apr 29 00:23:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 28 02:55:08 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		493227	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		452015	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		212124	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		127004	21.109	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.440%	
7) Chloroethane-d5	2.899	69		97471	22.596	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.400%	
11) 1,1-Dichloroethene-d2	4.021	63		227053	16.552	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.200%	
21) 2-Butanone-d5	7.075	46		109540	55.172	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.340%	
24) Chloroform-d	7.648	84		309512	23.392	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.560%	
26) 1,2-Dichloroethane-d4	8.307	65		187273m	25.962	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.840%	
32) Benzene-d6	8.276	84		621819	22.659	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.640%	
36) 1,2-Dichloropropane-d6	9.270	67		203213	22.893	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.560%	
41) Toluene-d8	10.325	98		551714	22.742	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.960%	
43) trans-1,3-Dichloroprop...	10.575	79		83893	24.253	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.000%	
47) 2-Hexanone-d5	10.922	63		76843	55.738	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.480%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		166044	25.381	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.520%	
66) 1,2-Dichlorobenzene-d4	13.848	152		184748	25.421	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.680%	
Target Compounds						Qvalue	
13) Acetone	4.118	43		60382	32.811	ug/L	98
16) Methylene chloride	4.923	84		17670	1.896	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
Data File : VW025752.D
Acq On : 28 Apr 2023 10:27
Operator : SY/MD
Sample : 02526-02
Misc : 4.24g/10mL/MSVOA_W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCM7

Manual IntegrationsAPPROVED

Quant Time: Apr 29 00:23:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 28 02:55:08 2023
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt
04/29/2023
Supervised By :Mahesh
Dadoda
05/01/2023

