




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
 Data File : VW025760.D
 Acq On : 28 Apr 2023 15:17
 Operator : SY/MD
 Sample : 02526-15
 Misc : 5.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCF9

Manual IntegrationsAPPROVED

Quant Time: Apr 29 00:24:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 28 02:55:08 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/29/2023
 Supervised By :Mahesh Dadoda 05/01/2023

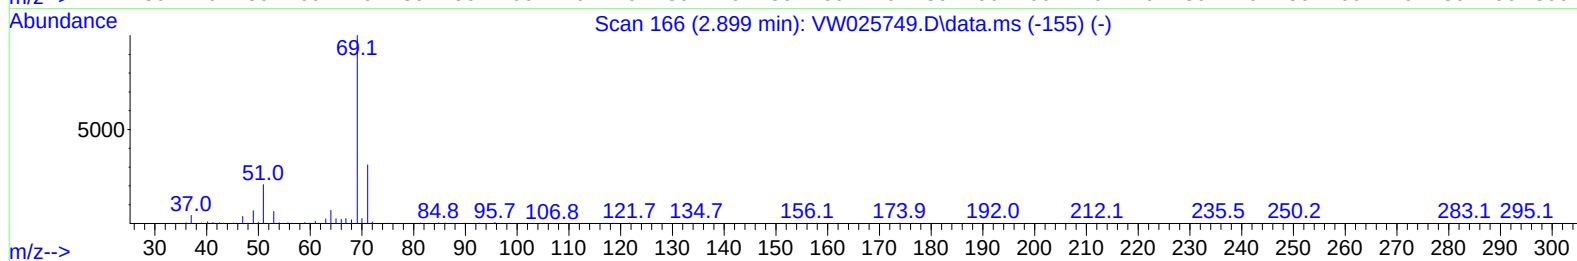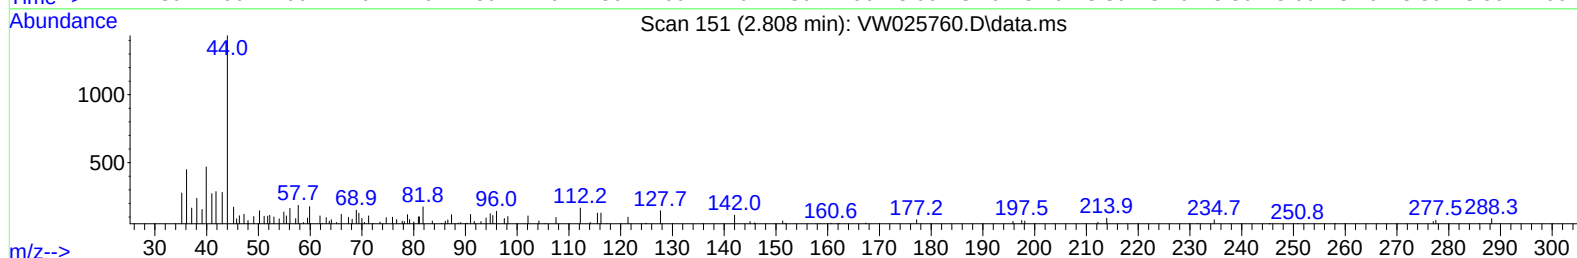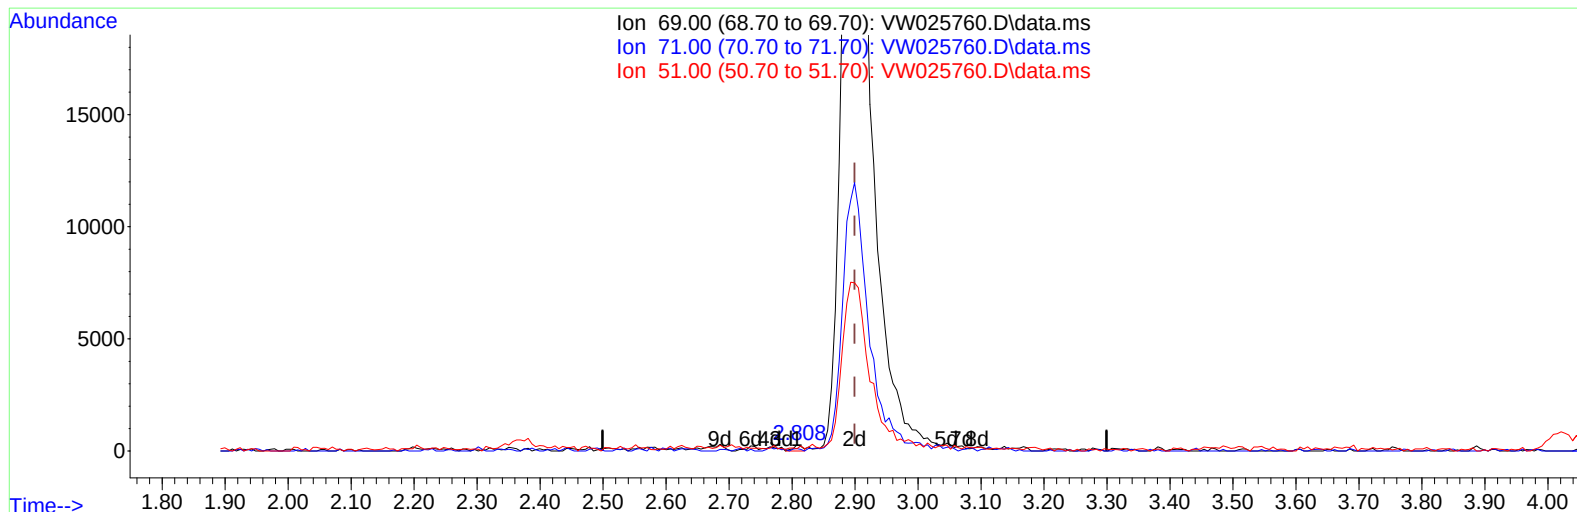

TIC: VW025760.D\data.ms

(7) Chloroethane-d5 (S)

2.808min (-0.091) 0.05 ug/L

response 271

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	36.53
51.00	13.40	16.61
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
 Data File : VW025760.D
 Acq On : 28 Apr 2023 15:17
 Operator : SY/MD
 Sample : 02526-15
 Misc : 5.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCF9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/29/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 29 00:24:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 28 02:55:08 2023
 Response via : Initial Calibration

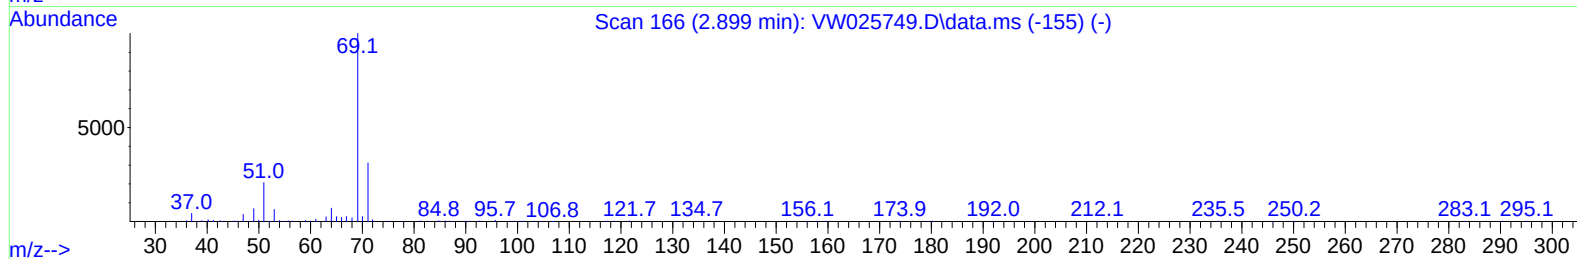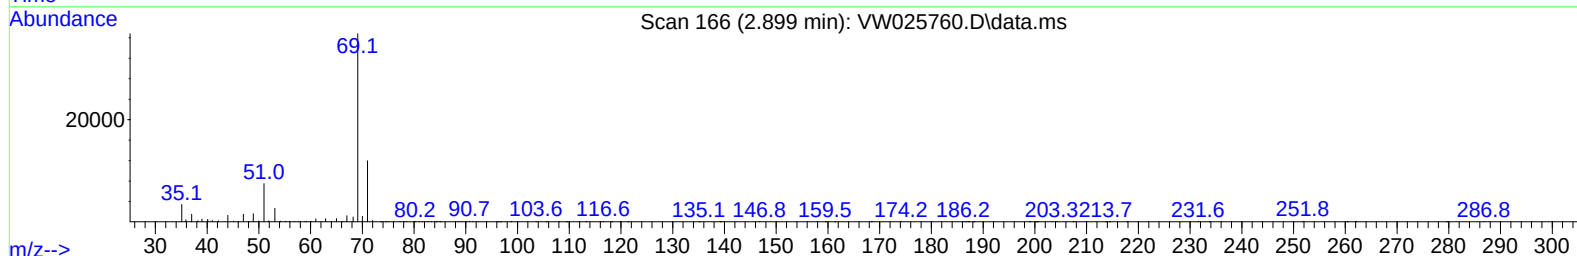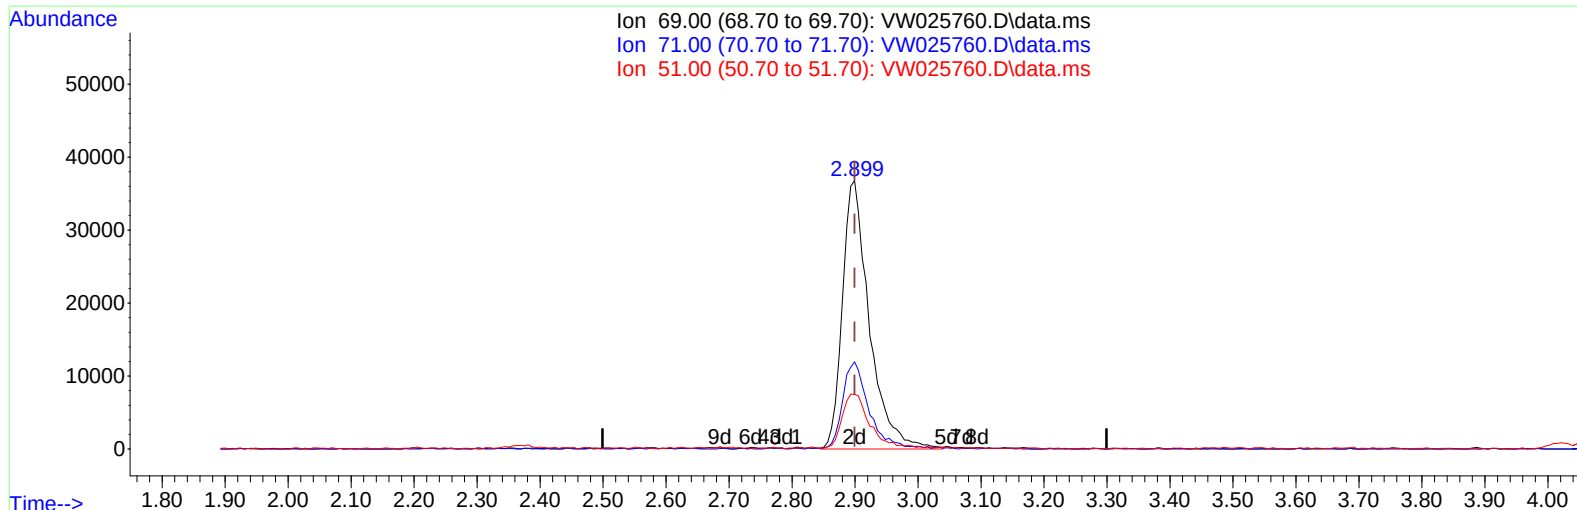

TIC: VW025760.D\data.ms

(7) Chloroethane-d5 (S)

2.899min (+ 0.000) 20.73 ug/L m

response 109251

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	0.09#
51.00	13.40	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
 Data File : VW025760.D
 Acq On : 28 Apr 2023 15:17
 Operator : SY/MD
 Sample : 02526-15
 Misc : 5.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCF9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/29/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 29 00:24:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 28 02:55:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	602611	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	551552	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	265983	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	130268	17.721	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	70.880%		
7) Chloroethane-d5	2.899	69	109251m	20.729	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	82.920%		
11) 1,1-Dichloroethene-d2	4.027	63	244951	14.616	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	58.480%		
21) 2-Butanone-d5	7.075	46	159752	65.857	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	131.720%		
24) Chloroform-d	7.648	84	366817	22.691	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	90.760%		
26) 1,2-Dichloroethane-d4	8.307	65	227076	25.766	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	103.080%		
32) Benzene-d6	8.276	84	696436	20.798	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	83.200%		
36) 1,2-Dichloropropane-d6	9.270	67	239996	22.158	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	88.640%		
41) Toluene-d8	10.319	98	596145	20.138	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	80.560%		
43) trans-1,3-Dichloroprop...	10.575	79	94570	22.405	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	89.640%		
47) 2-Hexanone-d5	10.922	63	107658	63.997	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	128.000%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	221625	27.764	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	111.040%		
66) 1,2-Dichlorobenzene-d4	13.848	152	221492	24.306	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	97.240%		
Target Compounds					Qvalue	
13) Acetone	4.118	43	54664	24.312	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
Data File : VW025760.D
Acq On : 28 Apr 2023 15:17
Operator : SY/MD
Sample : 02526-15
Misc : 5.99g/10mL/MSVOA_W/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCF9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/29/2023
Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 29 00:24:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 28 02:55:08 2023
Response via : Initial Calibration

