




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
Data File : VW025764.D
Acq On : 28 Apr 2023 16:52
Operator : SY/MD
Sample : 02526-10
Misc : 5.59g/10mL/MSVOA_W/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCF4

Manual IntegrationsAPPROVED

Quant Time: Apr 29 00:25:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 28 02:55:08 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/29/2023
Supervised By :Mahesh Dadoda 05/01/2023

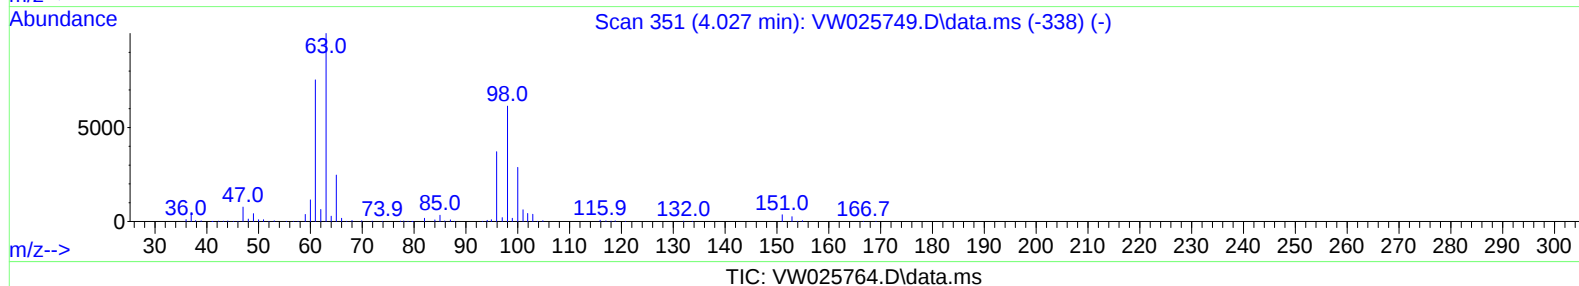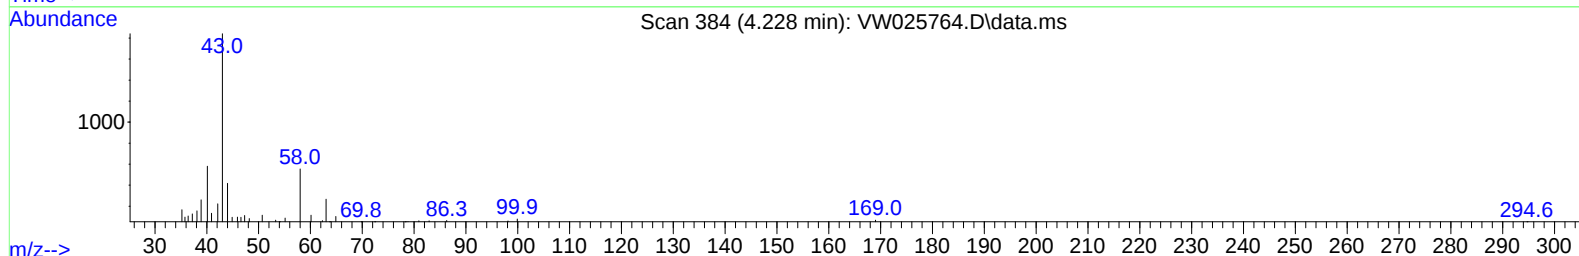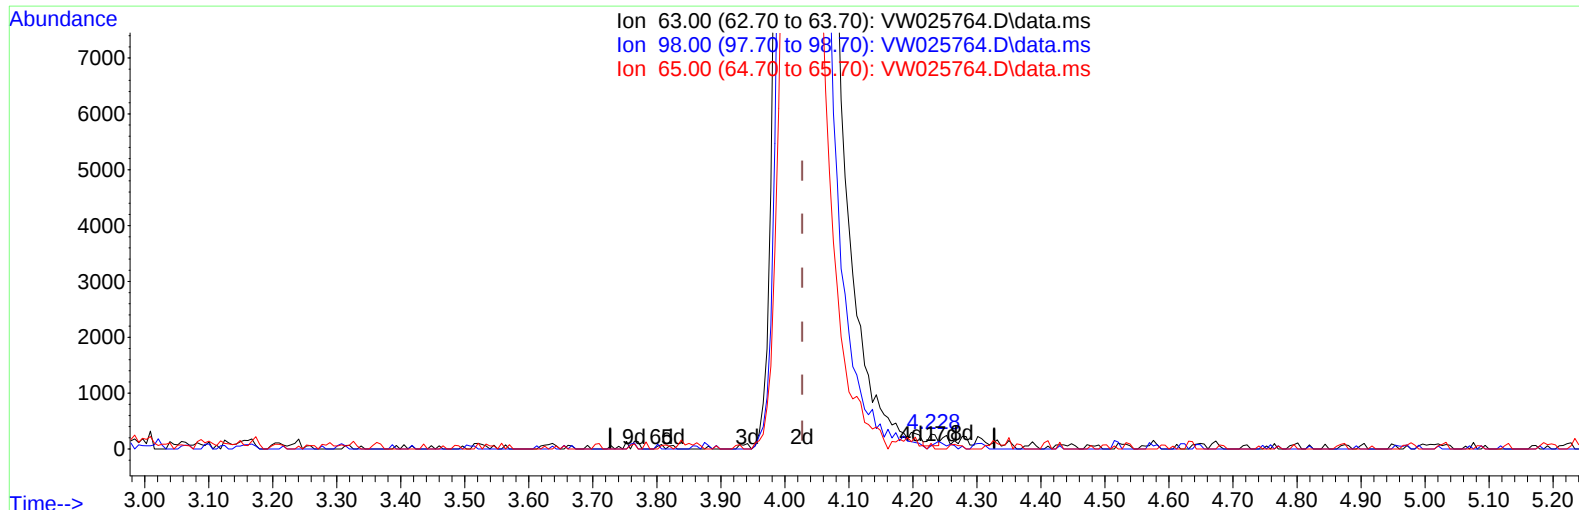

TIC: VW025764.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.228min (+ 0.201) 0.01 ug/L

response 200

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.90	81.50
65.00	22.30	18.50
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
Data File : VW025764.D
Acq On : 28 Apr 2023 16:52
Operator : SY/MD
Sample : 02526-10
Misc : 5.59g/10mL/MSVOA_W/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCF4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/29/2023
Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 29 00:25:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 28 02:55:08 2023
Response via : Initial Calibration

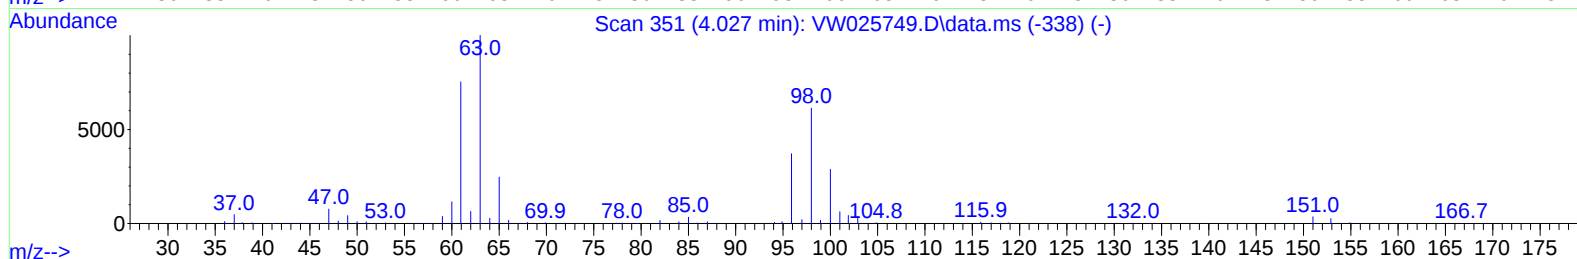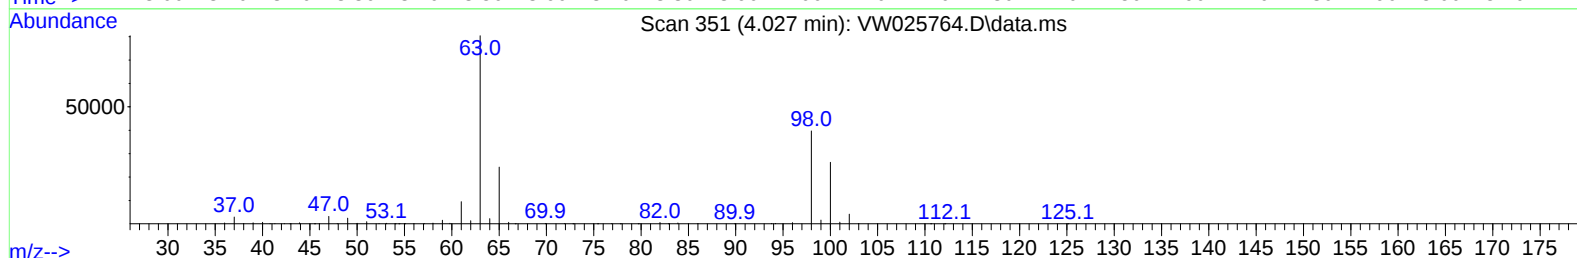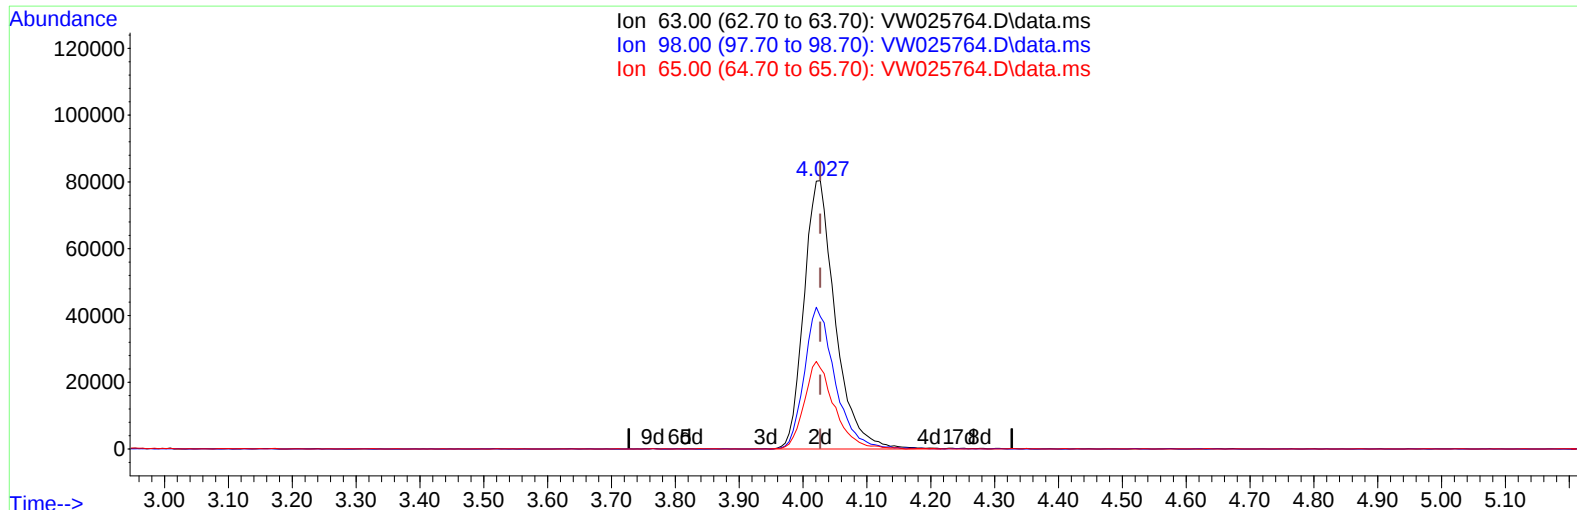

TIC: VW025764.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.027min (-0.000) 15.93 ug/L m

response 274241

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.90	0.06#
65.00	22.30	0.01#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
 Data File : VW025764.D
 Acq On : 28 Apr 2023 16:52
 Operator : SY/MD
 Sample : 02526-10
 Misc : 5.59g/10mL/MSVOA_W/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCF4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/29/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 29 00:25:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 28 02:55:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	619188	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	559592	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	259442	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	140420	18.591	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	74.360%		
7) Chloroethane-d5	2.899	69	121591	22.453	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	89.800%		
11) 1,1-Dichloroethene-d2	4.027	63	274241m	15.925	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	63.720%		
21) 2-Butanone-d5	7.075	46	154700	62.067	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	124.140%		
24) Chloroform-d	7.648	84	398122	23.968	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	95.880%		
26) 1,2-Dichloroethane-d4	8.307	65	235113	25.964	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	103.840%		
32) Benzene-d6	8.276	84	760967	22.399	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	89.600%		
36) 1,2-Dichloropropane-d6	9.276	67	256103	23.305	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	93.240%		
41) Toluene-d8	10.325	98	660010	21.975	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	87.920%		
43) trans-1,3-Dichloroprop...	10.575	79	97890	22.859	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	91.440%		
47) 2-Hexanone-d5	10.922	63	105714	61.938	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	123.880%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	224116	27.672	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	110.680%		
66) 1,2-Dichlorobenzene-d4	13.848	152	224911	25.303	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	101.200%		
Target Compounds					Qvalue	
13) Acetone	4.112	43	494501	214.042	ug/L	99
22) 2-Butanone	7.173	43	36182	12.352	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
Data File : VW025764.D
Acq On : 28 Apr 2023 16:52
Operator : SY/MD
Sample : 02526-10
Misc : 5.59g/10mL/MSVOA_W/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCF4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/29/2023
Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 29 00:25:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 28 02:55:08 2023
Response via : Initial Calibration

